

Data Path : Z:\HPCHEM1\BNA M\DATA\BM111715\
 Data File : BM003152.D
 Acq On : 16 Nov 2015 20:50
 Operator : UM/IZ
 Sample : G4323-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Nov 17 00:21:32 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM103015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 17 00:18:48 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	141547	20.00	ng/ul	0.00
18) Naphthalene-d8	10.54	136	609369	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.39	164	340672	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.13	188	758458	20.00	ng/ul	0.00
78) Chrysene-d12	21.33	240	847294	20.00	ng/ul	0.00
86) Perylene-d12	23.59	264	856170	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.20	96	11625	3.87	ng/uL	0.00
5) Phenol-d5	6.90	99	232024	20.74	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.07	67	130060	19.88	ng/ul	0.00
9) 2-Chlorophenol-d4	7.27	132	198257	20.91	ng/ul	0.00
13) 4-Methylphenol-d8	8.45	113	187859	20.82	ng/ul	0.00
19) Nitrobenzene-d5	8.90	128	89908	24.19	ng/ul	0.00
22) 2-Nitrophenol-d4	9.62	143	95894	25.47	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.15	165	181353	21.48	ng/ul	0.00
29) 4-Chloroaniline-d4	10.67	131	216517	19.82	ng/ul	0.00
44) Dimethylphthalate-d6	13.80	166	570375	22.25	ng/ul	0.00
47) Acenaphthylene-d8	14.08	160	688457	21.20	ng/ul	0.00
52) 4-Nitrophenol-d4	14.58	143	104195	24.12	ng/ul	0.00
58) Fluorene-d10	15.39	176	504242	22.76	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.50	200	74501	21.21	ng/ul	0.00
71) Anthracene-d10	17.23	188	717663	21.34	ng/ul	0.00
79) Pyrene-d10	19.53	212	857189	20.55	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.44	264	886155	21.78	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
6) Phenol	6.93	94	13610	1.18	ng/ul#	91
45) Dimethylphthalate	13.84	163	313142	11.99	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM111715\
Data File : BM003152.D
Acq On : 16 Nov 2015 20:50
Operator : UM/IZ
Sample : G4323-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Nov 17 00:21:32 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM103015.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 17 00:18:48 2015
Response via : Initial Calibration

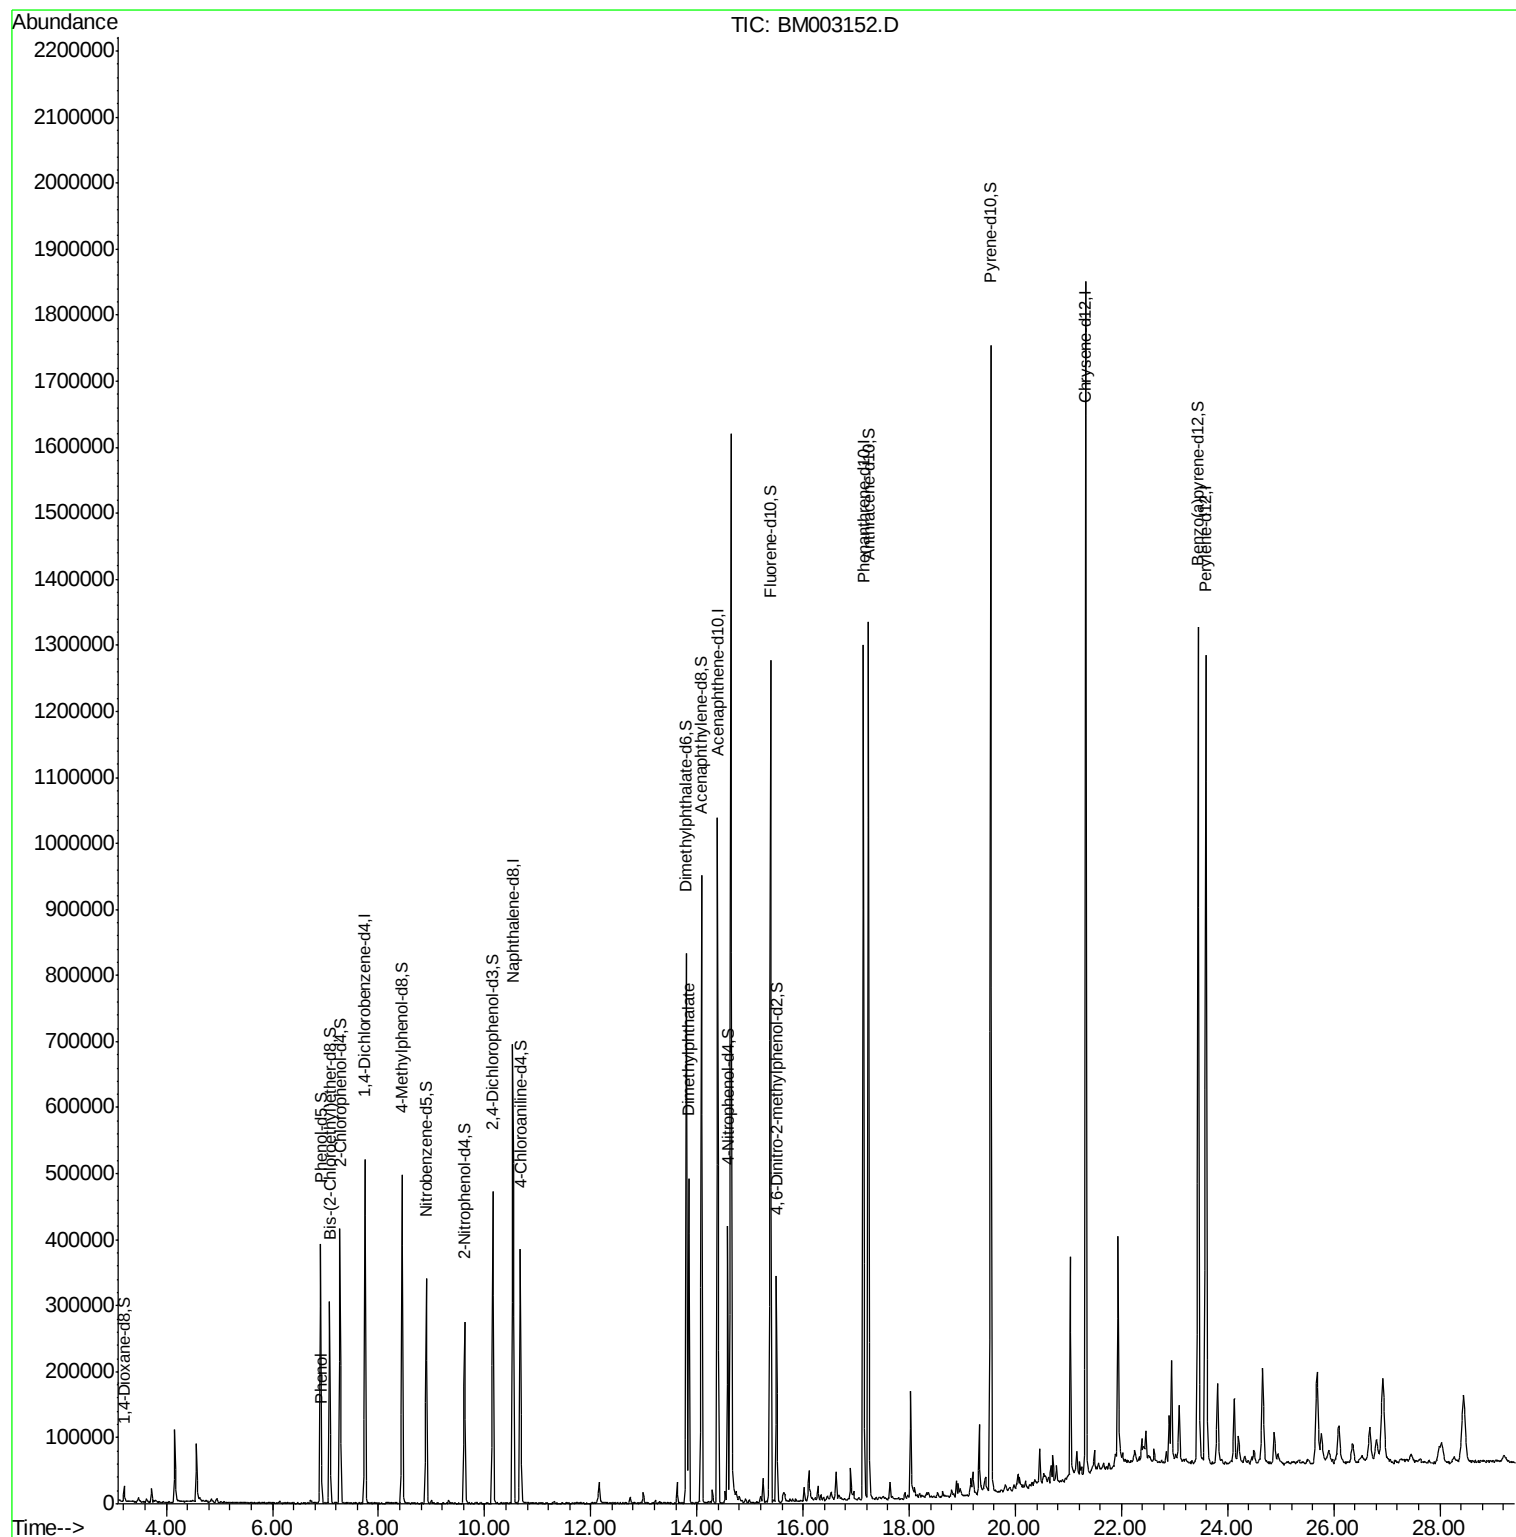

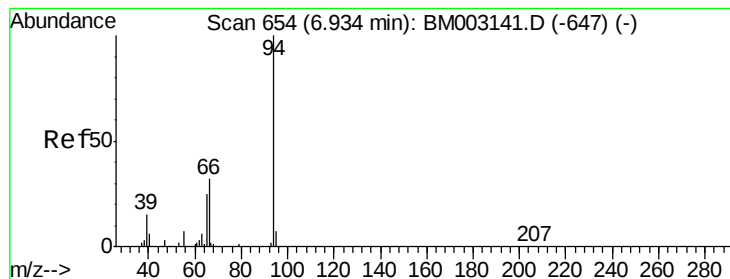

#6

Phenol

Concen: 1.18 ng/ul

RT: 6.93 min Scan# 654

Delta R.T. -0.00 min

Lab File: BM003152.D

Acq: 16 Nov 2015 20:50

Instrument :

BNA_M

ClientSampleId :


Tot Ion: 94 Resp: 13610

Ion Ratio Lower Upper

94 100

65 26.5 18.7 28.1




66 36.5 24.2 36.2#

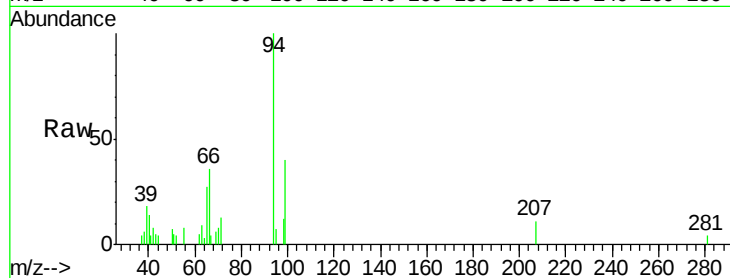

Abundance Ion 94.00 (93.70 to 94.70): BM003141.D (-647) (-)

Ion 65.00 (64.70 to 65.70): BM003141.D (-647) (-)

Ion 66.00 (65.70 to 66.70): BM003141.D (-647) (-)

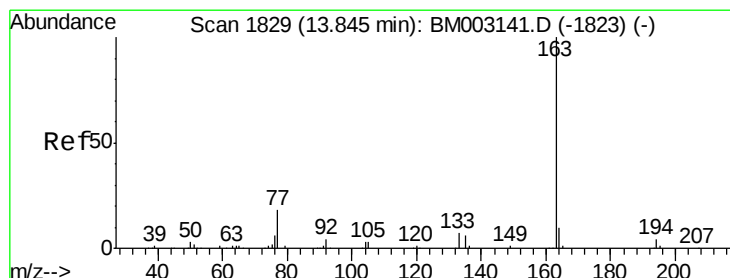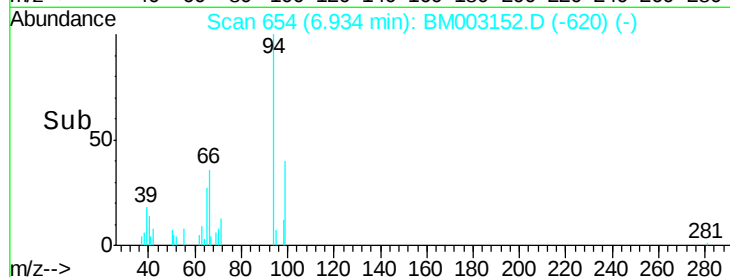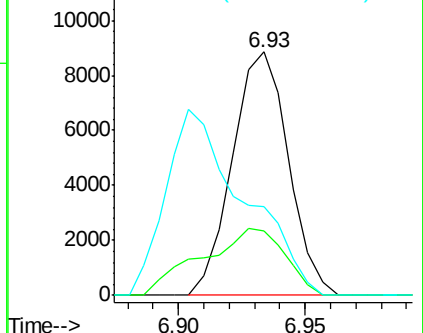

#45

Dimethylphthalate

Concen: 11.99 ng/ul

RT: 13.84 min Scan# 1829

Delta R.T. -0.00 min

Lab File: BM003152.D

Acq: 16 Nov 2015 20:50


Tgt Ion:163 Resp: 313142

Ion Ratio Lower Upper

163 100

194 3.9 3.2 4.8

164 9.8 7.8 11.8

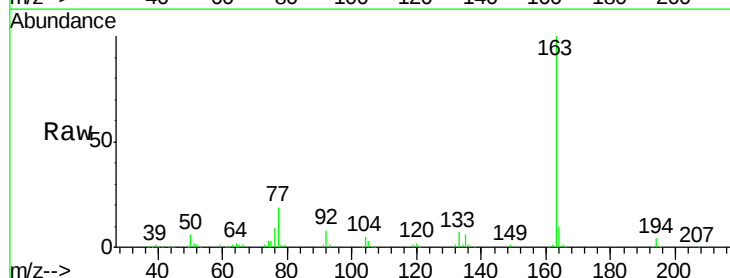

Abundance Ion 163.00 (162.70 to 163.70): BM003141.D (-1823) (-)

Ion 194.00 (193.70 to 194.70): BM003141.D (-1823) (-)

Ion 164.00 (163.70 to 164.70): BM003141.D (-1823) (-)

