

Data Path : Z:\HPCHEM1\BNA M\DATA\BM111715\
 Data File : BM003144.D
 Acq On : 16 Nov 2015 15:59
 Operator : UM/IZ
 Sample : G4309-20
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9KL4

Quant Time: Nov 17 00:20:36 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM103015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 17 00:18:48 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	123859	20.00	ng/ul	0.00
18) Naphthalene-d8	10.53	136	537298	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.39	164	291572	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.14	188	639135	20.00	ng/ul	0.00
78) Chrysene-d12	21.33	240	678700	20.00	ng/ul	0.00
86) Perylene-d12	23.59	264	669970	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.20	96	13778	5.24	ng/uL	0.00
5) Phenol-d5	6.90	99	282649	28.87	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.07	67	164778	28.78	ng/ul	0.00
9) 2-Chlorophenol-d4	7.27	132	244290	29.44	ng/ul	0.00
13) 4-Methylphenol-d8	8.45	113	232628	29.47	ng/ul	0.00
19) Nitrobenzene-d5	8.90	128	113832	34.74	ng/ul	0.00
22) 2-Nitrophenol-d4	9.62	143	121620	36.64	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.15	165	219685	29.51	ng/ul	0.00
29) 4-Chloroaniline-d4	10.67	131	317009	32.91	ng/ul	0.00
44) Dimethylphthalate-d6	13.80	166	697687	31.81	ng/ul	0.00
47) Acenaphthylene-d8	14.09	160	850052	30.58	ng/ul	0.00
52) 4-Nitrophenol-d4	14.58	143	117421	31.76	ng/ul	0.00
58) Fluorene-d10	15.39	176	601846	31.73	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.50	200	85620	28.93	ng/ul	0.00
71) Anthracene-d10	17.23	188	916252	32.34	ng/ul	0.00
79) Pyrene-d10	19.53	212	1030189	30.83	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.45	264	1086757	34.13	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.84	163	194046	8.68	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM111715\
Data File : BM003144.D
Acq On : 16 Nov 2015 15:59
Operator : UM/IZ
Sample : G4309-20
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9KL4

Quant Time: Nov 17 00:20:36 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM103015.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 17 00:18:48 2015
Response via : Initial Calibration

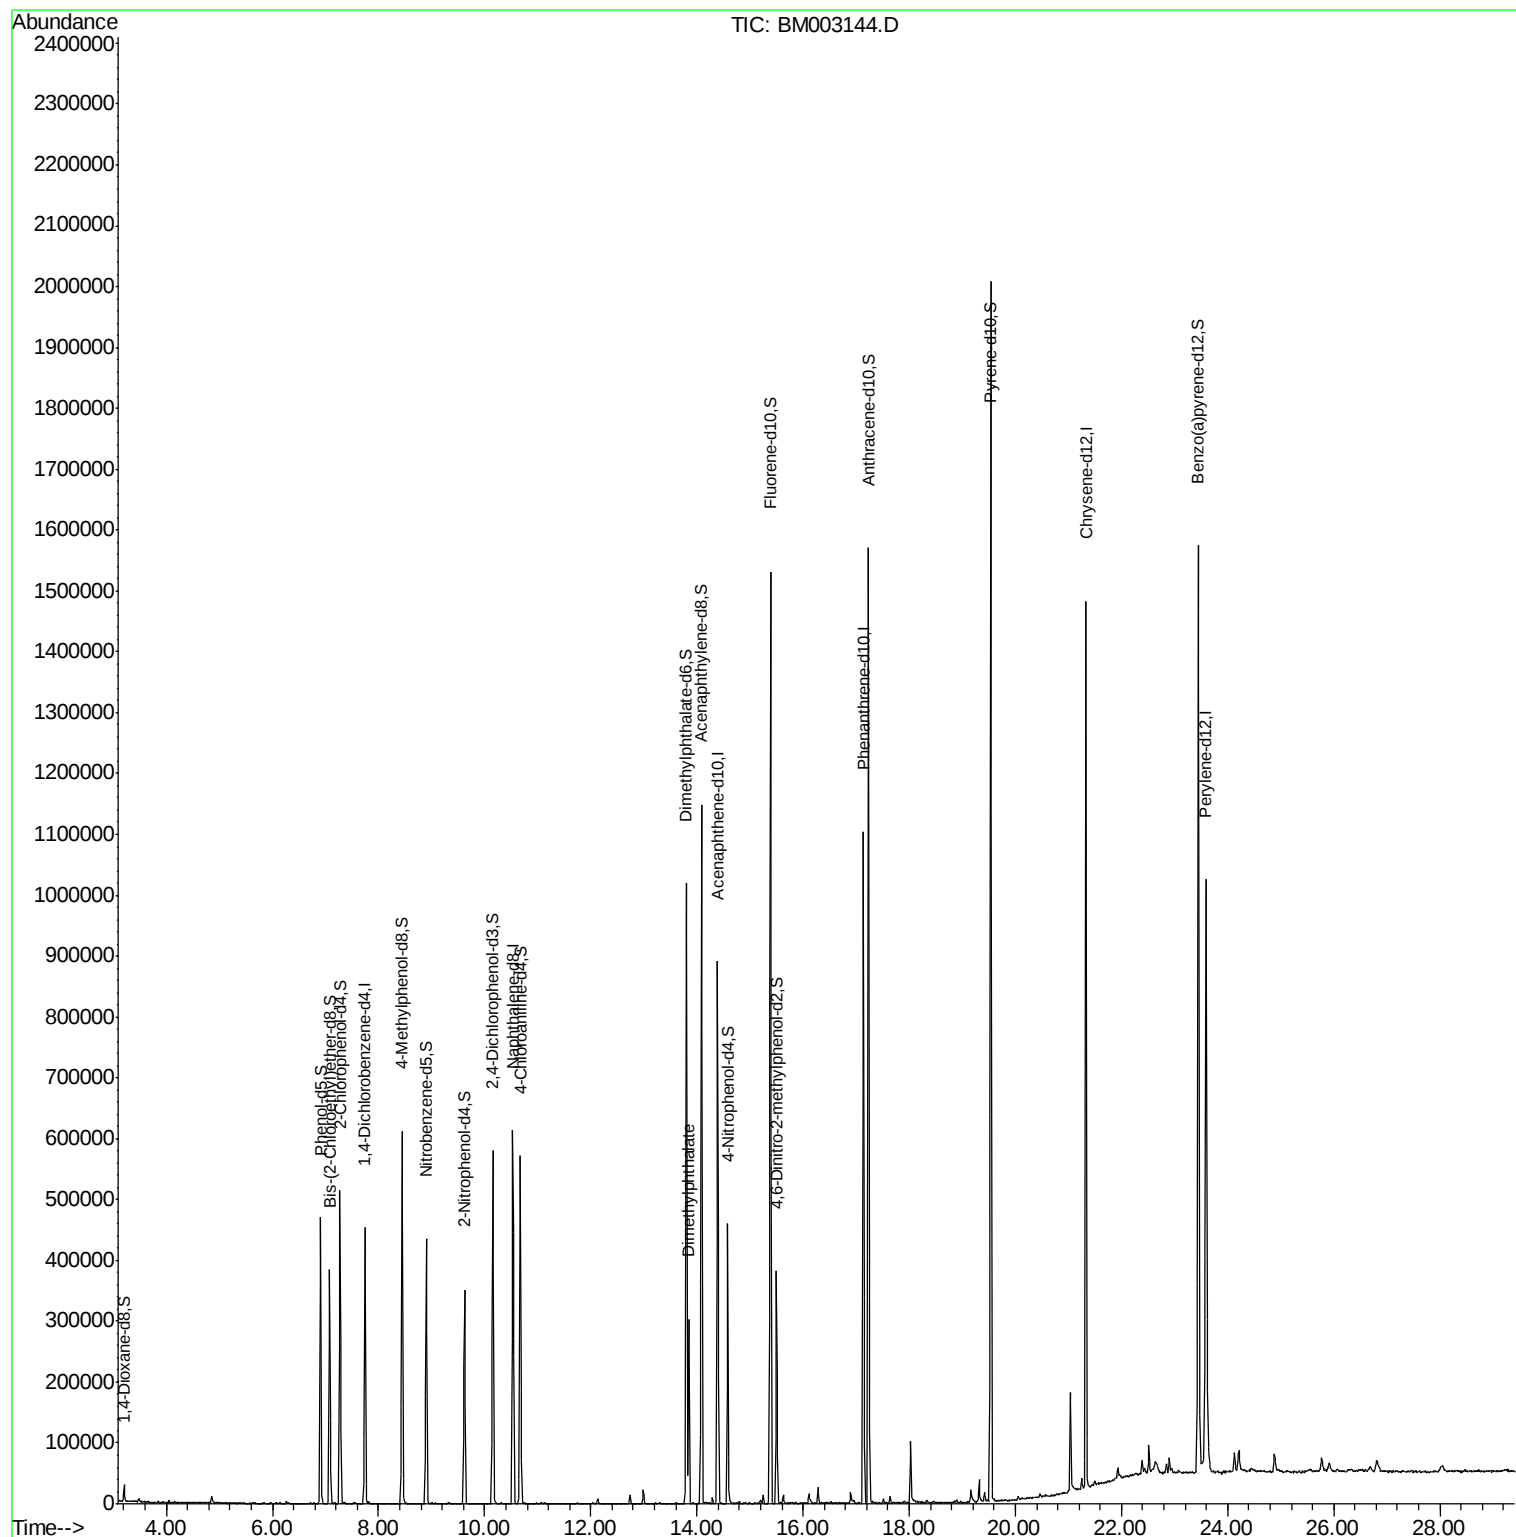

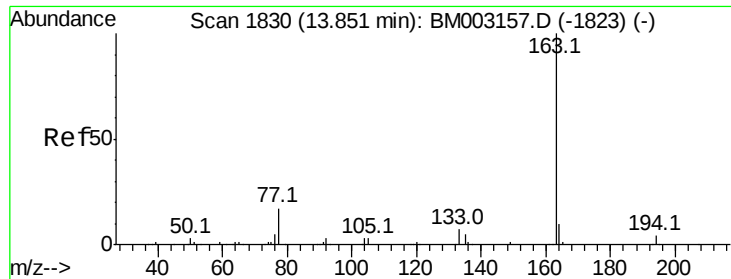

#45

Dimethylphthalate

Concen: 8.68 ng/ul

RT: 13.84 min Scan# 1829

Delta R.T. 0.00 min

Lab File: BM003144.D

Acq: 16 Nov 2015 15:59

Instrument :

BNA_M

ClientSampleId :

D9KL4


Tot Ion:163 Resp: 194046

Ion Ratio Lower Upper

163 100

194 4.0 3.2 4.8

164 10.5 7.8 11.8

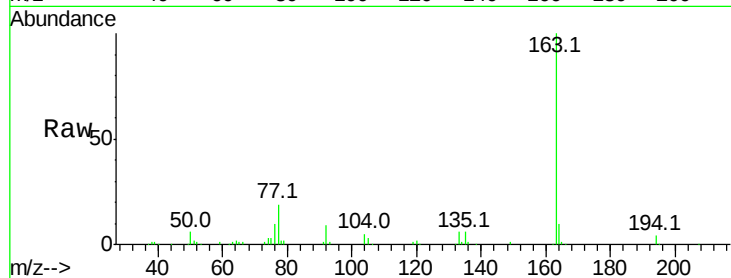

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

