

Data Path : Z:\HPCHEM1\BNA M\DATA\BM111715\
 Data File : BM003150.D
 Acq On : 16 Nov 2015 19:37
 Operator : UM/IZ
 Sample : G4309-26
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9KN6

Quant Time: Nov 17 00:21:18 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM103015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 17 00:18:48 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	111821	20.00	ng/ul	0.00
18) Naphthalene-d8	10.53	136	485500	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.39	164	270144	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.14	188	581426	20.00	ng/ul	0.00
78) Chrysene-d12	21.33	240	599815	20.00	ng/ul	0.00
86) Perylene-d12	23.59	264	609957	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.20	96	13864	5.84	ng/uL	0.00
5) Phenol-d5	6.90	99	264549	29.93	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.07	67	156767	30.33	ng/ul	0.00
9) 2-Chlorophenol-d4	7.27	132	231459	30.90	ng/ul	0.00
13) 4-Methylphenol-d8	8.45	113	221767	31.12	ng/ul	0.00
19) Nitrobenzene-d5	8.90	128	108915	36.79	ng/ul	0.00
22) 2-Nitrophenol-d4	9.62	143	115715	38.58	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.15	165	211004	31.36	ng/ul	0.00
29) 4-Chloroaniline-d4	10.67	131	319175	36.67	ng/ul	0.00
44) Dimethylphthalate-d6	13.80	166	681642	33.54	ng/ul	0.00
47) Acenaphthylene-d8	14.08	160	827154	32.12	ng/ul	0.00
52) 4-Nitrophenol-d4	14.58	143	73533	21.47	ng/ul	0.00
58) Fluorene-d10	15.39	176	584387	33.26	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.50	200	55856	20.74	ng/ul	0.00
71) Anthracene-d10	17.23	188	868418	33.69	ng/ul	0.00
79) Pyrene-d10	19.53	212	940505	31.85	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.45	264	1023240	35.30	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.85	163	211074	10.19	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM111715\
Data File : BM003150.D
Acq On : 16 Nov 2015 19:37
Operator : UM/IZ
Sample : G4309-26
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9KN6

Quant Time: Nov 17 00:21:18 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM103015.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 17 00:18:48 2015
Response via : Initial Calibration

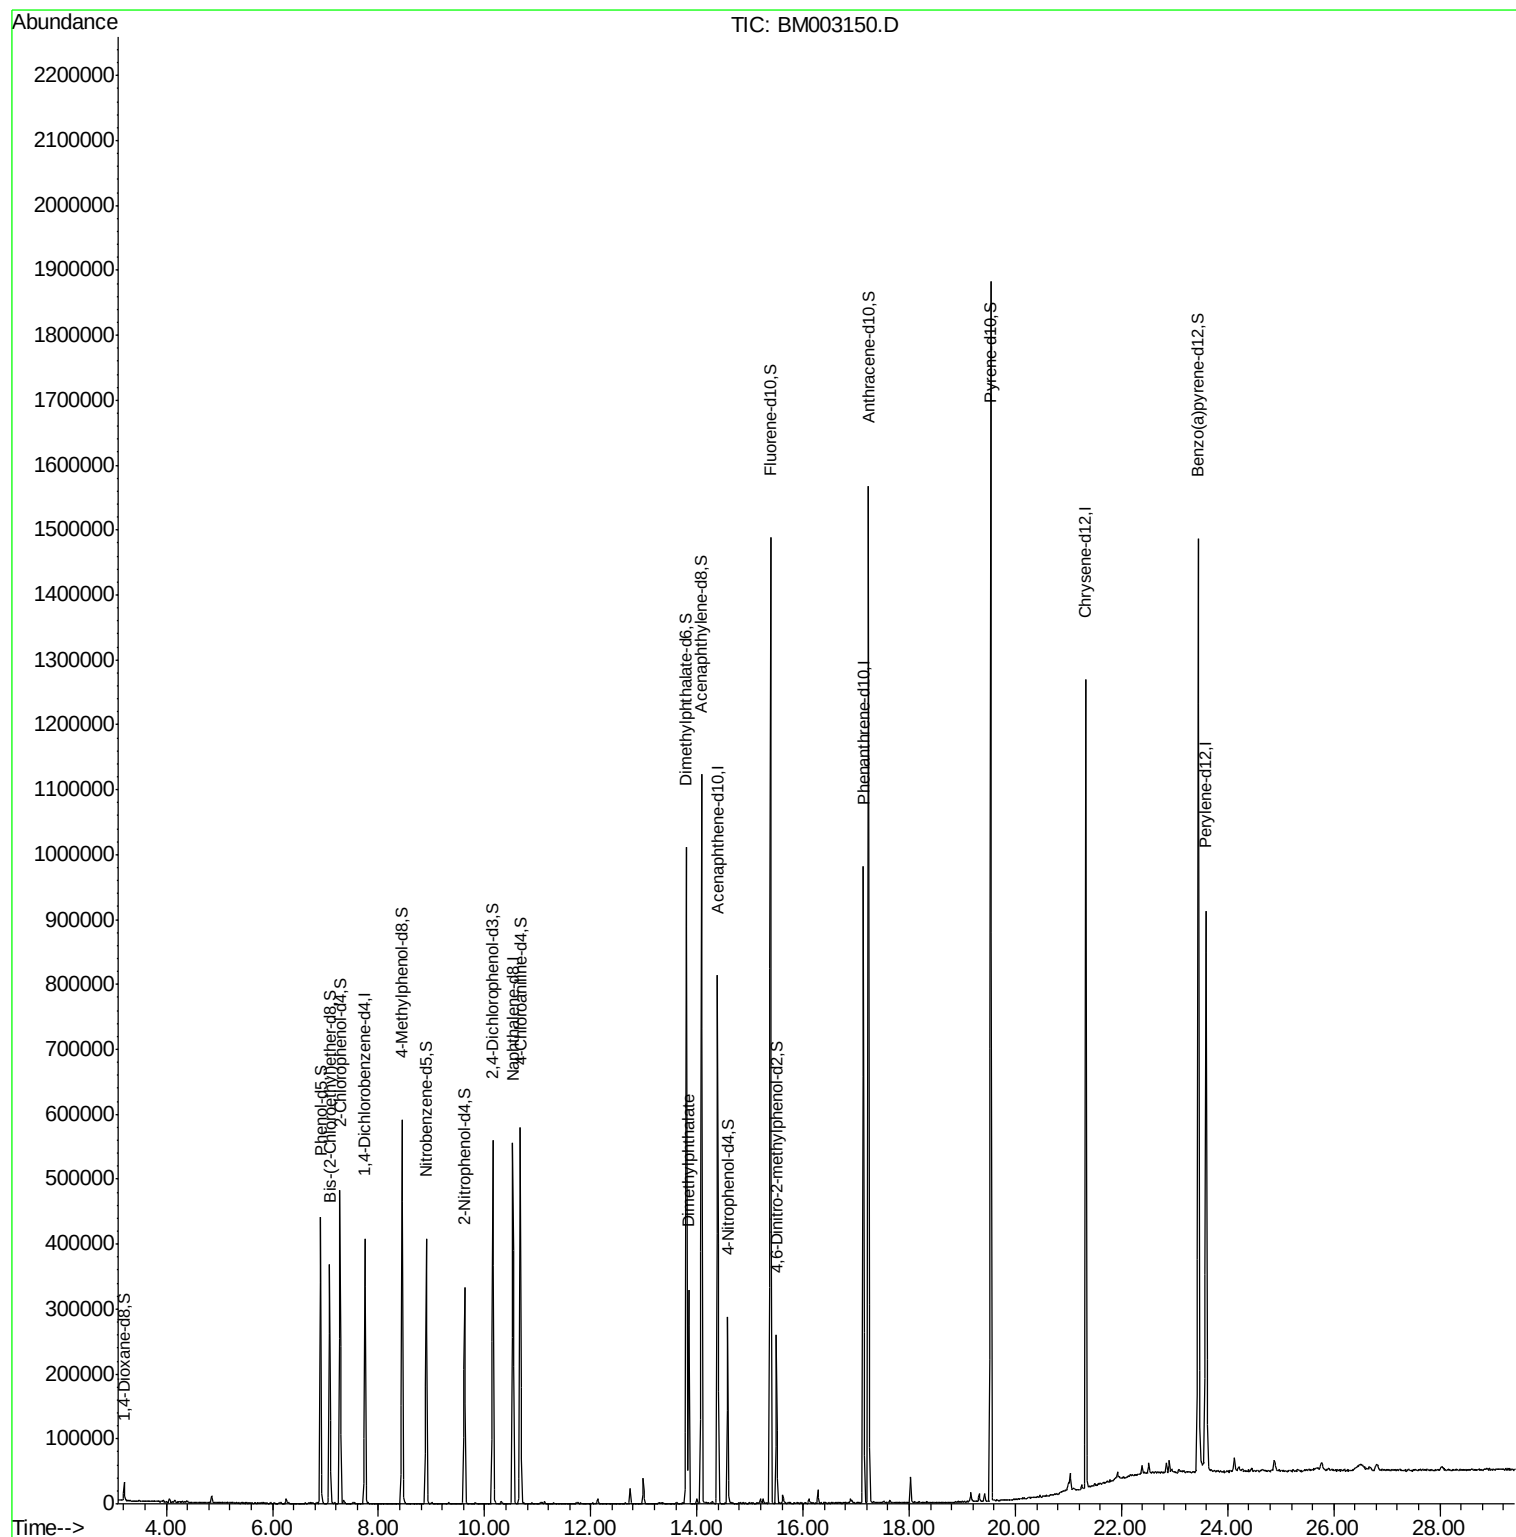

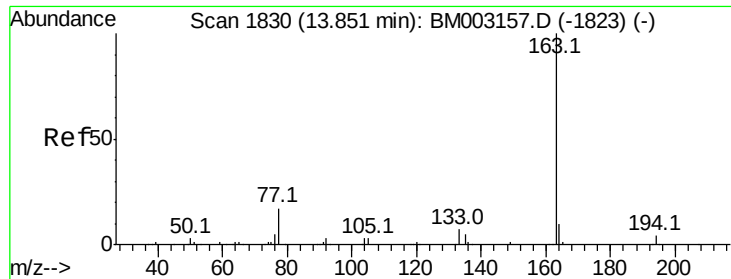

#45

Dimethylphthalate

Concen: 10.19 ng/ul

RT: 13.85 min Scan# 1829

Delta R.T. 0.00 min

Lab File: BM003150.D

Acq: 16 Nov 2015 19:37

Instrument :

BNA_M

ClientSampleId :

D9KN6


Tot Ion:163 Resp: 211074

Ion Ratio Lower Upper

163 100

194 3.9 3.2 4.8

164 10.0 7.8 11.8

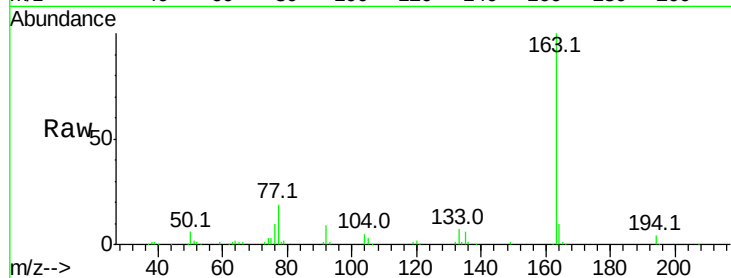

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

