

Data Path : Z:\HPCHEM1\BNA M\DATA\BM111715\
 Data File : BM003151.D
 Acq On : 16 Nov 2015 20:13
 Operator : UM/IZ
 Sample : G4323-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4HT6

Quant Time: Nov 17 00:21:25 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM103015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 17 00:18:48 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	134459	20.00	ng/ul	0.00
18) Naphthalene-d8	10.53	136	572170	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.39	164	314777	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.13	188	709791	20.00	ng/ul	0.00
78) Chrysene-d12	21.33	240	790027	20.00	ng/ul	0.00
86) Perylene-d12	23.59	264	783807	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.20	96	11247	3.94	ng/uL	0.00
5) Phenol-d5	6.90	99	206675	19.44	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.07	67	121764	19.59	ng/ul	0.00
9) 2-Chlorophenol-d4	7.27	132	180697	20.06	ng/ul	0.00
13) 4-Methylphenol-d8	8.45	113	168958	19.71	ng/ul	0.00
19) Nitrobenzene-d5	8.90	128	80537	23.08	ng/ul	0.00
22) 2-Nitrophenol-d4	9.62	143	85358	24.15	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.15	165	158096	19.94	ng/ul	0.00
29) 4-Chloroaniline-d4	10.67	131	205830	20.06	ng/ul	0.00
44) Dimethylphthalate-d6	13.80	166	508307	21.46	ng/ul	0.00
47) Acenaphthylene-d8	14.08	160	597424	19.91	ng/ul	0.00
52) 4-Nitrophenol-d4	14.58	143	78432	19.65	ng/ul	0.00
58) Fluorene-d10	15.39	176	424644	20.74	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.50	200	55144	16.78	ng/ul	0.00
71) Anthracene-d10	17.23	188	651876	20.72	ng/ul	0.00
79) Pyrene-d10	19.53	212	725381	18.65	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.44	264	751336	20.17	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.85	163	267872	11.10	ng/ul	99




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM111715\
Data File : BM003151.D
Acq On : 16 Nov 2015 20:13
Operator : UM/IZ
Sample : G4323-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4HT6

Quant Time: Nov 17 00:21:25 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM103015.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 17 00:18:48 2015
Response via : Initial Calibration

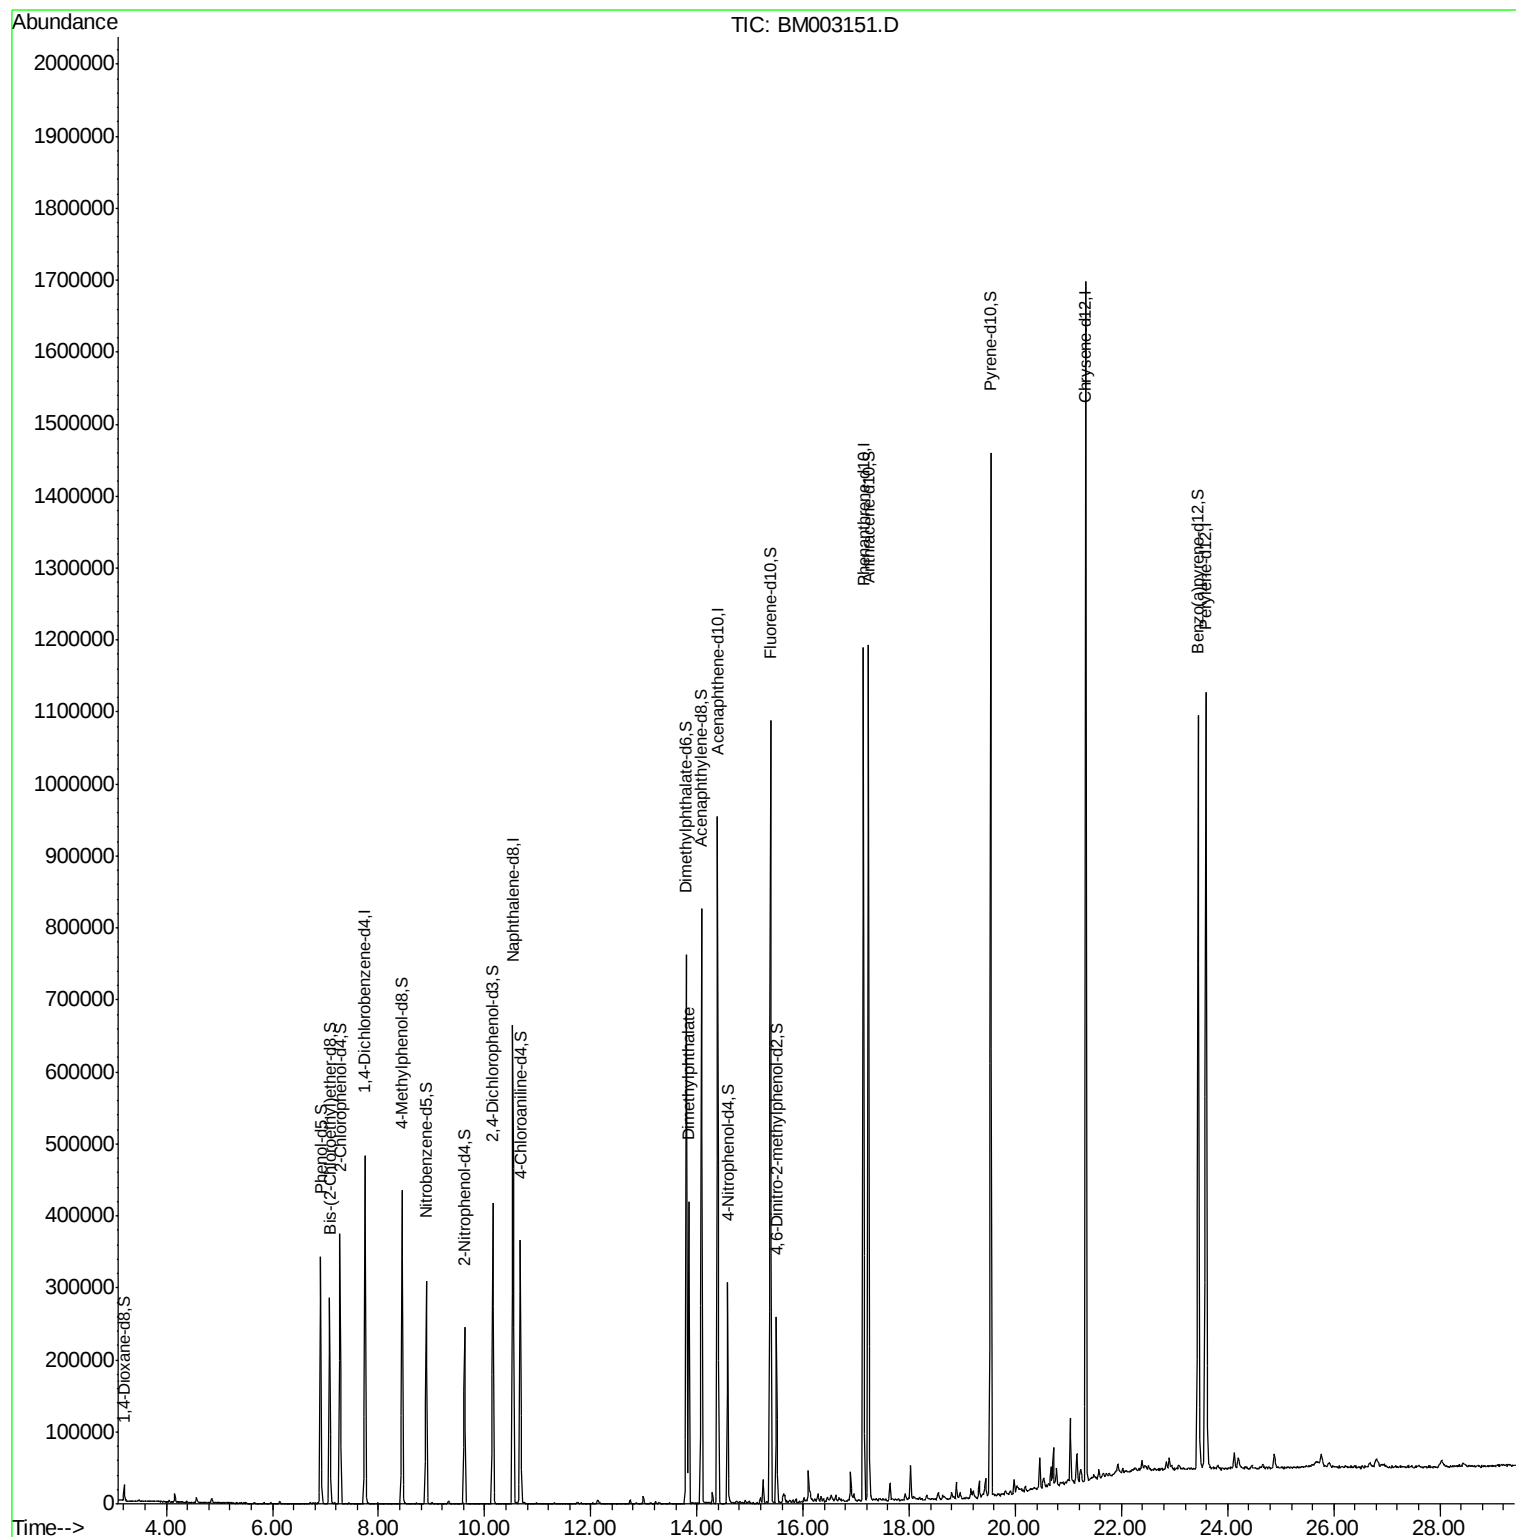

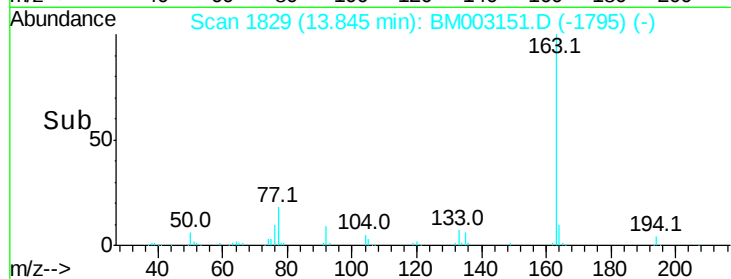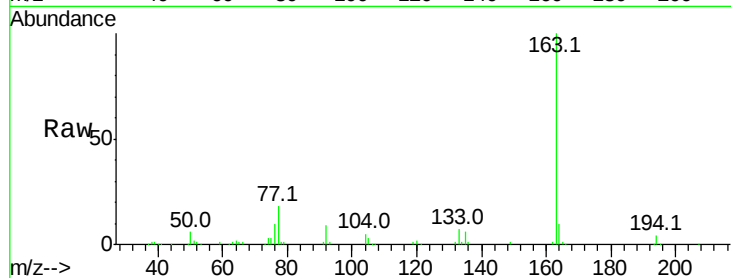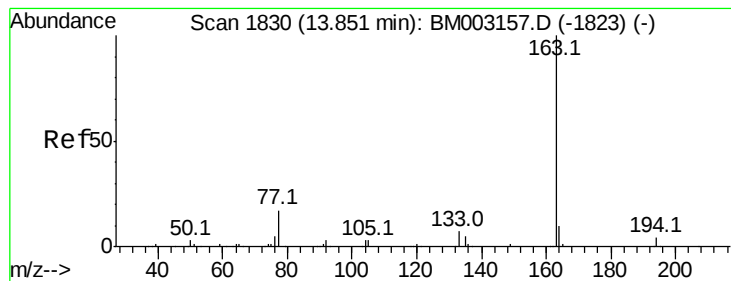

#45

Dimethylphthalate

Concen: 11.10 ng/ul

RT: 13.85 min Scan# 1829

Delta R.T. 0.00 min

Lab File: BM003151.D

Acq: 16 Nov 2015 20:13

Instrument :

BNA_M

ClientSampleId :

A4HT6

Tot Ion:163 Resp: 267872

Ion Ratio Lower Upper

163 100

194 3.9 3.2 4.8

164 10.2 7.8 11.8

