

Data Path : Z:\HPCHEM1\BNA M\DATA\BM111715\
 Data File : BM003156.D
 Acq On : 16 Nov 2015 23:14
 Operator : UM/IZ
 Sample : G4323-26
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4J46

Manual Integrations
 APPROVED

mmdadoda
 11/17/2015 5:57:33 PM

Quant Time: Nov 17 02:14:28 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM103015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 17 00:18:48 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.75	152	145889	20.00	ng/ul	0.00
18) Naphthalene-d8	10.53	136	654785	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.39	164	366764	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.14	188	763187	20.00	ng/ul	0.00
78) Chrysene-d12	21.33	240	767946	20.00	ng/ul	0.00
86) Perylene-d12	23.59	264	774950	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.20	96	8286	2.68	ng/uL	0.00
5) Phenol-d5	6.90	99	146180	12.67	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.07	67	90072	13.36	ng/ul	0.00
9) 2-Chlorophenol-d4	7.27	132	132240	13.53	ng/ul	0.00
13) 4-Methylphenol-d8	8.45	113	92551	9.95	ng/ul	0.00
19) Nitrobenzene-d5	8.90	128	61948	15.51	ng/ul	0.00
22) 2-Nitrophenol-d4	9.62	143	65198	16.12	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.15	165	117689	12.97	ng/ul	0.00
29) 4-Chloroaniline-d4	10.67	131	86484	7.37	ng/ul	0.00
44) Dimethylphthalate-d6	13.80	166	378065	13.70	ng/ul	0.00
47) Acenaphthylene-d8	14.08	160	394678	11.29	ng/ul	0.00
52) 4-Nitrophenol-d4	14.58	143	41006	8.82	ng/ul	0.00
58) Fluorene-d10	15.39	176	262437	11.00	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.50	200	31362	8.87	ng/ul	0.00
71) Anthracene-d10	17.23	188	329109	9.73	ng/ul	0.00
79) Pyrene-d10	19.53	212	310399	8.21	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.44	264	246971	6.71	ng/ul	-0.01

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.85	163	219569	7.81	ng/ul	99
70) Phenanthrene	17.18	178	199173	4.61	ng/ul	99
77) Fluoranthene	19.20	202	280542m	6.42	ng/ul	
80) Pyrene	19.56	202	257333	5.12	ng/ul#	92
83) Benzo(a)anthracene	21.31	228	120845	2.87	ng/ul	96
85) Chrysene	21.36	228	127996	3.07	ng/ul	97
88) Benzo(b)fluoranthene	22.90	252	165841	3.71	ng/ul	98
89) Benzo(k)fluoranthene	22.94	252	47291m	1.14	ng/ul	
91) Benzo(a)pyrene	23.49	252	111364m	2.63	ng/ul	
92) Indeno(1,2,3-cd)pyrene	25.86	276	73470	1.58	ng/ul#	89
94) Benzo(g,h,i)perylene	26.56	276	66844	1.60	ng/ul	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM111715\
Data File : BM003156.D
Acq On : 16 Nov 2015 23:14
Operator : UM/IZ
Sample : G4323-26
Misc :
ALS Vial : 17 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
A4J46

Quant Time: Nov 17 02:14:28 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM103015.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 17 00:18:48 2015
Response via : Initial Calibration

Manual Integrations
APPROVED

mmdadoda
11/17/2015 5:57:33 PM

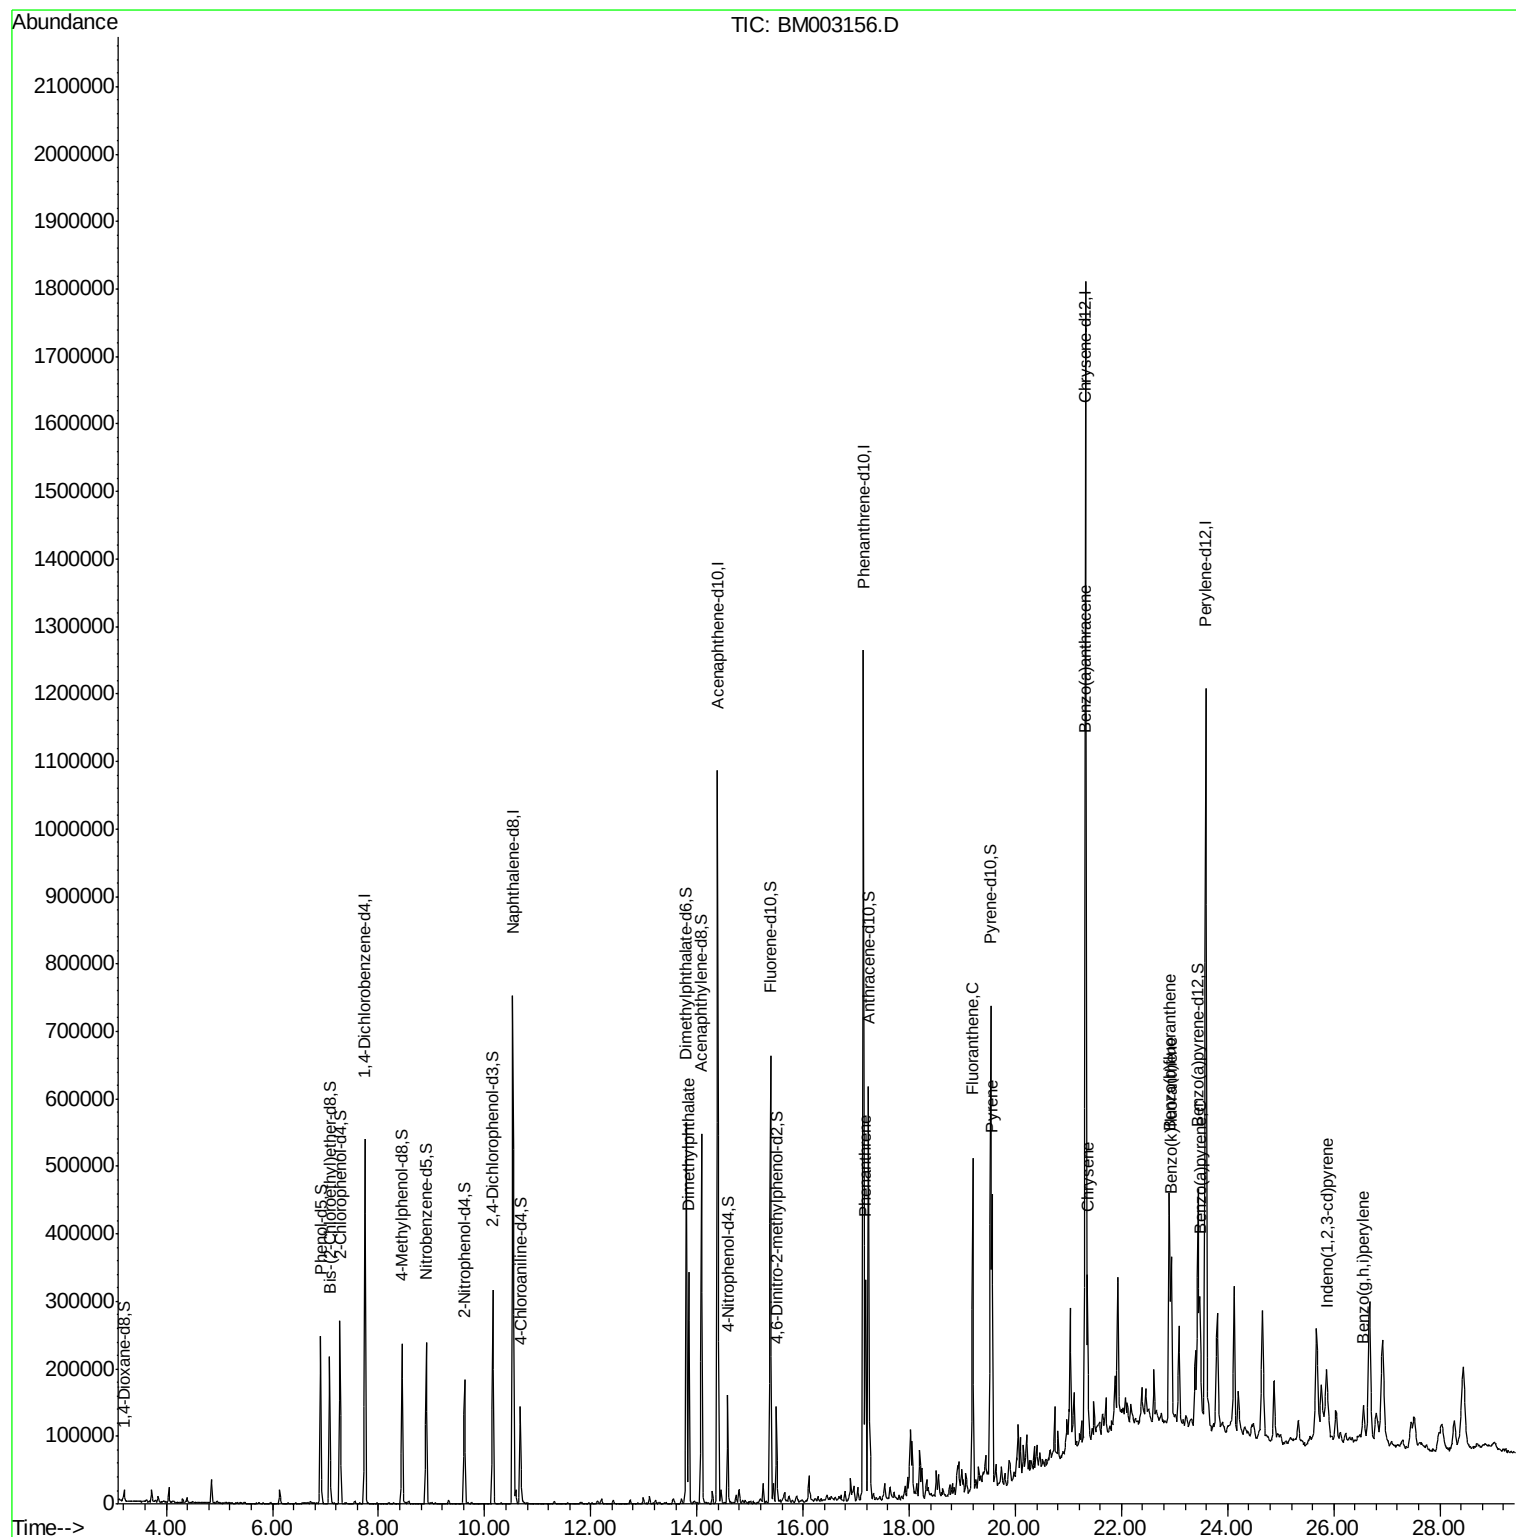

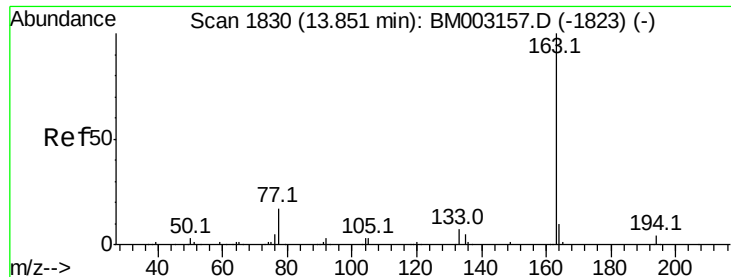

#45

Dimethylphthalate

Concen: 7.81 ng/ul

RT: 13.85 min Scan# 1829

Delta R.T. 0.00 min

Lab File: BM003156.D

Acq: 16 Nov 2015 23:14

Instrument :

BNA_M





ClientSampleId :

A4J46

Tot Ion:	163	Resp:	219569
Ion Ratio	Lower	Upper	
163	100		
194	3.9	3.2	4.8
164	10.1	7.8	11.8

Manual Integrations
APPROVED

mmdadoda
11/17/2015 5:57:33 PM

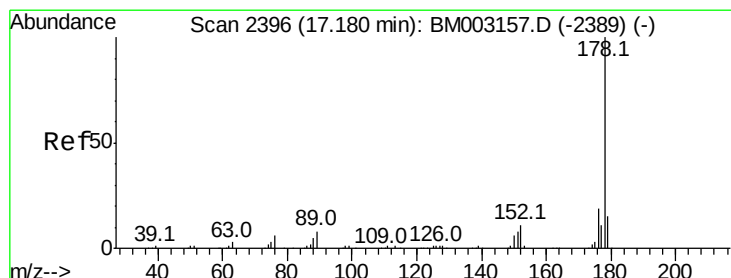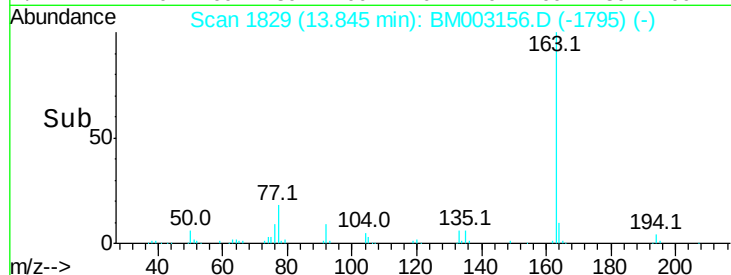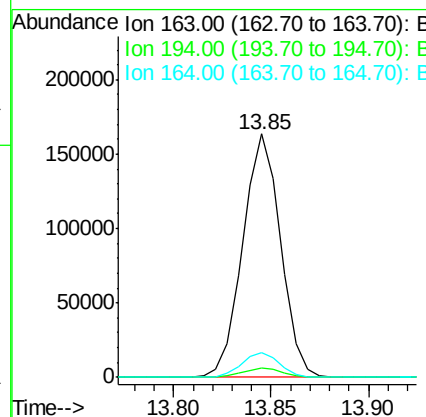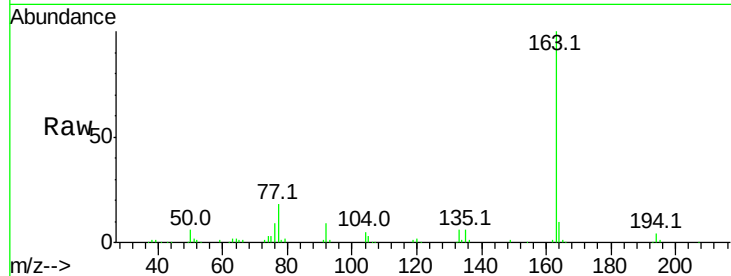

#70

Phenanthrene

Concen: 4.61 ng/ul




RT: 17.18 min Scan# 2396


Delta R.T. 0.00 min

Lab File: BM003156.D

Acq: 16 Nov 2015 23:14

Tgt Ion:	178	Resp:	199173
Ion Ratio	Lower	Upper	
178	100		
179	15.3	12.2	18.4
176	19.2	14.7	22.1

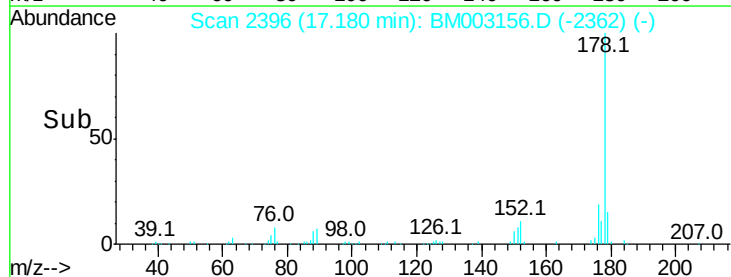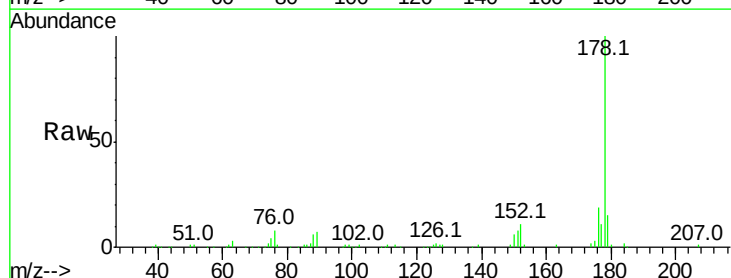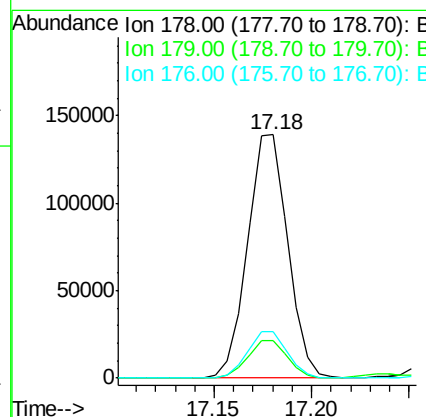

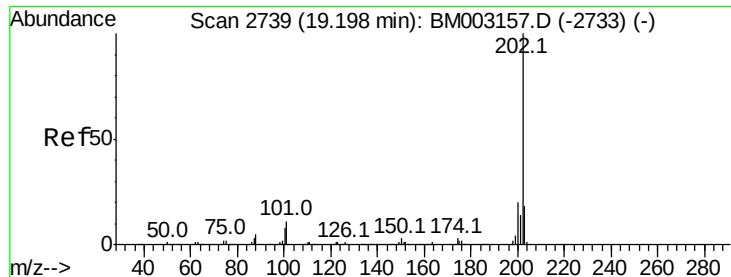

#77

Fluoranthene

Concen: 6.42 ng/ul m

RT: 19.20 min Scan# 2739

Delta R.T. 0.00 min

Lab File: BM003156.D

Acq: 16 Nov 2015 23:14

Instrument :

BNA_M





ClientSampleId :

A4J46

Tot Ion:	202	Resp:	280542
Ion Ratio	Lower	Upper	
202	100		
101	10.4	10.4	15.6#
100	7.9	7.8	11.6

Manual Integrations
APPROVED

mmdadoda
11/17/2015 5:57:33 PM

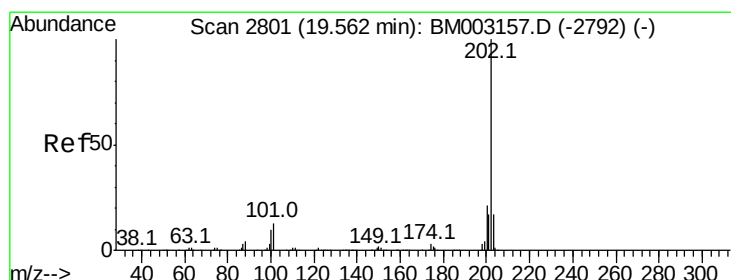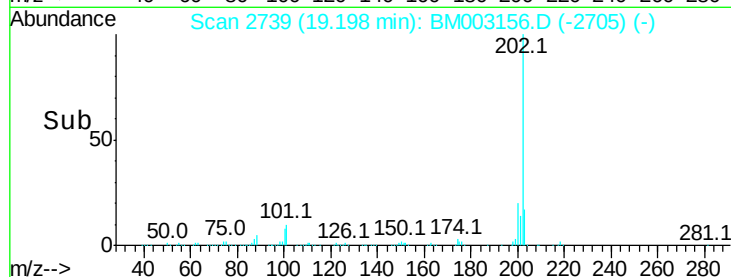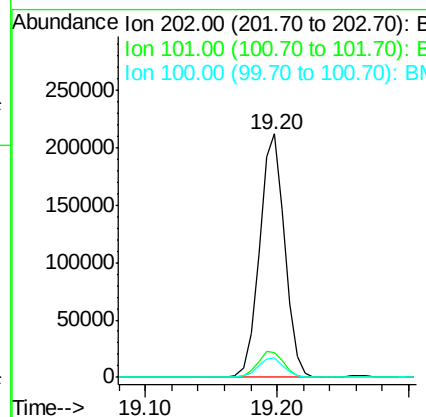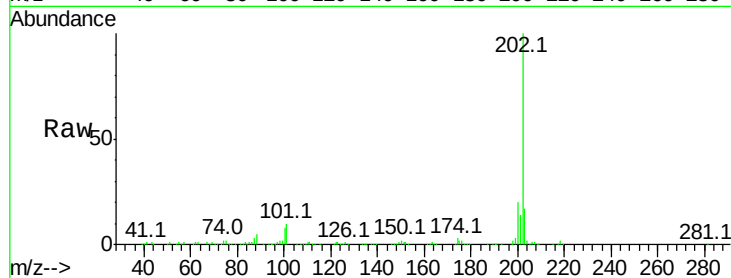

#80

Pyrene

Concen: 5.12 ng/ul




RT: 19.56 min Scan# 2801


Delta R.T. 0.00 min

Lab File: BM003156.D

Acq: 16 Nov 2015 23:14

Tgt Ion:	202	Resp:	257333
Ion Ratio	Lower	Upper	
202	100		
101	12.7	12.6	18.8
100	9.9	10.6	15.8#

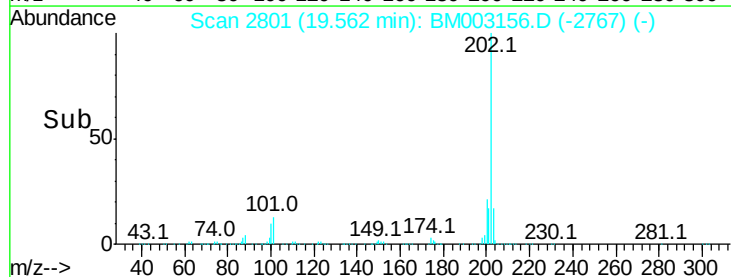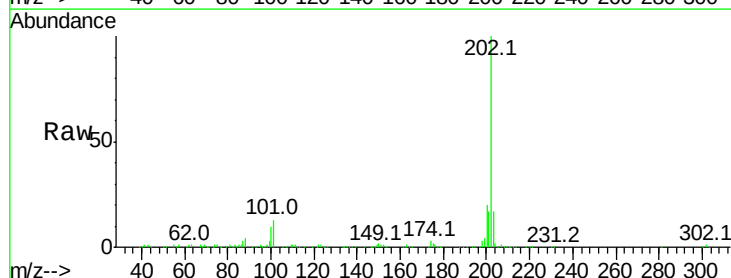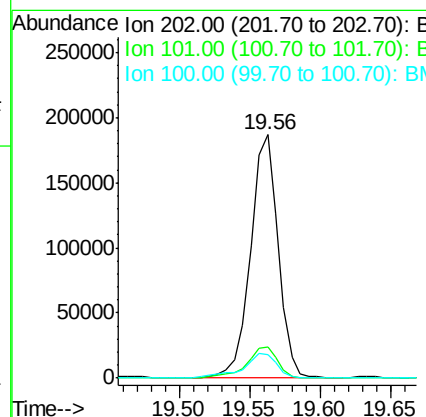

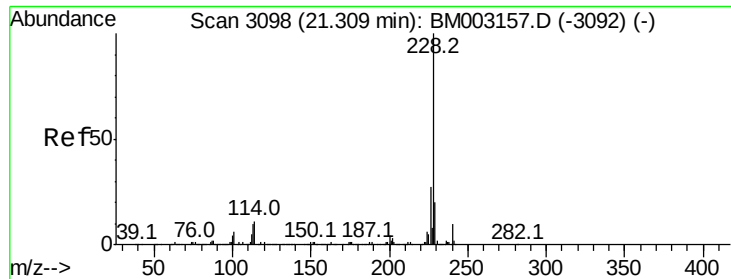





#83
Benzo(a)anthracene
Concen: 2.87 ng/ul
RT: 21.31 min Scan# 3098
Delta R.T. -0.01 min
Lab File: BM003156.D
Acq: 16 Nov 2015 23:14

Instrument :
BNA_M
ClientSampleId :
A4J46

Tot Ion	Ratio	Resp	Lower	Upper
228	100	120845		
229	21.6		15.6	23.4
226	27.9		21.0	31.6




Manual Integrations
APPROVED


mmdadoda
11/17/2015 5:57:33 PM

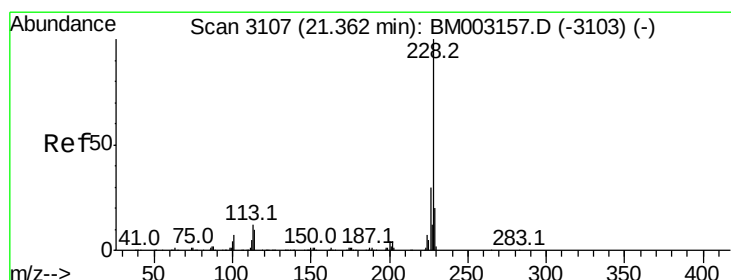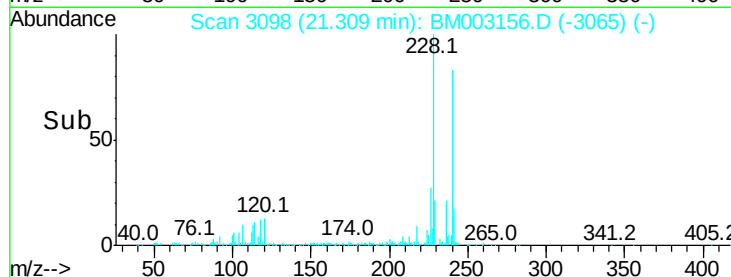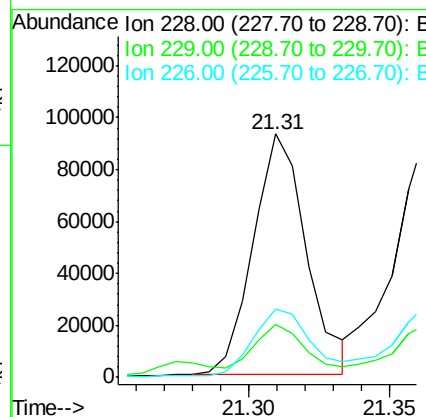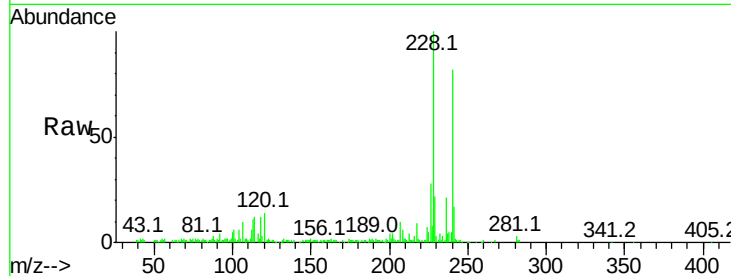

#85
Chrysene
Concen: 3.07 ng/ul
RT: 21.36 min Scan# 3107
Delta R.T. -0.01 min
Lab File: BM003156.D
Acq: 16 Nov 2015 23:14

Tgt Ion	Ratio	Resp	Lower	Upper
228	100	127996		
226	29.8		23.3	34.9
229	22.0		15.8	23.6

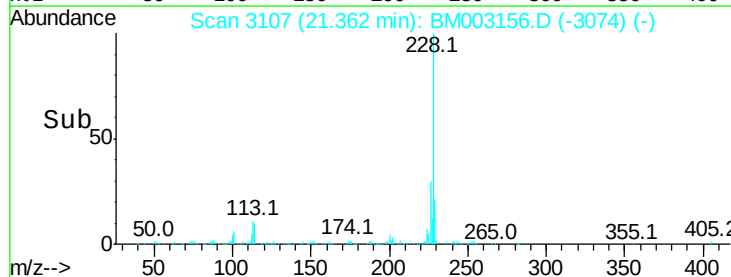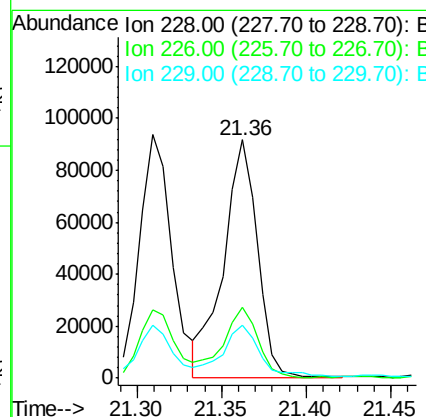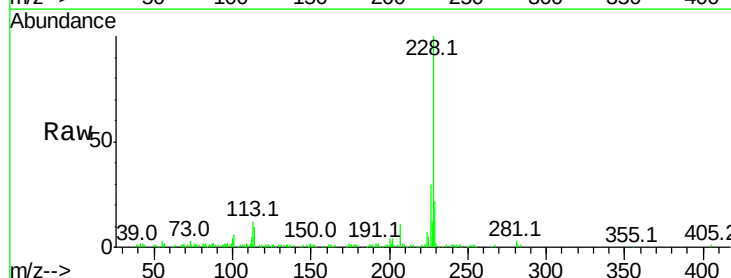

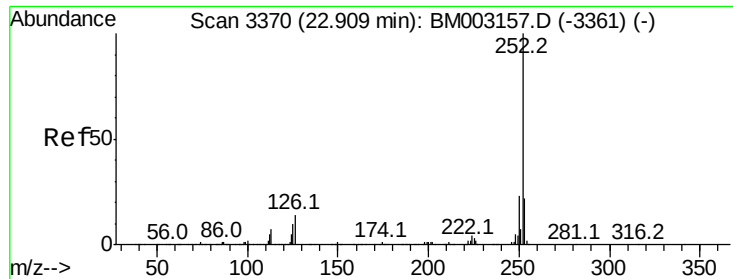

#88

Benzo(b)fluoranthene

Concen: 3.71 ng/ul

RT: 22.90 min Scan# 3369

Delta R.T. -0.01 min

Lab File: BM003156.D


Acq: 16 Nov 2015 23:14

Instrument :

BNA_M

ClientSampleId :




A4J46

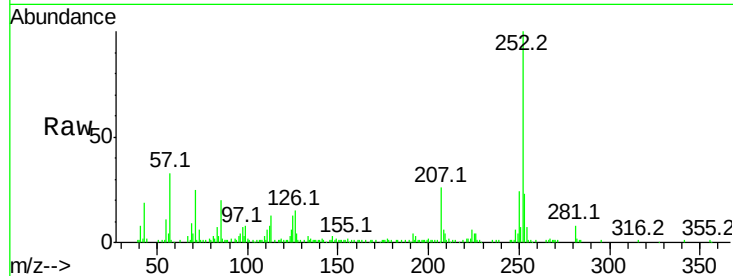

Tot Ion	Ratio	Lower	Upper
252	100		
253	23.1	17.4	26.2
125	12.6	10.7	16.1

Manual Integrations
APPROVED

mmdadoda
11/17/2015 5:57:33 PM

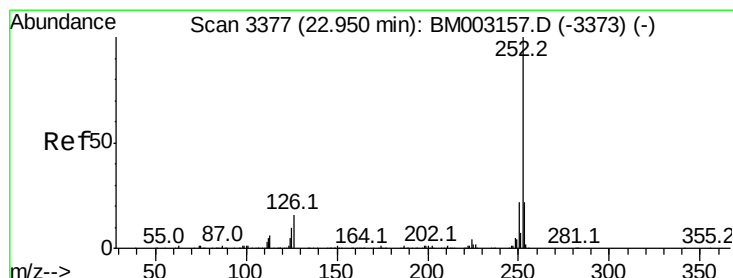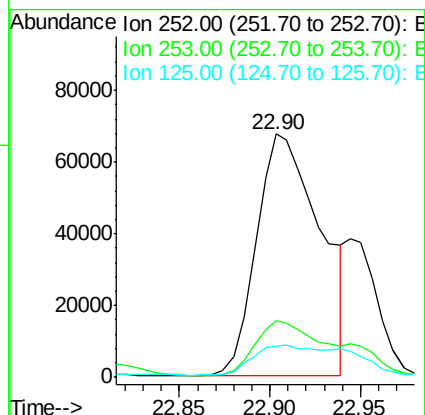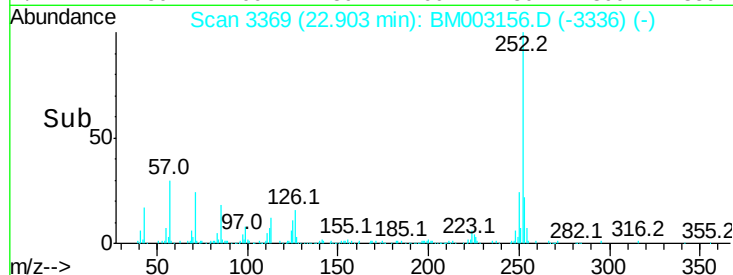

#89

Benzo(k)fluoranthene


Concen: 1.14 ng/ul m

RT: 22.94 min Scan# 3376



Delta R.T. -0.01 min


Lab File: BM003156.D

Acq: 16 Nov 2015 23:14

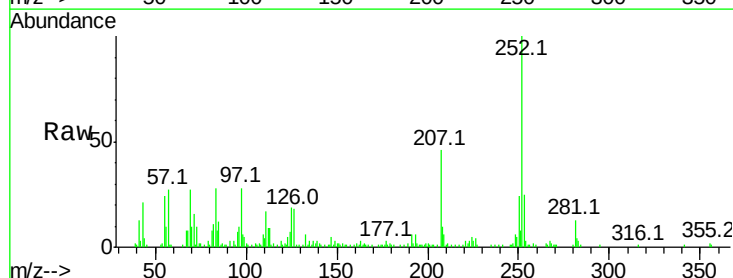

Tgt Ion	Ratio	Lower	Upper
252	100		
253	24.6	17.4	26.0
125	18.9	11.1	16.7#

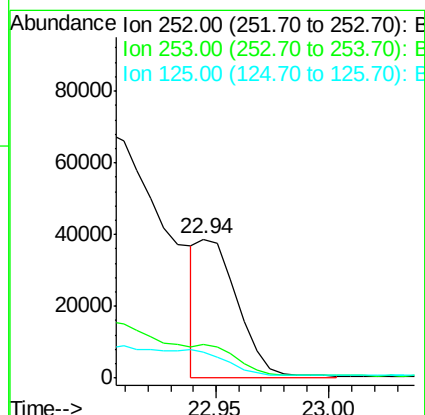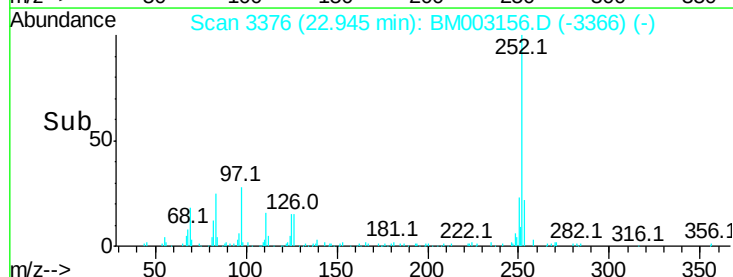

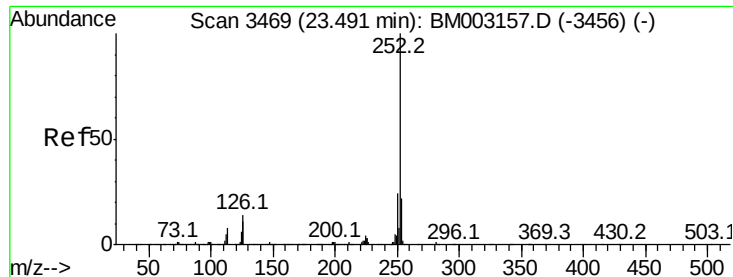

#91

Benzo(a)pyrene

Concen: 2.63 ng/ul m

RT: 23.49 min Scan# 3468

Delta R.T. -0.01 min

Lab File: BM003156.D

Acq: 16 Nov 2015 23:14

Instrument :

BNA_M





ClientSampleId :

A4J46

Tot Ion	Ratio	Resp Lower	Upper
252	100		
253	23.4	17.1	25.7
125	11.9	11.9	17.9#

Manual Integrations
APPROVED

mmdadoda
11/17/2015 5:57:33 PM

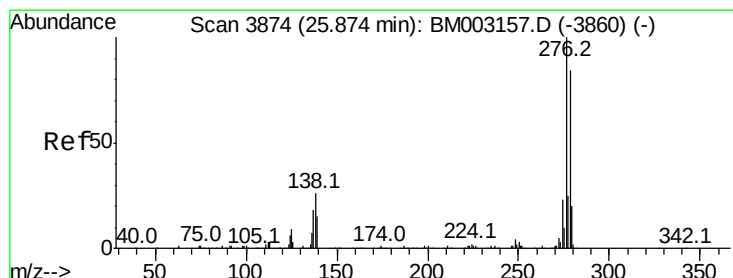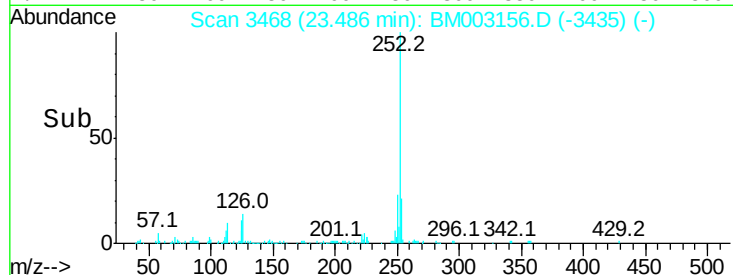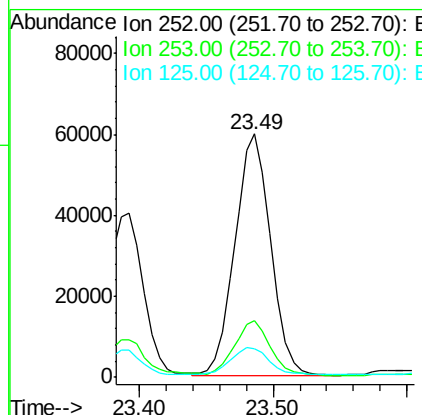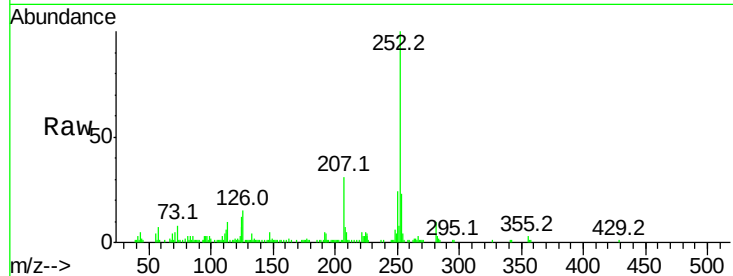

#92

Indeno(1,2,3-cd)pyrene

Concen: 1.58 ng/ul




RT: 25.86 min Scan# 3872




Delta R.T. -0.02 min

Lab File: BM003156.D

Acq: 16 Nov 2015 23:14

Tgt Ion	Ratio	Resp Lower	Upper
276	100		
138	23.0	26.6	40.0#
277	25.5	20.2	30.4

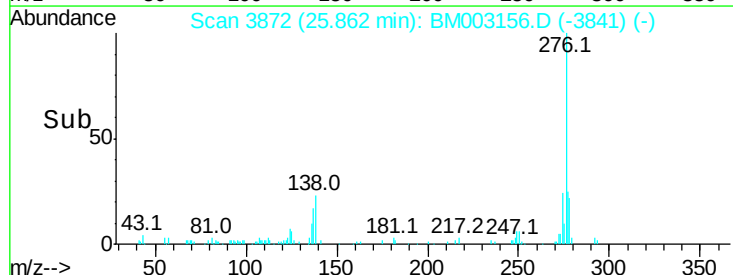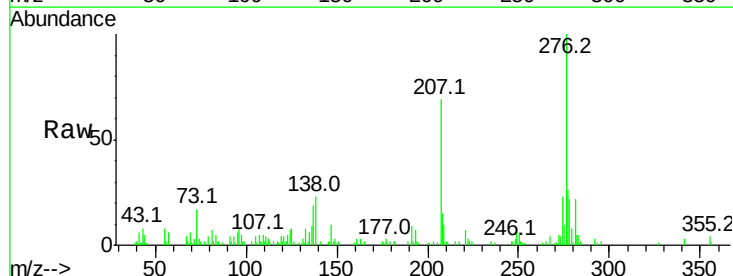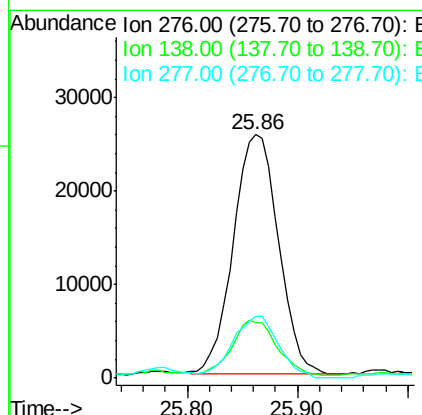

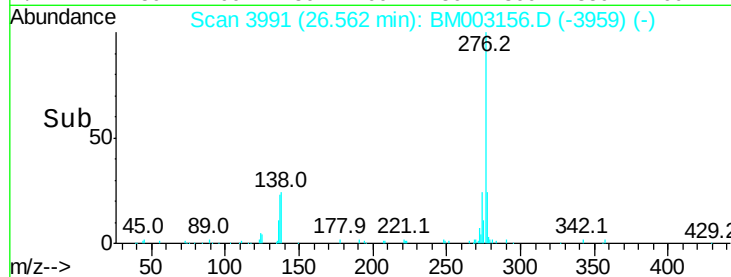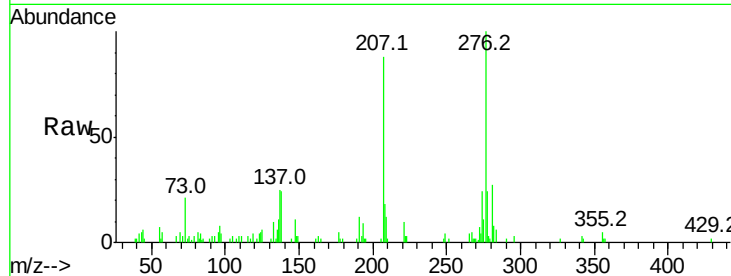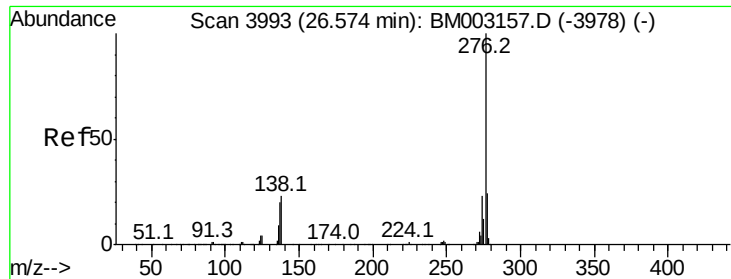

#94

Benzo(a,h,i)perylene

Concen: 1.60 ng/ul

RT: 26.56 min Scan# 3991

Delta R.T. -0.01 min

Lab File: BM003156.D

Acq: 16 Nov 2015 23:14

Instrument :

BNA_M

ClientSampleId :

A4J46

Tot Ion: 276 Resp: 66844

Ion Ratio Lower Upper

276 100

138 24.2 23.8 35.6

277 23.9 19.4 29.2

Manual Integrations
APPROVED

mmdadoda
11/17/2015 5:57:33 PM

