


Data Path : Z:\HPCHEM1\BNA M\Data\BM111715\
Data File : BM003140.D
Acq On : 16 Nov 2015 13:32
Operator : UM/IZ
Sample : DFTPP44
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP44

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM102715.M
Title : SVOA CALIBRATION
Last Update : Wed Oct 28 01:48:36 2015

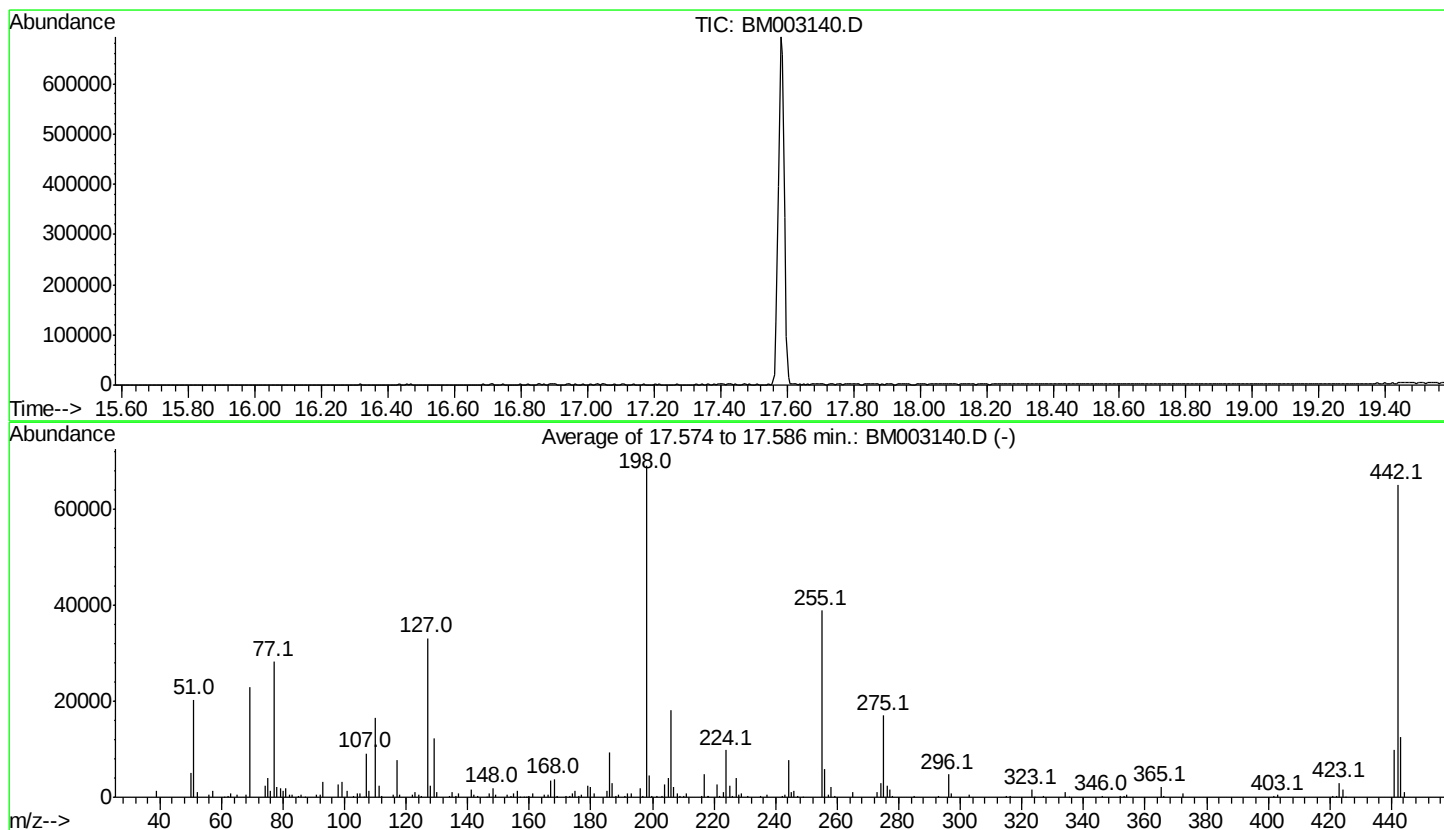

AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2458

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.3	20285	PASS
68	69	0.00	2	1.8	415	PASS
69	198	0.00	100	33.2	22970	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.0	33186	PASS
197	198	0.00	2	0.4	255	PASS
198	198	100	100	100.0	69122	PASS
199	198	5	9	6.7	4620	PASS
275	198	10	60	24.6	17008	PASS
365	198	1	100	3.2	2195	PASS
441	443	0.01	100	78.8	9955	PASS
442	198	50	100	94.2	65117	PASS
443	442	15	24	19.4	12637	PASS

Scan 2458 (17.545 min): BM003140.D
DFTPP44

m/z	Abundance
40.00	311.0
44.00	447.0
207.00	860.0

Instrument :
BNA_M
ClientSampleId :
DFTPP44

m/z	Abundance
39.00	1240.0
43.90	419.0
50.00	4117.0
51.10	16744.0
52.10	985.0
56.00	530.0
57.00	1173.0
62.10	308.0
63.00	828.0
65.00	408.0
68.00	411.0
69.00	18704.0
74.00	2082.0
75.00	3081.0
76.00	994.0
77.10	23016.0
78.00	1600.0
79.00	1578.0
80.00	1097.0
81.00	1525.0
82.00	385.0
83.00	323.0
85.90	440.0
91.00	382.0
92.00	471.0
93.00	2471.0
98.00	2029.0
99.00	2977.0
100.90	869.0
104.00	592.0
105.00	616.0
107.00	6897.0
108.00	1135.0
110.00	12635.0
111.00	2007.0
111.90	301.0
115.90	412.0
117.00	5745.0
118.00	545.0
122.00	464.0
123.00	864.0
124.00	327.0
127.00	25224.0
128.00	2232.0
129.00	9322.0
130.00	763.0
135.00	773.0
136.10	312.0
137.00	881.0
141.00	1351.0
141.90	346.0
147.00	652.0
148.00	1505.0
149.00	583.0
153.00	356.0
153.90	322.0
155.00	658.0
156.00	958.0
161.00	538.0
165.00	445.0
166.00	377.0
167.00	2659.0
168.00	3660.0
168.90	404.0
174.00	506.0
175.00	934.0
177.00	420.0
179.00	1777.0
180.00	1730.0
180.90	677.0
185.00	744.0
186.10	6526.0
187.00	1960.0
189.00	390.0
191.90	556.0
193.00	632.0
196.00	1239.0
198.00	47336.0
199.00	3192.0
204.00	2165.0
205.10	2857.0
206.10	12074.0
207.00	2757.0
208.00	583.0
211.10	495.0
217.00	3391.0
217.90	425.0
221.10	1872.0
222.00	343.0
223.00	820.0
224.00	6490.0
225.10	1501.0

Instrument :
BNA_M
ClientSampleId :
DFTPP44

226.00	364.0
227.00	2908.0
228.00	513.0
229.00	662.0
237.00	550.0
243.10	320.0
244.10	4891.0
245.00	686.0
246.00	1070.0
255.10	25320.0
256.00	3996.0
257.10	433.0
258.00	1450.0
265.00	679.0
273.00	772.0
274.10	1945.0
275.00	10265.0
276.10	1442.0
277.10	1028.0
296.00	2934.0
297.10	483.0
323.10	958.0
334.00	636.0
365.00	1362.0
372.10	472.0
423.10	1542.0
424.10	1088.0
441.10	4961.0
442.10	32408.0
443.10	6812.0
444.00	651.0

Instrument :
BNA_M
ClientSampleId :
DFTPP44

m/z	Abundance
39.00	1726.0
40.00	411.0
44.00	365.0
50.10	6052.0
51.00	24368.0
52.00	1380.0
56.00	760.0
57.00	1724.0
61.00	348.0
62.00	391.0
63.00	1130.0
65.00	569.0
68.00	446.0
69.00	27480.0
74.00	2805.0
75.00	4847.0
76.00	1568.0
77.10	33712.0
78.10	2569.0
79.00	2166.0
80.00	1735.0
81.00	2477.0
82.00	560.0
83.00	527.0
84.90	492.0
86.00	672.0
86.90	378.0
91.00	532.0
92.00	602.0
93.00	3831.0
98.00	3283.0
99.00	3672.0
101.00	1552.0
103.00	479.0
104.00	835.0
105.00	805.0
106.00	302.0
107.00	11280.0
108.00	1593.0
110.00	20280.0
111.00	2967.0
111.90	309.0
116.00	560.0
117.00	9520.0
118.00	859.0
122.00	725.0
123.00	1128.0
124.00	572.0
125.00	426.0
127.00	40040.0
128.00	2869.0
129.00	14957.0
130.00	1143.0
134.00	404.0
135.00	1331.0
135.90	410.0
137.00	1014.0
141.00	1891.0
142.00	528.0
143.00	497.0
146.00	397.0
147.00	1041.0
148.00	2364.0
149.00	742.0
152.90	599.0
154.00	534.0
155.00	1062.0
156.00	1565.0
158.00	359.0
159.00	322.0
160.00	496.0
161.00	932.0
165.00	721.0
165.90	490.0
167.00	4014.0
168.00	4272.0
169.10	510.0
172.00	385.0
172.90	485.0
174.00	911.0
175.00	1596.0
176.00	507.0
176.90	769.0
179.00	2689.0
180.00	2539.0
181.00	1023.0
185.00	1662.0
186.00	10887.0
187.00	3153.0
188.00	516.0
189.00	767.0
191.00	397.0

Instrument :
BNA_M
ClientSampleId :
DFTPP44

192.00	1024.0
193.00	1133.0
196.00	1912.0
197.00	437.0
198.00	83016.0
199.00	5499.0
200.00	369.0
201.60	319.0
203.00	550.0
204.00	2984.0
205.00	4924.0
206.10	21576.0
207.10	3410.0
208.00	916.0
209.00	397.0
210.20	414.0
211.10	851.0
216.00	420.0
217.00	5927.0
218.10	702.0
221.00	3185.0
223.00	1204.0
224.10	11585.0
225.10	3261.0
226.00	422.0
227.00	4830.0
228.10	771.0
229.00	923.0
230.90	390.0
235.00	396.0
237.00	735.0
242.10	520.0
243.00	711.0
244.10	9253.0
245.10	1206.0
246.00	1693.0
247.00	420.0
249.00	316.0
255.10	45552.0
256.00	6785.0
257.00	651.0
258.00	2687.0
259.00	462.0
265.00	1074.0
273.00	1274.0
274.10	3440.0
275.10	19968.0
276.10	2803.0
277.00	1729.0
278.00	345.0
285.10	319.0
293.00	426.0
296.00	5537.0
297.00	812.0
303.00	592.0
315.00	535.0
316.00	325.0
323.10	1807.0
326.90	326.0
334.10	1271.0
335.10	397.0
346.00	386.0
352.10	475.0
353.00	371.0
354.10	547.0
365.10	2363.0
366.00	360.0
372.10	991.0
402.00	430.0
403.10	599.0
421.10	516.0
422.00	592.0
423.10	3527.0
424.10	1675.0
441.10	11399.0
442.10	73720.0
443.10	14348.0
444.10	1451.0

Instrument :
BNA_M
ClientSampleId :
DFTPP44

m/z	Abundance
39.10	1421.0
40.00	348.0
43.90	412.0
50.00	4911.0
51.10	19744.0
52.00	937.0
55.90	625.0
57.00	1203.0
63.00	873.0
65.00	507.0
67.90	389.0
69.00	22728.0
74.00	2367.0
75.00	3785.0
76.10	1160.0
77.10	27816.0
78.00	2163.0
79.00	1640.0
80.00	1241.0
81.00	1945.0
82.00	596.0
83.00	453.0
84.90	445.0
86.00	653.0
90.90	540.0
92.00	559.0
93.00	3158.0
98.00	2478.0
99.00	2792.0
101.00	1261.0
103.00	381.0
104.00	758.0
104.90	621.0
107.00	9303.0
108.00	1663.0
110.00	16624.0
111.00	2438.0
111.90	392.0
116.00	440.0
117.00	8018.0
118.00	600.0
122.00	533.0
123.00	952.0
124.00	513.0
124.90	384.0
127.00	34296.0
128.00	2259.0
129.00	12811.0
130.00	1209.0
133.90	315.0
134.90	1073.0
135.90	394.0
137.00	842.0
141.00	1590.0
142.00	526.0
143.00	355.0
147.00	987.0
148.00	1937.0
148.90	588.0
153.00	484.0
154.00	307.0
155.00	960.0
156.00	1583.0
157.00	303.0
160.00	571.0
161.10	885.0
164.90	590.0
166.00	663.0
167.00	3634.0
168.00	3539.0
169.00	394.0
171.90	380.0
173.00	476.0
174.00	742.0
175.00	1379.0
176.00	466.0
177.00	665.0
179.00	2900.0
180.00	2247.0
181.00	786.0
185.10	1274.0
186.00	10711.0
187.00	3332.0
188.10	326.0
188.90	543.0
191.00	385.0
192.00	841.0
193.00	1036.0
196.00	2092.0
197.00	328.0
198.00	77016.0
199.00	5171.0

Instrument :
BNA_M
ClientSampleId :
DFTPP44

199.90	406.0
201.50	379.0
203.00	511.0
204.00	2916.0
205.10	4628.0
206.10	20856.0
207.10	3207.0
208.00	1008.0
209.00	379.0
210.20	323.0
211.00	788.0
215.90	471.0
217.00	5430.0
217.90	613.0
221.10	2940.0
221.90	713.0
223.10	1141.0
224.10	11507.0
225.10	2708.0
226.10	348.0
227.00	4590.0
228.00	659.0
229.00	1029.0
230.90	303.0
235.00	373.0
237.00	691.0
242.10	602.0
243.00	572.0
244.10	9004.0
245.00	1192.0
246.10	1630.0
247.00	334.0
255.00	45712.0
256.00	6511.0
257.00	695.0
258.00	2623.0
259.00	457.0
265.10	1102.0
273.10	1248.0
274.00	3653.0
275.10	20792.0
276.10	2603.0
277.00	1675.0
278.00	362.0
285.00	317.0
293.00	383.0
296.10	5935.0
297.00	862.0
303.10	670.0
315.00	573.0
316.10	378.0
323.10	1780.0
324.10	411.0
327.00	339.0
334.00	1203.0
346.00	426.0
352.00	613.0
353.10	403.0
354.10	720.0
365.10	2861.0
366.00	373.0
372.10	1088.0
402.00	459.0
403.10	715.0
421.10	653.0
422.00	507.0
423.10	4082.0
424.10	1682.0
425.10	313.0
441.10	13506.0
442.10	89224.0
443.10	16752.0
444.10	1444.0

Instrument :
BNA_M
ClientSampleId :
DFTPP44