


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111717\
Data File : BM013034.D
Acq On : 18 Nov 2017 11:36
Operator : SJ/JU
Sample : I6405-21 5X
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BE2W2

Manual Integrations
APPROVED

SOHIL
11/20/2017 4:30:37 PM

Quant Time: Nov 20 06:52:29 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111617.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Nov 20 06:14:09 2017
Response via : Initial Calibration

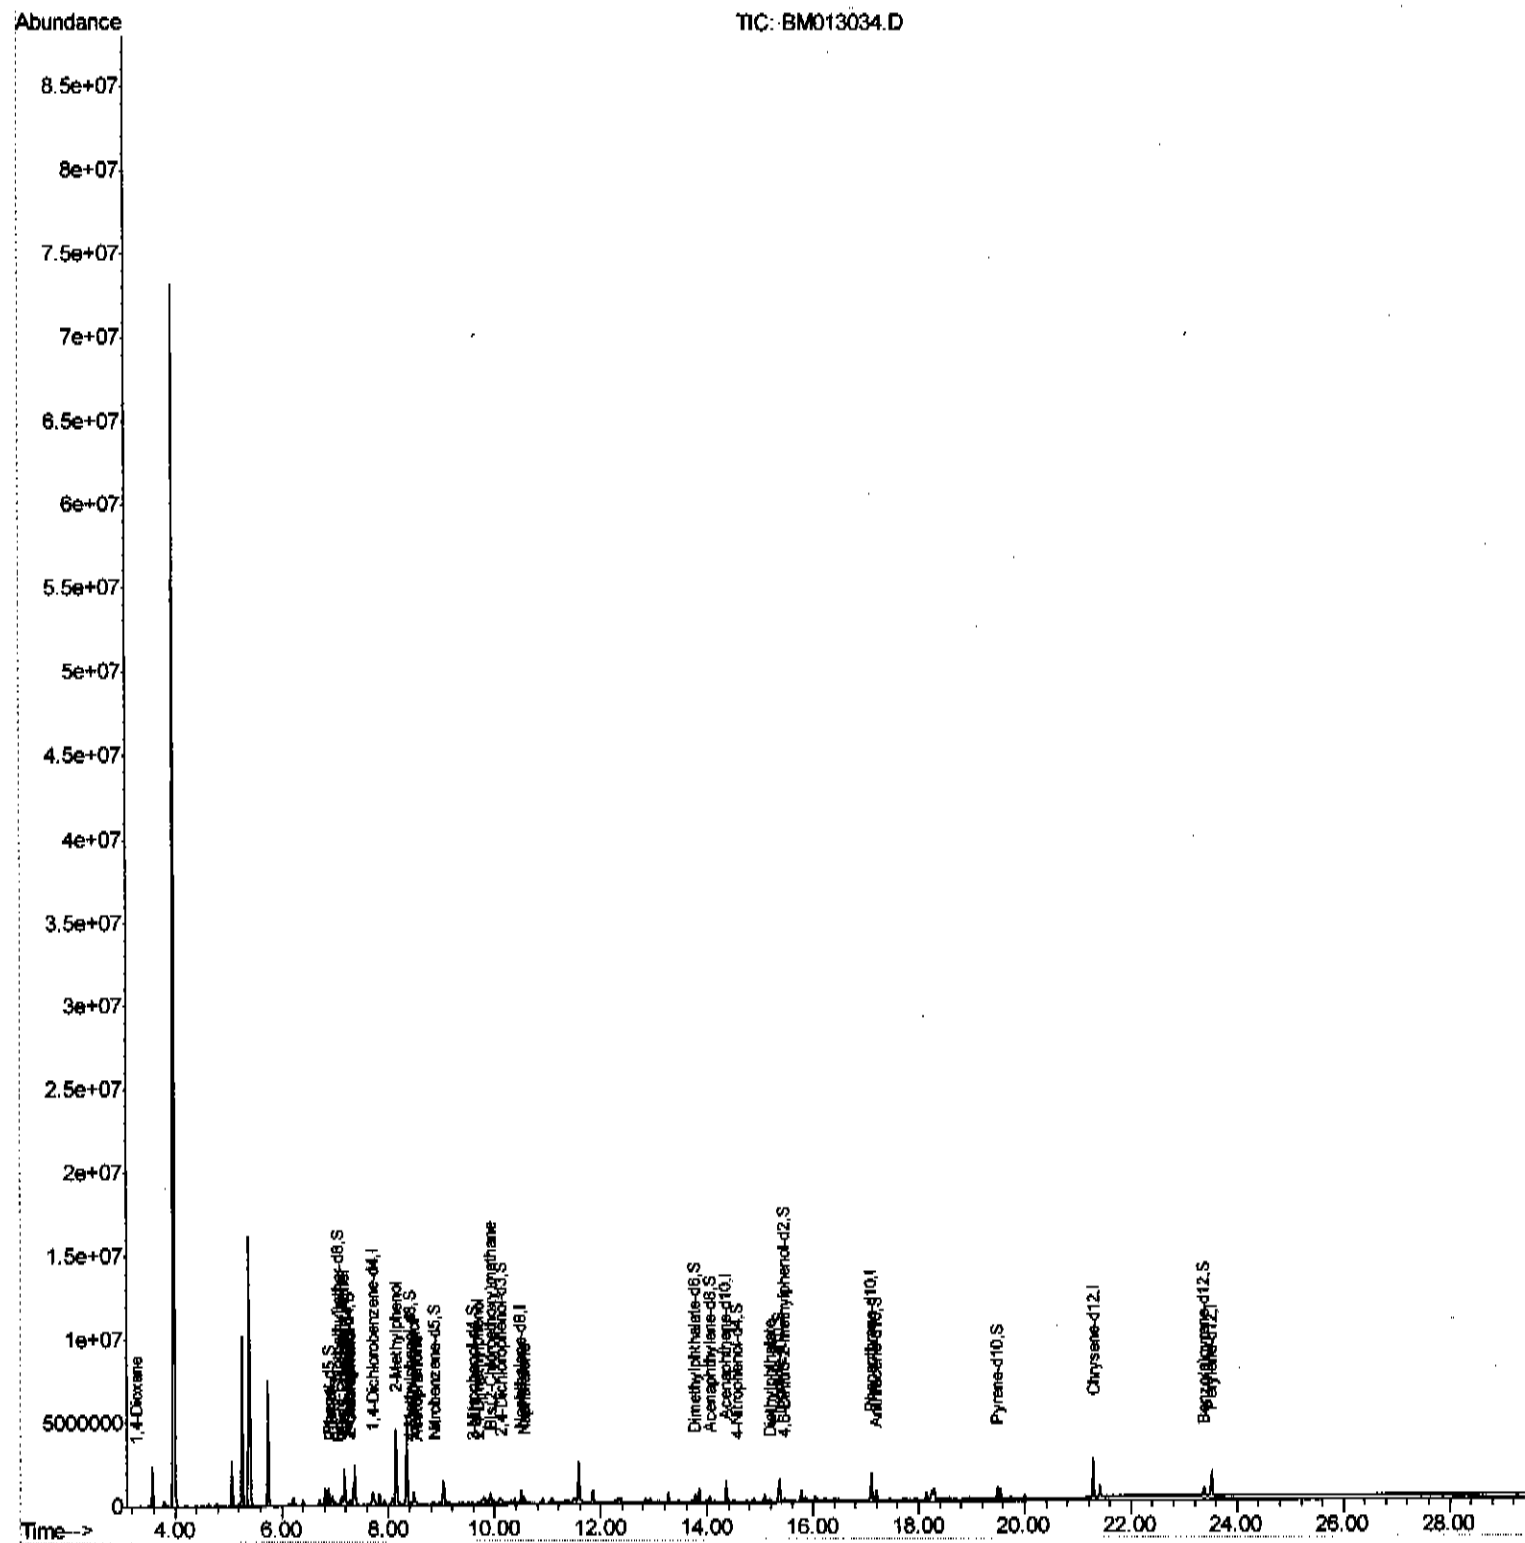




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111717\
 Data File : BM013034.D
 Acq On : 18 Nov 2017 11:36
 Operator : SJ/JU
 Sample : I6405-21 5X
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 BE2W2

Manual Integrations
 APPROVED

SOHIL
 11/20/2017 4:30:37 PM

Quant Time: Nov 20 06:16:16 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111617.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 20 06:14:09 2017
 Response via : Initial Calibration

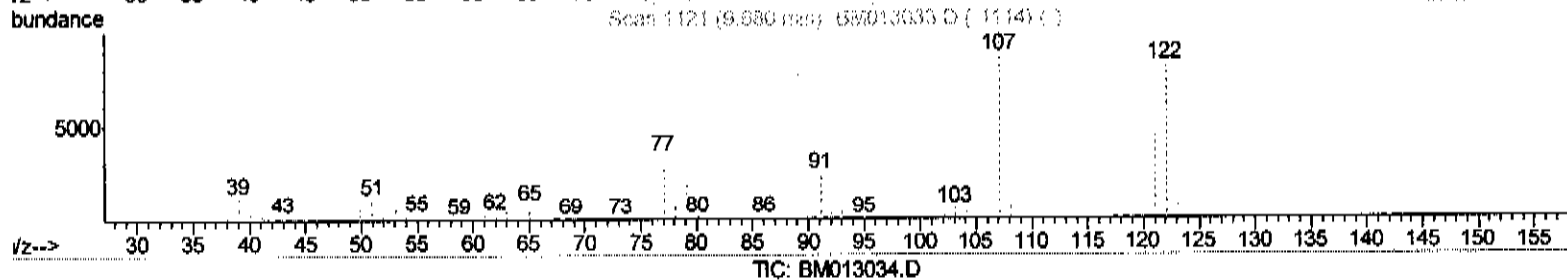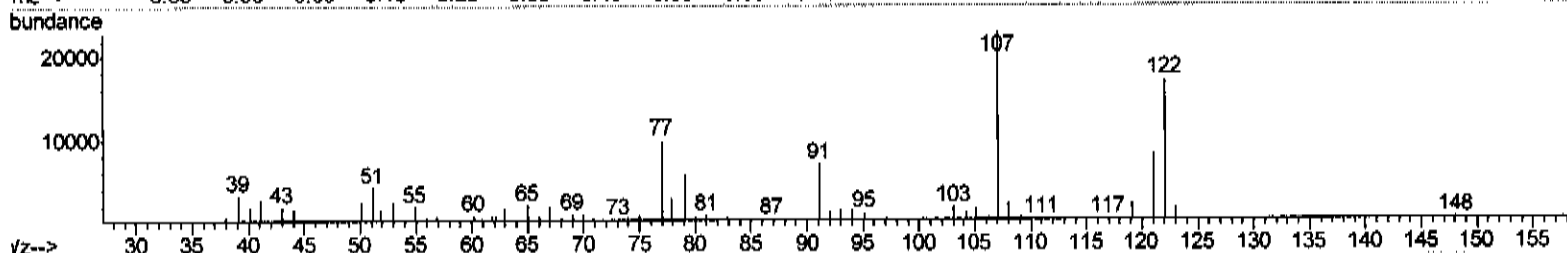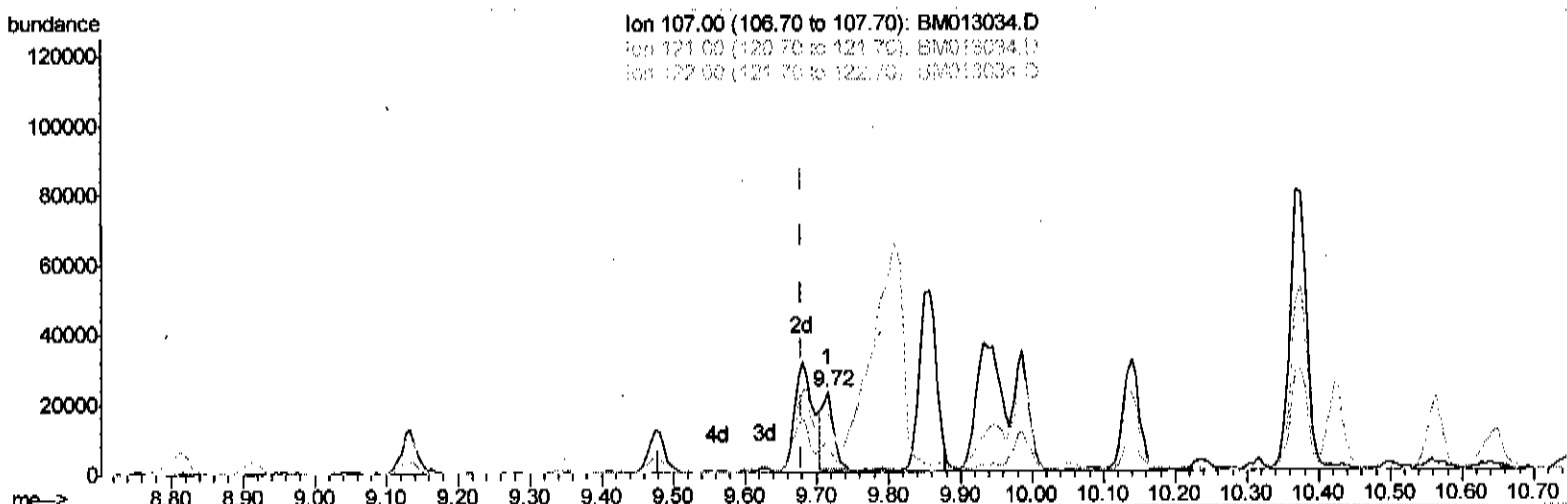

(24) 2,4-Dimethylphenol

9.716min (+0.035) 1.88ng/ul

response 22998

Ion	Exp%	Act%
107.00	100	100
121.00	39.90	36.53
122.00	72.20	74.58
0.00	0.00	0.00


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111717\
 Data File : BM013034.D
 Acq On : 18 Nov 2017 11:36
 Operator : SJ/JU
 Sample : I6405-21 5X
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
BE2W2

Manual Integrations
APPROVED

SOHIL
11/20/2017 4:30:37 PM

Quant Time: Nov 20 06:16:16 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111617.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 20 06:14:09 2017
 Response via : Initial Calibration

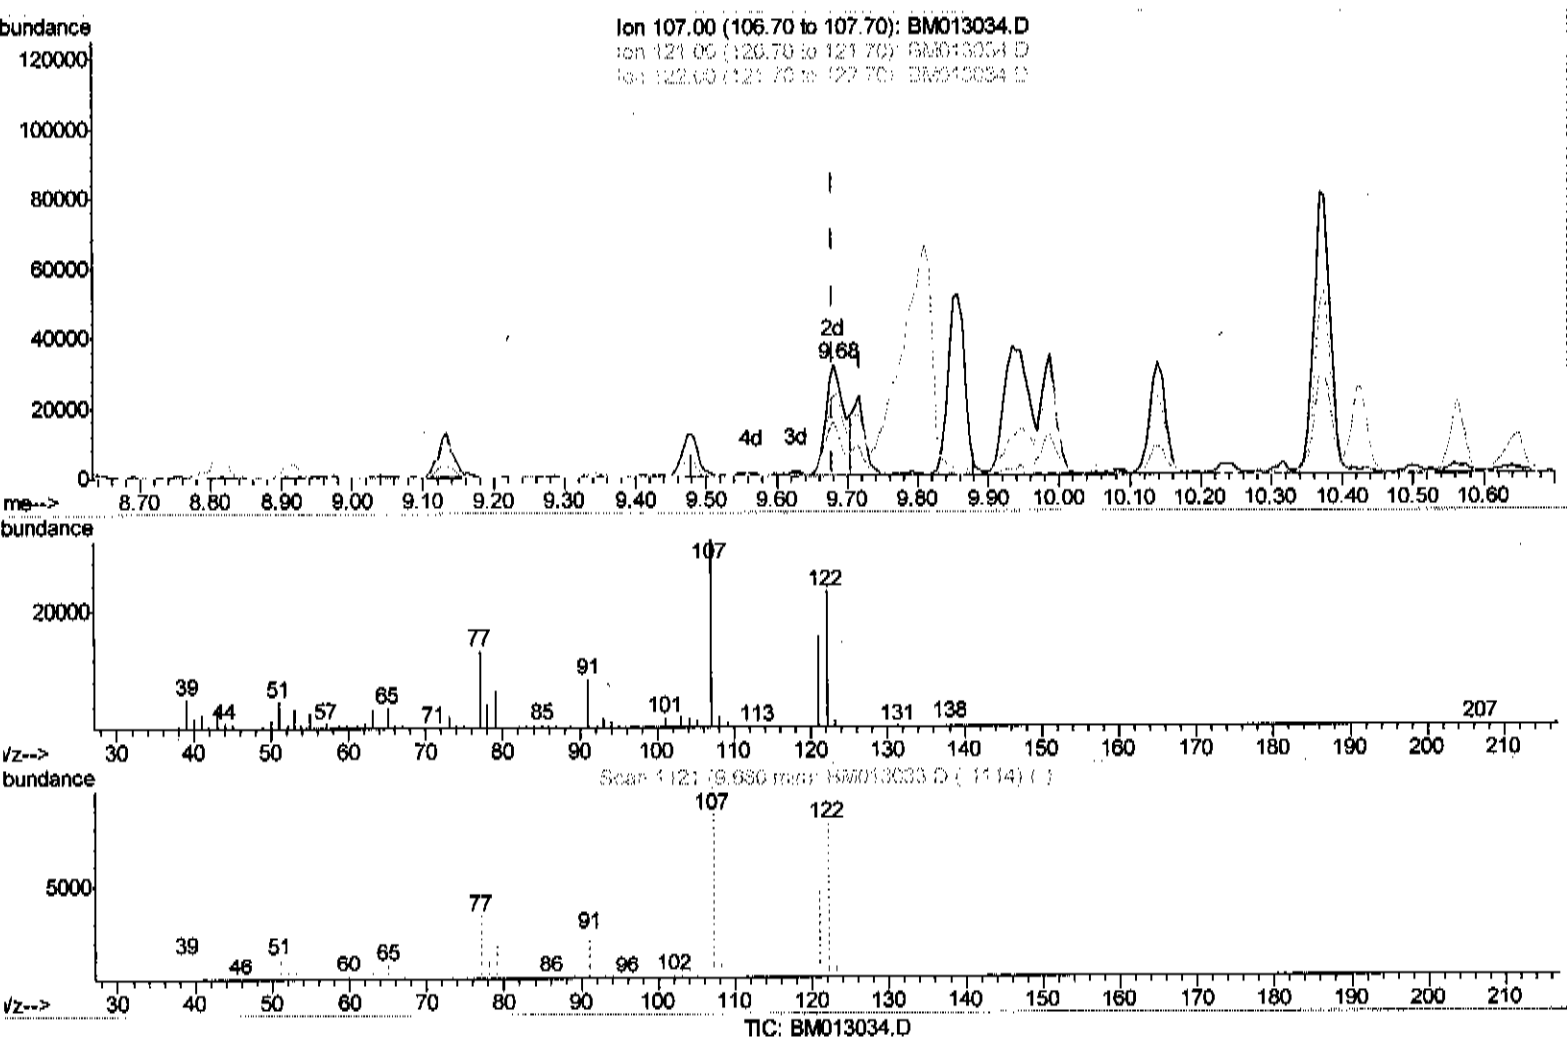

(24) 2,4-Dimethylphenol
 9.681min (+0.000) 4.80ng/ul mgy 11/20/17

response 58791

Ion	Exp%	Act%
107.00	100	100
121.00	39.90	48.55#
122.00	72.20	72.12
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111717\
 Data File : BM013034.D
 Acq On : 18 Nov 2017 11:36
 Operator : SJ/JU
 Sample : I6405-21 5X
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 BE2W2

Manual Integrations
 APPROVED

SOHIL
 11/20/2017 4:30:37 PM

Quant Time: Nov 20 06:39:03 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111617.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 20 06:14:09 2017
 Response via : Initial Calibration

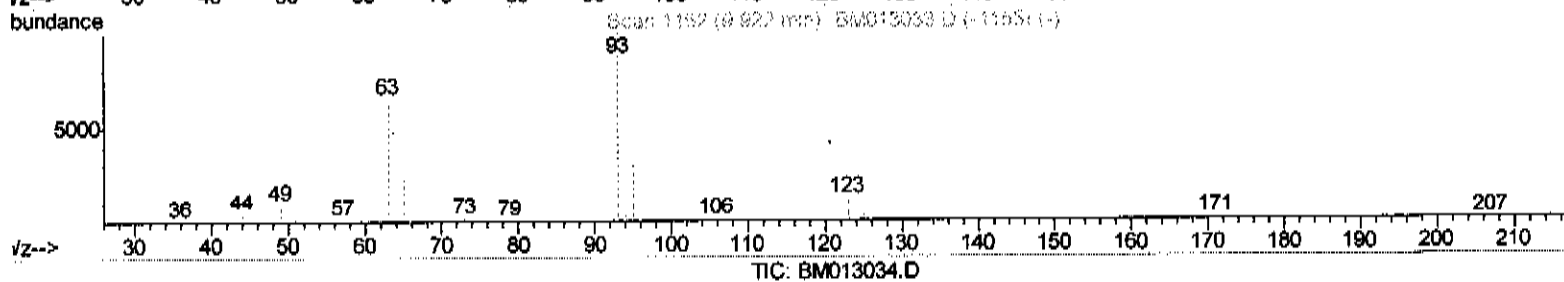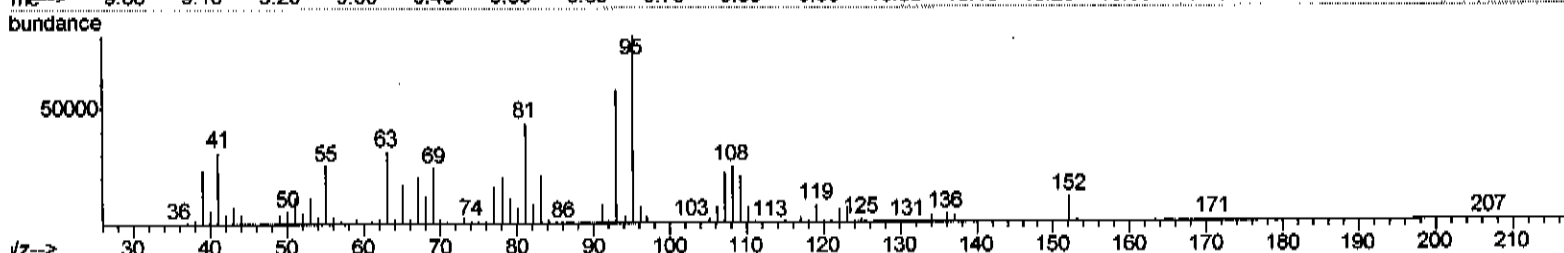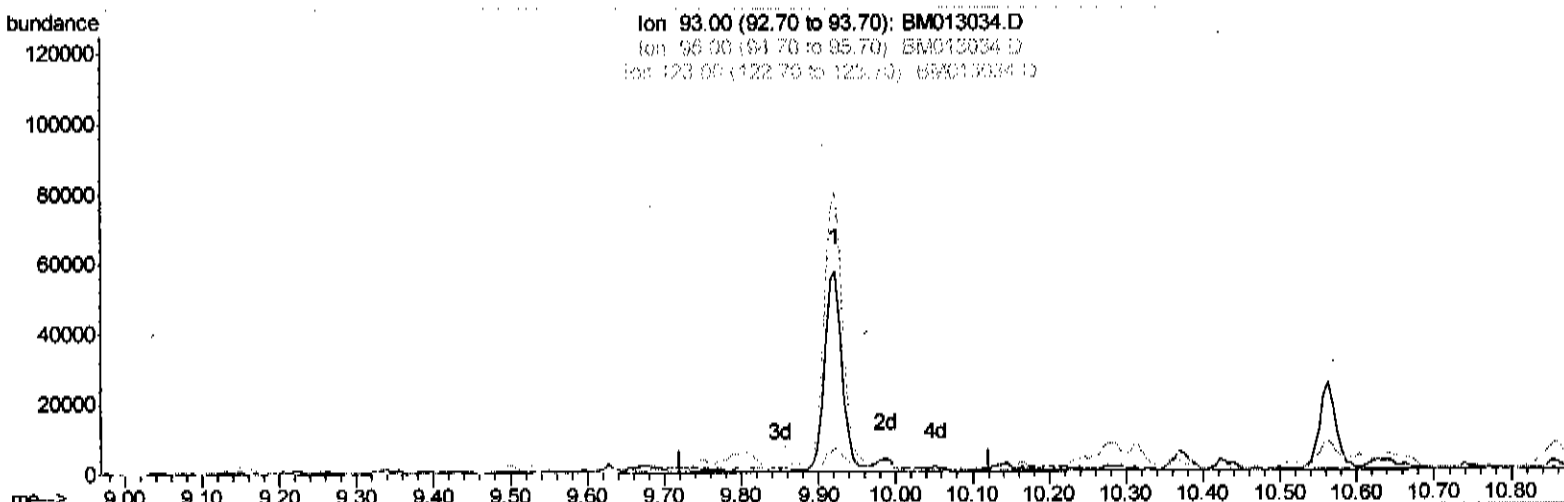

(25) Bis(2-Chloroethoxy)methane

9.922min (-9.922) 0.00ng/ul d

response 0

Ion	Exp%	Act%
93.00	100	0.00
95.00	35.60	0.00
123.00	11.10	0.00
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111717\
 Data File : BM013034.D
 Acq On : 18 Nov 2017 11:36
 Operator : SJ/JU
 Sample : I6405-21 5X
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 BE2W2

Manual Integrations
 APPROVED

SOHIL
 11/20/2017 4:30:37 PM

Quant Time: Nov 20 06:39:03 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111617.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 20 06:14:09 2017
 Response via : Initial Calibration

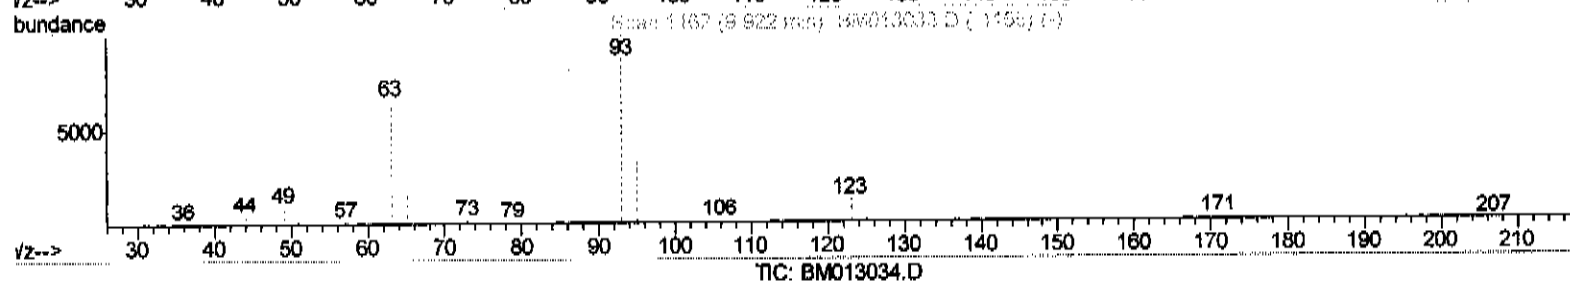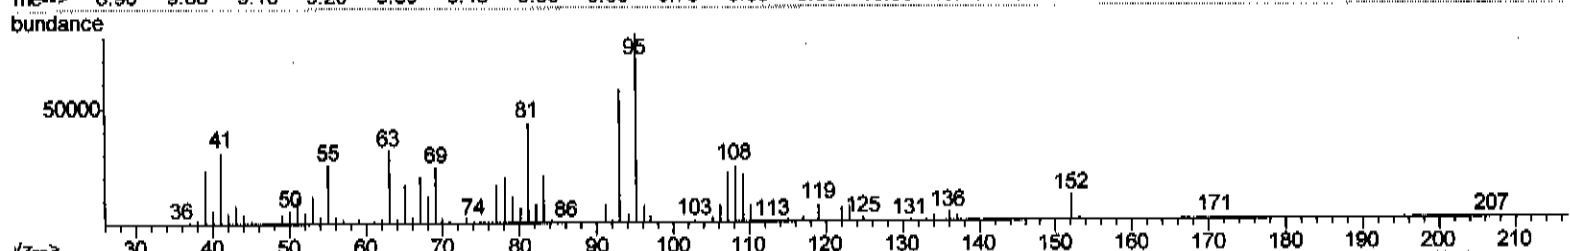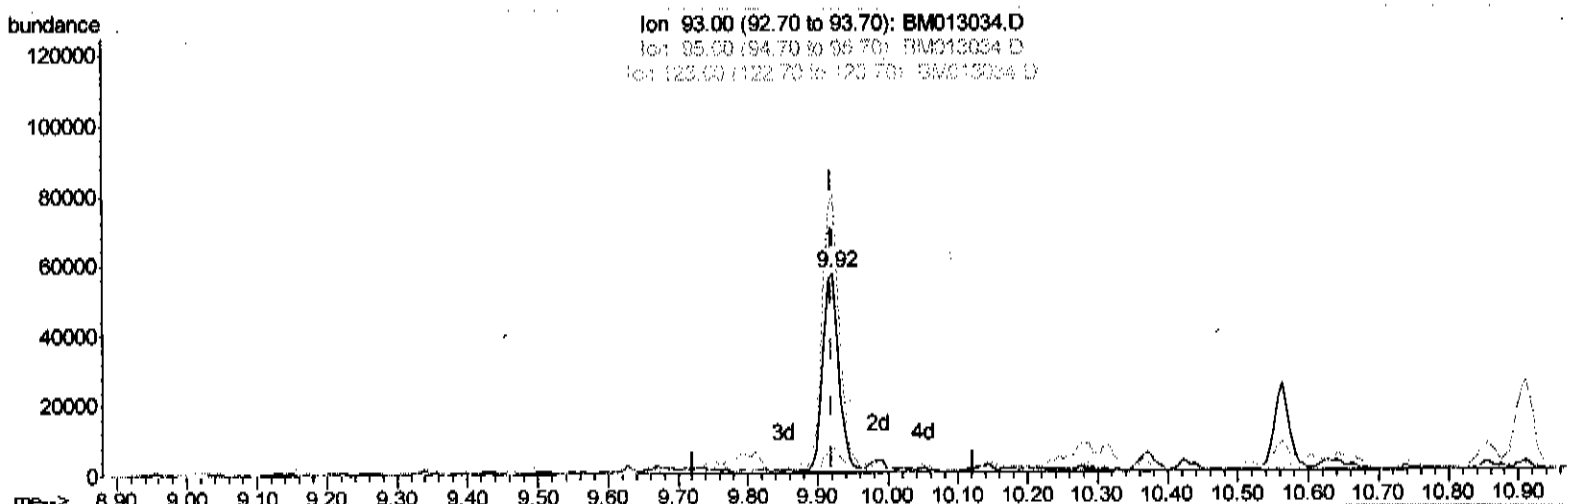

(25) Bis(2-Chloroethoxy)methane

9.922min (+0.000) 6.79ng/ul m

ju 11/21/17

response 89750

Ion	Exp%	Act%
93.00	100	100
95.00	35.60	140.88#
123.00	11.10	12.36
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111717\
Data File : BM013034.D
Acq On : 18 Nov 2017 11:36
Operator : SJ/JU
Sample : I6405-21 5X
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BE2W2

Manual Integrations
APPROVED
SOHIL
11/20/2017 4:30:37 PM

Quant Time: Nov 20 06:52:29 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111617.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Nov 20 06:14:09 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	153716	20.00	ng/ul	0.00
18) Naphthalene-d8	10.50	136	631589	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.36	164	382848	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.10	188	900415	20.00	ng/ul	0.00
75) Chrysene-d12	21.29	240	1062586	20.00	ng/ul	0.00
83) Perylene-d12	23.52	264	1064604	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.25	96	1310	0.39	ng/uL	0.00
5) Phenol-d5	6.89	99	18214	1.37	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.06	67	54675	7.24	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	59345	5.58	ng/ul	0.00
13) 4-Methylphenol-d8	8.42	113	37764	3.46	ng/ul	0.00
19) Nitrobenzene-d5	8.86	128	36436	8.09	ng/ul	0.00
22) 2-Nitrophenol-d4	9.59	143	37778	8.82	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.12	165	72737	6.69	ng/ul	0.00
29) 4-Chloroaniline-d4	10.62	131	1253	0.11	ng/ul	-0.01
43) Dimethylphthalate-d6	13.77	166	243041	7.24	ng/ul	0.00
46) Acenaphthylene-d8	14.05	160	292471	6.84	ng/ul	0.00
51) 4-Nitrophenol-d4	14.56	143	8576	1.68	ng/ul	0.01
57) Fluorene-d10	15.35	176	205958	7.22	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.46	200	29060	7.44	ng/ul	0.00
70) Anthracene-d10	17.20	188	335277	7.27	ng/ul	0.00
76) Pyrene-d10	19.49	212	384144	7.08	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.37	264	393862	7.30	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) 1,4-Dioxane	3.29	88	5567	1.53	ng/uL#	71
6) Phenol	6.92	94	91922	6.99	ng/ul#	85
8) Bis(2-Chloroethyl)ether	7.15	93	190139	19.22	ng/ul	97
10) 2-Chlorophenol	7.28	128	82576	7.84	ng/ul	99
11) 2-Methylphenol	8.16	108	52288	5.24	ng/ul	98
14) Acetophenone	8.53	105	69822	4.18	ng/ul#	76
16) 4-Methylphenol	8.48	108	264844	25.00	ng/ul	84
24) 2,4-Dimethylphenol	9.68	107	58791m}	4.80	ng/ul	} → 24 11/21/12
25) Bis(2-Chloroethoxy)methane	9.92	93	89750m}	6.79	ng/ul	
28) Naphthalene	10.55	128	188123	5.78	ng/ul	97
56) Diethylphthalate	15.19	149	93785	2.89	ng/ul	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed