

Data Path : Z:\HPCHEM1\BNA M\DATA\BM111717\
 Data File : BM013030.D
 Acq On : 18 Nov 2017 09:14
 Operator : SJ/JU
 Sample : I6405-03
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BE2S5

Quant Time: Nov 20 05:54:24 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM111617.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Nov 18 03:21:50 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	37703	20.00	ng/ul	0.00
18) Naphthalene-d8	10.50	136	58223	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.36	164	1821	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.10	188	392	20.00	ng/ul	0.00
75) Chrysene-d12	21.28	240	766	20.00	ng/ul	0.00
83) Perylene-d12	0.00	264	0	0.00	ng/ul	-23.52

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.25	96	4653	5.72	ng/uL	0.00
5) Phenol-d5	0.00	99	0	0.00	ng/ul	
7) Bis-(2-Chloroethyl)ether-d	0.00	67	0	0.00	ng/ul	
9) 2-Chlorophenol-d4	0.00	132	0	0.00	ng/ul	
13) 4-Methylphenol-d8	0.00	113	0	0.00	ng/ul	
19) Nitrobenzene-d5	0.00	128	0	0.00	ng/ul	
22) 2-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
26) 2,4-Dichlorophenol-d3	0.00	165	0	0.00	ng/ul	
29) 4-Chloroaniline-d4	0.00	131	0	0.00	ng/ul	
43) Dimethylphthalate-d6	0.00	166	0	0.00	ng/ul	
46) Acenaphthylene-d8	0.00	160	0	0.00	ng/ul	
51) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
57) Fluorene-d10	0.00	176	0	0.00	ng/ul	
62) 4,6-Dinitro-2-methylphenol	0.00	200	0	0.00	ng/ul	
70) Anthracene-d10	17.10	188	392	19.53	ng/ul	-0.09
76) Pyrene-d10	19.49	212	1028	26.27	ng/ul	0.00
87) Benzo(a)pyrene-d12	0.00	264	0	0.00	ng/ul	


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
56) Diethylphthalate	15.19	149	1395	9.033	ng/ul#	87




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM111717\
Data File : BM013030.D
Acq On : 18 Nov 2017 09:14
Operator : SJ/JU
Sample : I6405-03
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BE2S5

Quant Time: Nov 20 05:54:24 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM111617.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 18 03:21:50 2017
Response via : Initial Calibration

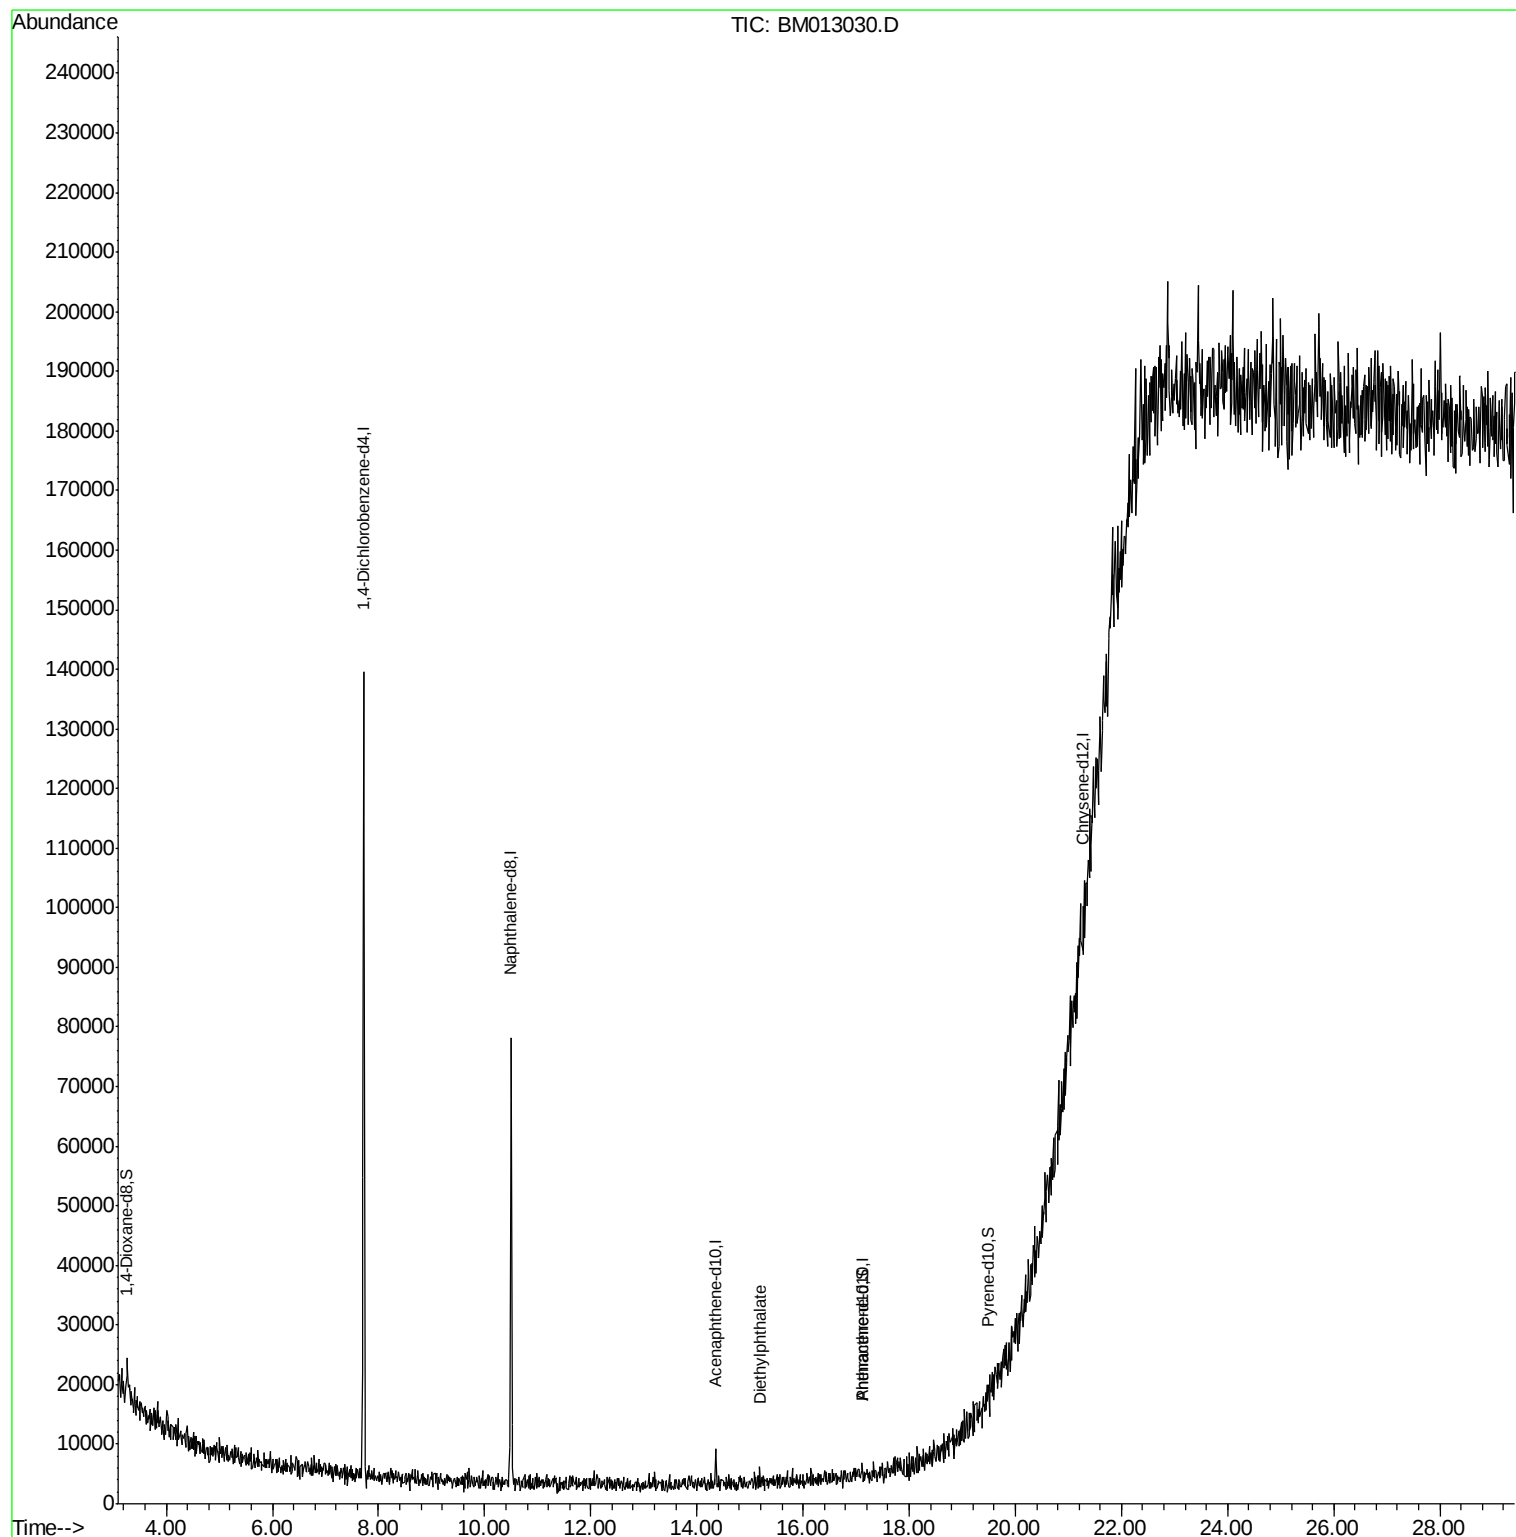

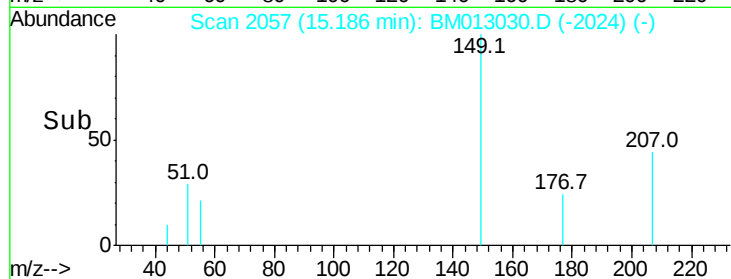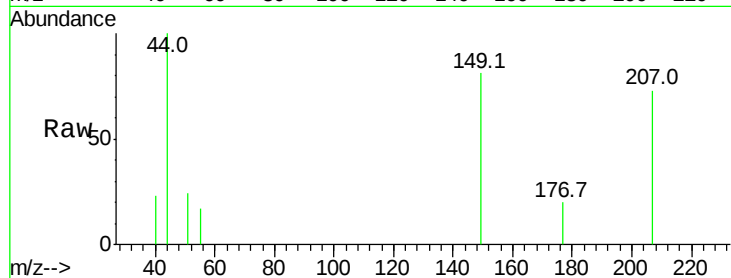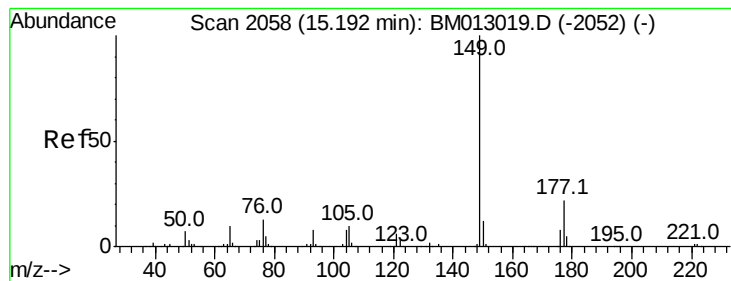

#56

Diethylphthalate

Concen: 9.033 ng/ul

RT: 15.19 min Scan# 2057

Delta R.T. -0.01 min

Lab File: BM013030.D

Acq: 18 Nov 2017 09:14

Instrument :

BNA_M

ClientSampleId :

BE2S5

Tot Ion:149 Resp: 1395

Ion Ratio Lower Upper

149 100

177 24.2 20.5 30.7

150 0.0 10.6 15.8#

