

Data Path : Z:\HPCHEM1\BNA M\DATA\BM111717\
 Data File : BM013006.D
 Acq On : 17 Nov 2017 19:04
 Operator : SJ/JU
 Sample : I6451-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BE2W7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111617.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	24	28	34	rVB	50446	62211	1.33%	0.135%
2	6.887	640	646	656	rBV	223447	346337	7.41%	0.752%
3	7.063	669	676	686	rBV	753461	1149379	24.60%	2.495%
4	7.251	702	708	718	rVB	835826	1295537	27.73%	2.812%
5	7.722	781	788	798	rBV	729620	1141492	24.43%	2.478%
6	8.422	898	907	914	rBV	640457	1008243	21.58%	2.189%
7	8.869	975	983	991	rBV	989254	1663699	35.61%	3.612%
8	9.587	1098	1105	1113	rBV	817844	1302232	27.88%	2.827%
9	10.122	1189	1196	1203	rBV	1220780	1976655	42.31%	4.291%
10	10.504	1253	1261	1268	rBV	937879	1553209	33.25%	3.372%
11	13.775	1811	1817	1828	rBV	2234134	3029885	64.86%	6.577%
12	14.051	1855	1864	1871	rBV	2551021	3677491	78.72%	7.983%
13	14.363	1910	1917	1924	rBV2	1275247	1995135	42.71%	4.331%
14	14.551	1942	1949	1955	rBV	171019	247297	5.29%	0.537%
15	15.357	2078	2086	2093	rBV	3060885	4331153	92.71%	9.402%
16	15.469	2098	2105	2114	rBV	765813	1041160	22.29%	2.260%
17	15.592	2122	2126	2136	rVB6	35322	60772	1.30%	0.132%
18	16.027	2193	2200	2206	rBV2	36951	56153	1.20%	0.122%
19	17.104	2377	2383	2391	rVB2	1577042	2208159	47.27%	4.794%
20	17.204	2393	2400	2410	rVV2	3238543	4458595	95.44%	9.679%
21	19.298	2751	2756	2760	rBV3	37451	46962	1.01%	0.102%
22	19.498	2784	2790	2797	rBV	3490189	4671674	100.00%	10.142%
23	21.286	3089	3094	3100	rBV	1784018	2261750	48.41%	4.910%
24	23.380	3443	3450	3459	rBV	2444008	4355236	93.23%	9.455%
25	23.521	3467	3474	3484	rVB	1079191	2124414	45.47%	4.612%


Sum of corrected areas: 46064830

Data Path : Z:\HPCHEM1\BNA M\DATA\BM111717\
Data File : BM013006.D
Acq On : 17 Nov 2017 19:04
Operator : SJ/JU
Sample : I6451-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BE2W7

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM111617.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

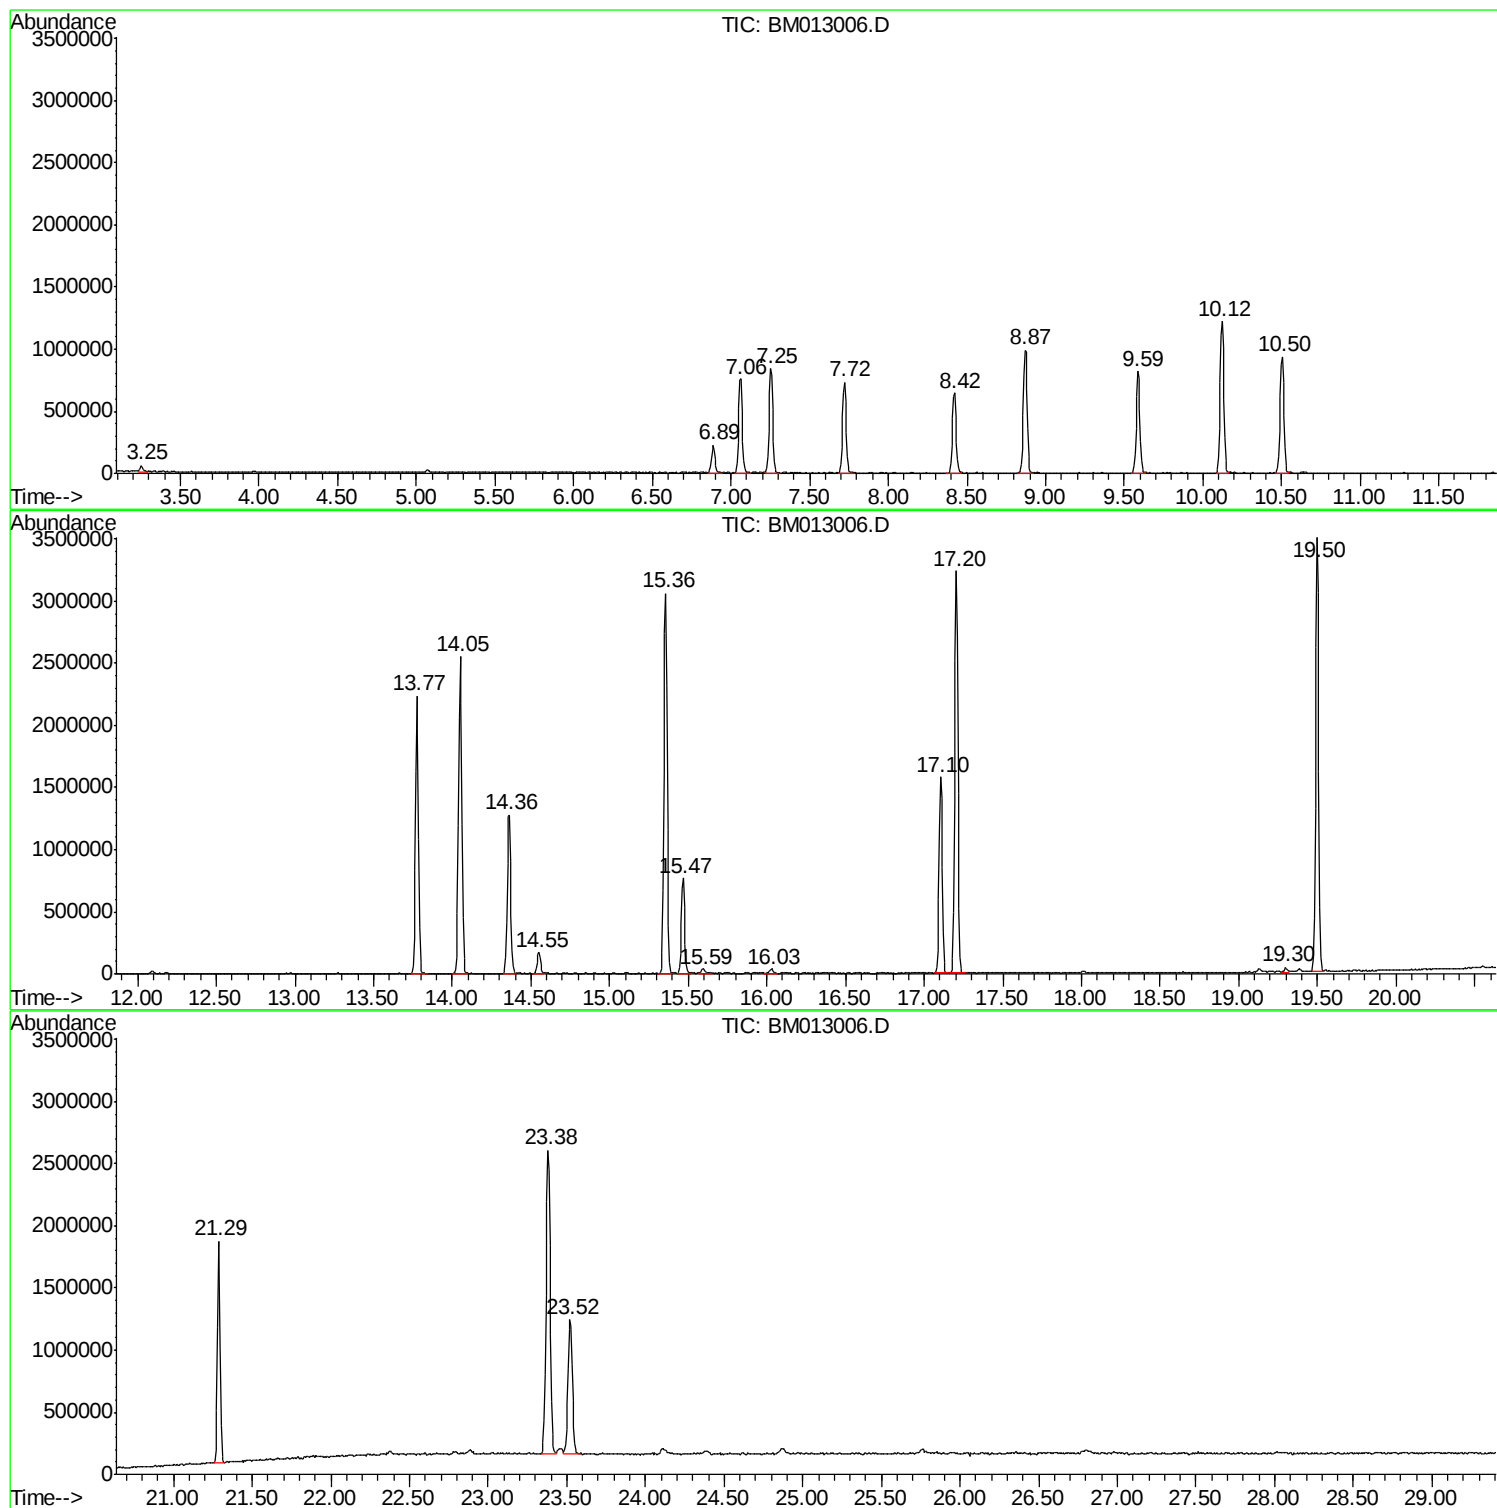

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111717\
Data File : BM013006.D
Acq On : 17 Nov 2017 19:04
Operator : SJ/JU
Sample : I6451-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BE2W7

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111617.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM111717\
Data File : BM013006.D
Acq On : 17 Nov 2017 19:04
Operator : SJ/JU
Sample : I6451-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BE2W7

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111617.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc