

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
 Data File : BM037519.D
 Acq On : 17 Nov 2022 10:21
 Operator : CG/JU
 Sample : PB149091BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Nov 17 12:15:15 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 17 00:46:50 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.145	152	5919	0.400	ng/ul	0.00
4) Naphthalene-d8	10.968	136	17346	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.766	164	11147	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.496	188	23375	0.400	ng/ul	0.00
17) Chrysene-d12	21.657	240	16588	0.400	ng/ul	0.00
23) Perylene-d12	24.156	264	19231	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.453	96	41352	6.009	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.541	152	8435	0.293	ng/ul	0.00
18) Fluoranthene-d10	19.509	212	18347	0.335	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.871	202	3591	0.043	ng/ul#	1
26) Benzo(a)pyrene	23.998	252	8072	0.106	ng/ul#	70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
Data File : BM037519.D
Acq On : 17 Nov 2022 10:21
Operator : CG/JU
Sample : PB149091BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Nov 17 12:15:15 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 17 00:46:50 2022
Response via : Initial Calibration




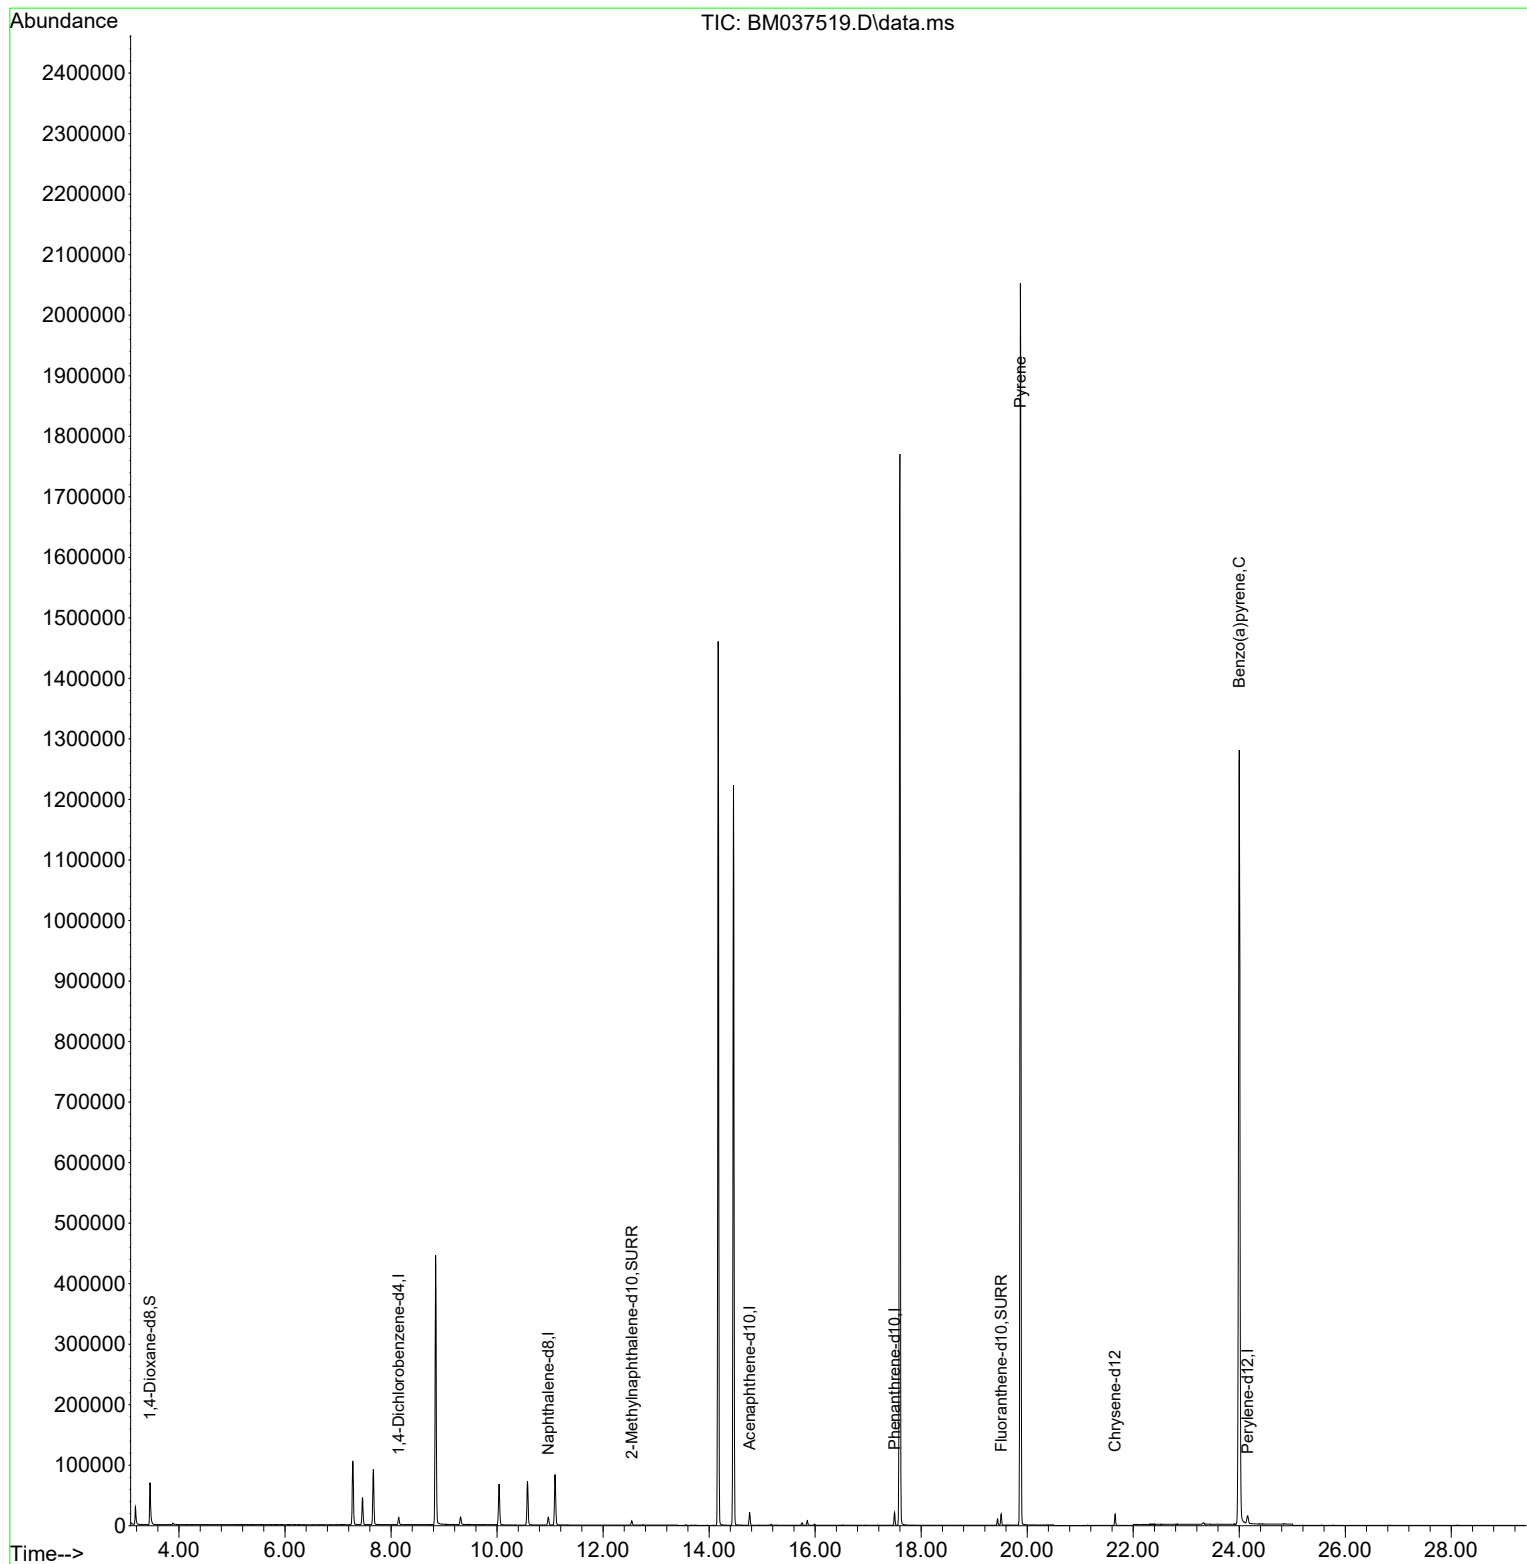


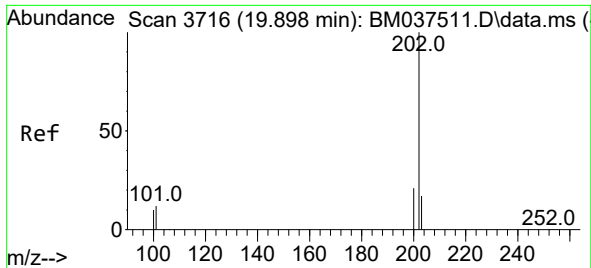

#20
Pyrene
Concen: 0.043 ng/ul
RT: 19.871 min Scan# 31
Delta R.T. -0.027 min
Lab File: BM037519.D
Acq: 17 Nov 2022 10:21

Instrument :
BNA_M
ClientSampleId :

Tgt Ion:202 Resp: 3591
Ion Ratio Lower Upper
202 100
101 159.9 10.1 15.1#
100 1256.4 8.0 12.0#

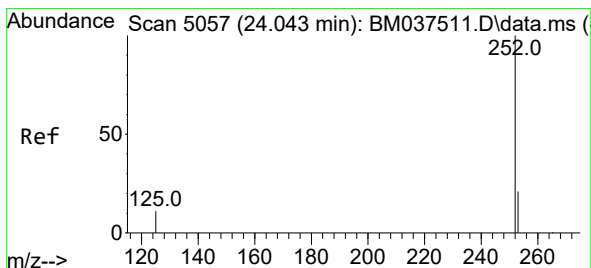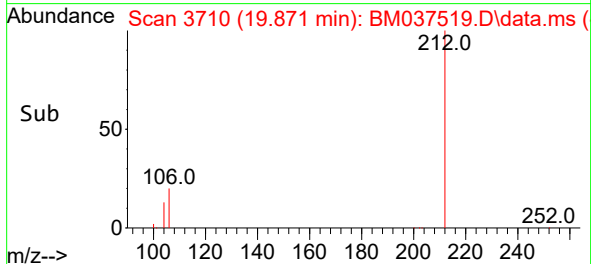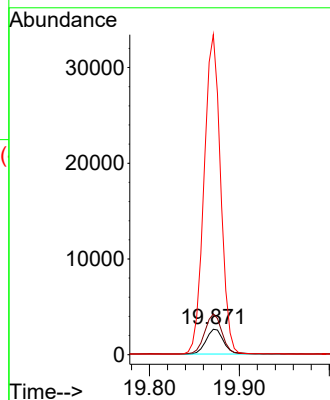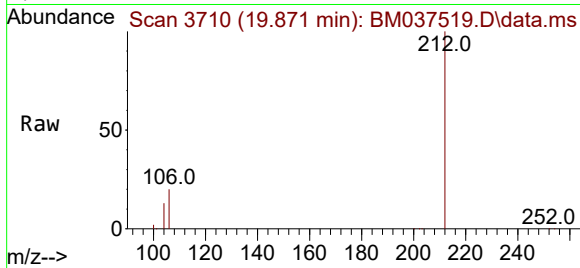

#26
Benzo(a)pyrene
Concen: 0.106 ng/ul
RT: 23.998 min Scan# 5042
Delta R.T. -0.045 min
Lab File: BM037519.D
Acq: 17 Nov 2022 10:21

Tgt Ion:252 Resp: 8072
Ion Ratio Lower Upper
252 100
253 35.4 18.8 28.2#
125 29.3 10.5 15.7#

