

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
 Data File : BM037553.D
 Acq On : 18 Nov 2022 08:08
 Operator : CG/JU
 Sample : PB149135BL
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Nov 18 23:12:07 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 18 06:51:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.136	152	6342	0.400	ng/ul	0.00
4) Naphthalene-d8	10.958	136	18229	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.756	164	11229	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.486	188	23686	0.400	ng/ul	0.00
17) Chrysene-d12	21.646	240	16473	0.400	ng/ul #	0.00
23) Perylene-d12	24.139	264	19375	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.449	96	48185	6.535	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.530	152	9315	0.308	ng/ul	0.00
18) Fluoranthene-d10	19.498	212	21050	0.387	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.866	202	4173	0.050	ng/ul#	1
26) Benzo(a)pyrene	23.982	252	9325	0.121	ng/ul#	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
Data File : BM037553.D
Acq On : 18 Nov 2022 08:08
Operator : CG/JU
Sample : PB149135BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Nov 18 23:12:07 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 18 06:51:41 2022
Response via : Initial Calibration




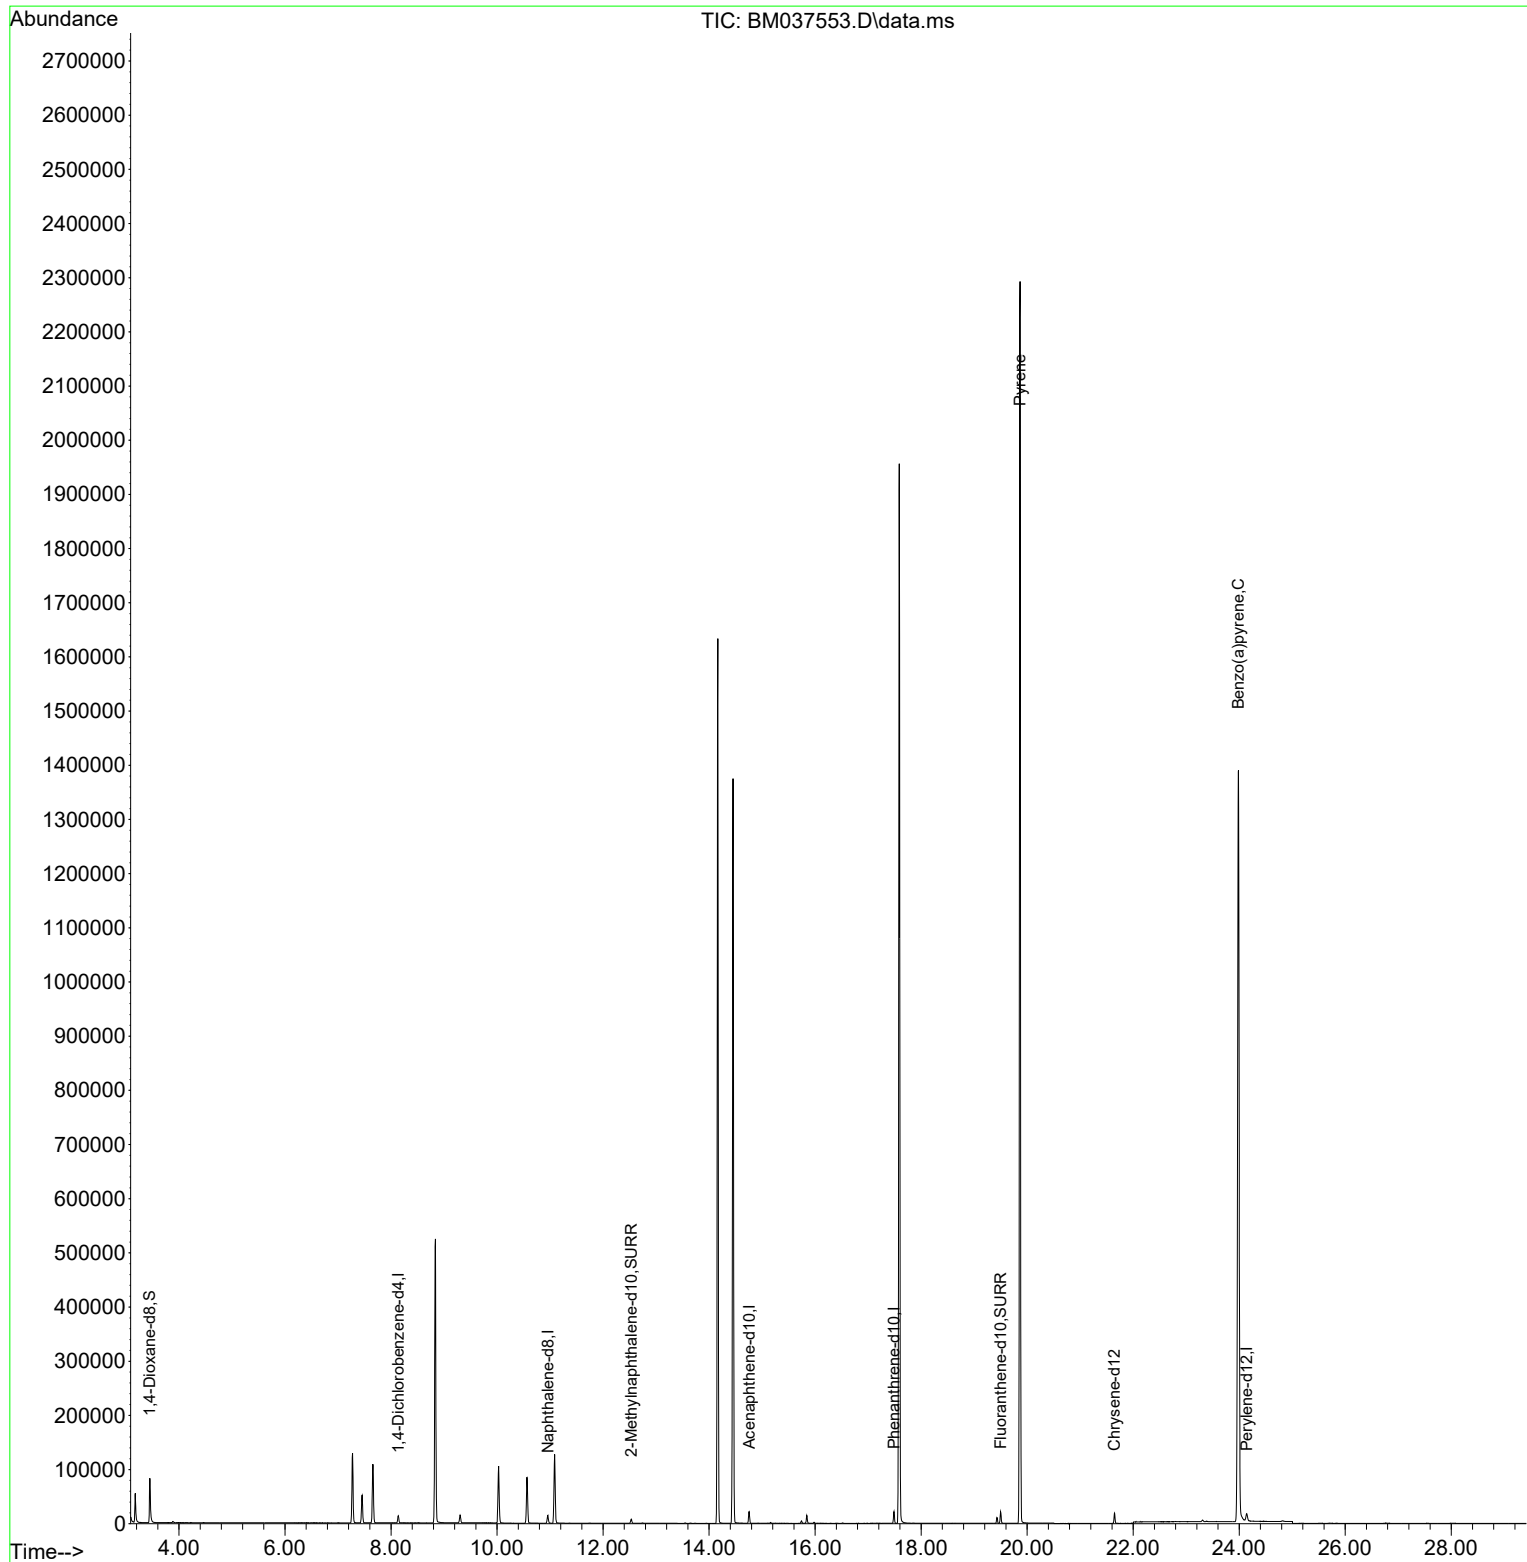


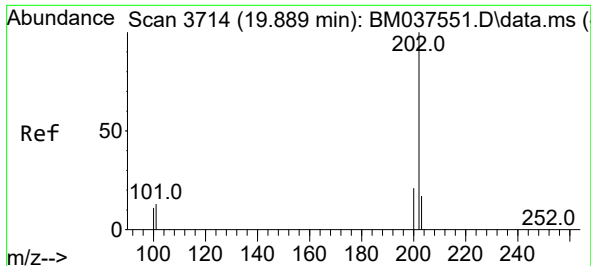

#20
Pyrene
Concen: 0.050 ng/ul
RT: 19.866 min Scan# 31
Delta R.T. -0.023 min
Lab File: BM037553.D
Acq: 18 Nov 2022 08:08

Instrument :
BNA_M
ClientSampleId :

Tgt Ion:202 Resp: 4173
Ion Ratio Lower Upper
202 100
101 152.0 10.1 15.1#
100 1135.8 8.0 12.0#

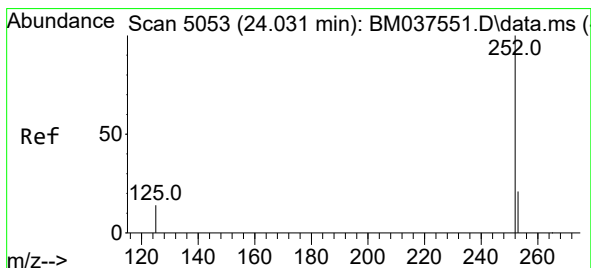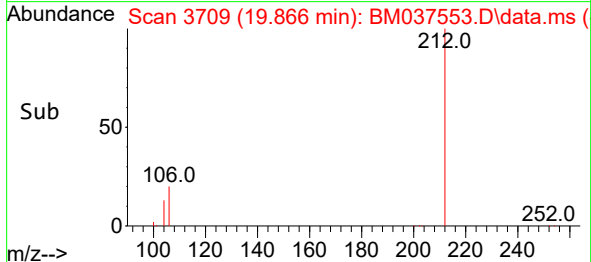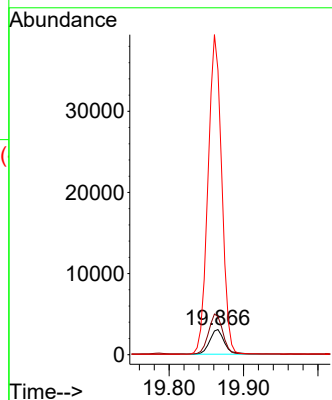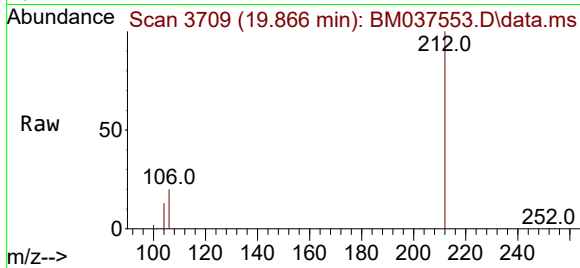

#26
Benzo(a)pyrene
Concen: 0.121 ng/ul
RT: 23.982 min Scan# 5036
Delta R.T. -0.047 min
Lab File: BM037553.D
Acq: 18 Nov 2022 08:08

Tgt Ion:252 Resp: 9325
Ion Ratio Lower Upper
252 100
253 37.5 18.8 28.2#
125 31.6 10.5 15.7#

