

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
 Data File : BM037567.D
 Acq On : 18 Nov 2022 16:40
 Operator : CG/JU
 Sample : PB149000BL
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Nov 18 23:13:58 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 18 06:51:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.136	152	6359	0.400	ng/ul	0.00
4) Naphthalene-d8	10.957	136	18773	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.756	164	12112	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.491	188	25823	0.400	ng/ul	0.00
17) Chrysene-d12	21.648	240	18644	0.400	ng/ul	0.00
23) Perylene-d12	24.144	264	21574	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.453	96	47015	6.359	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.536	152	9577	0.308	ng/ul	0.00
18) Fluoranthene-d10	19.499	212	21775	0.353	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.866	202	4331	0.046	ng/ul#	1
26) Benzo(a)pyrene	23.986	252	9729	0.114	ng/ul#	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
Data File : BM037567.D
Acq On : 18 Nov 2022 16:40
Operator : CG/JU
Sample : PB149000BL
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Nov 18 23:13:58 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 18 06:51:41 2022
Response via : Initial Calibration




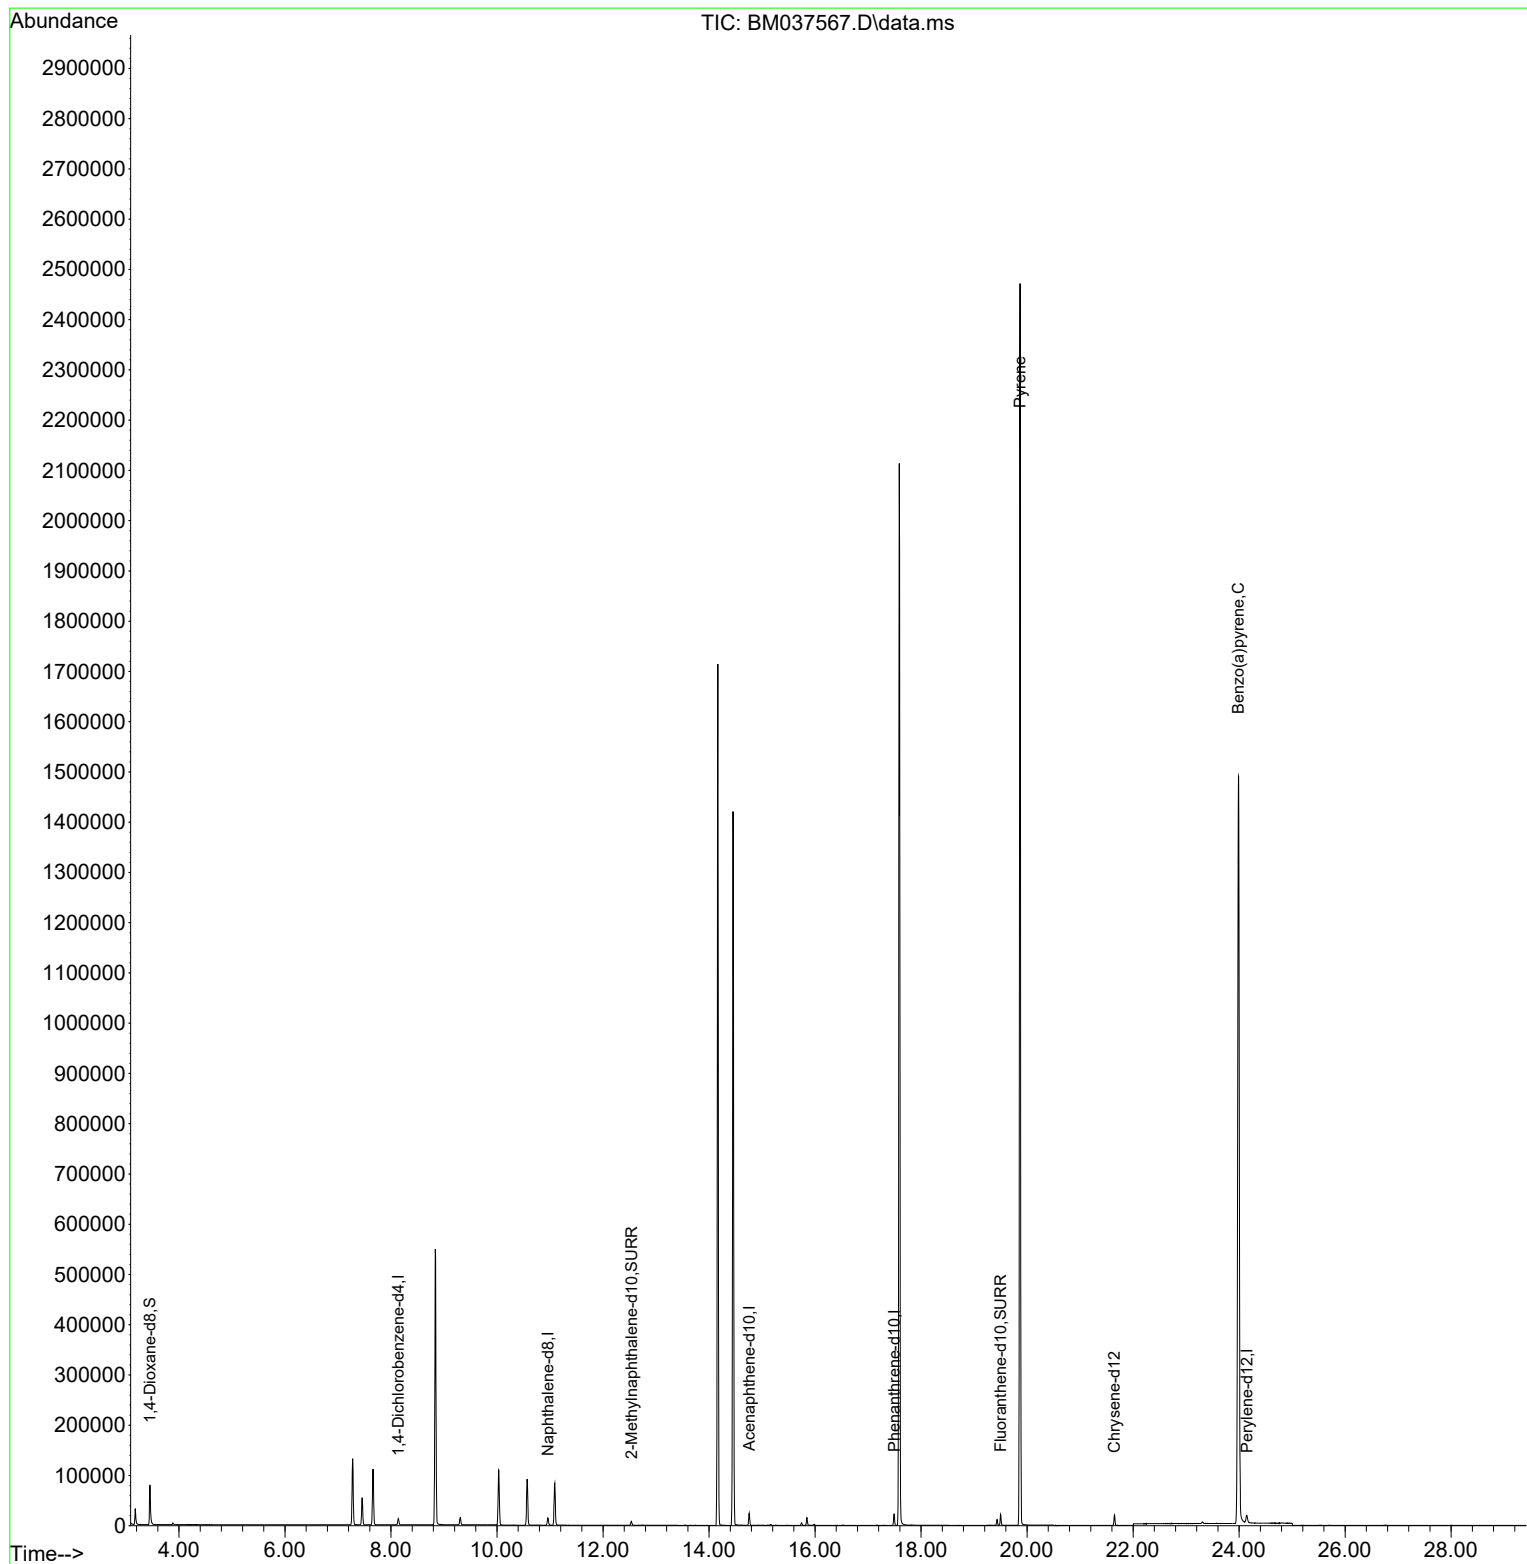


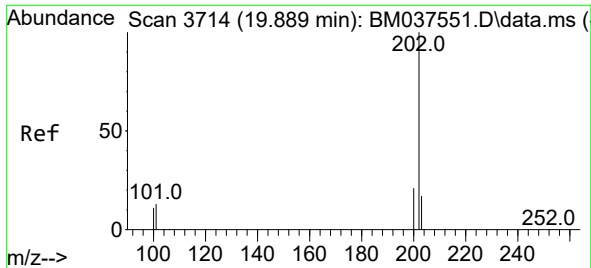

#20
Pyrene
Concen: 0.046 ng/ul
RT: 19.866 min Scan# 3714
Delta R.T. -0.022 min
Lab File: BM037567.D
Acq: 18 Nov 2022 16:40

Instrument :
BNA_M
ClientSampleId :

Tgt Ion:202 Resp: 4331
Ion Ratio Lower Upper
202 100
101 158.7 10.1 15.1#
100 1201.6 8.0 12.0#

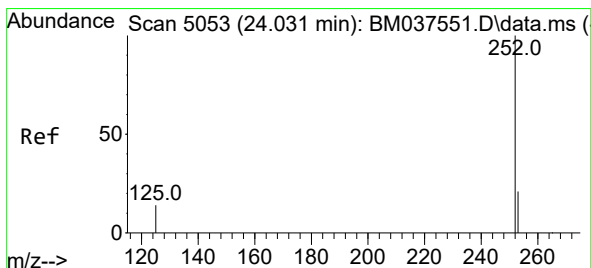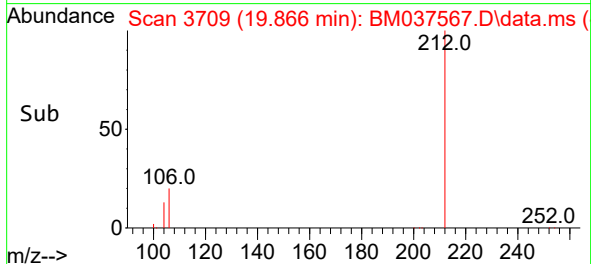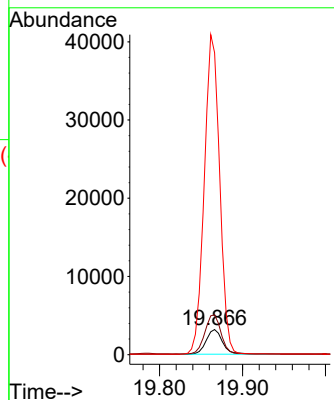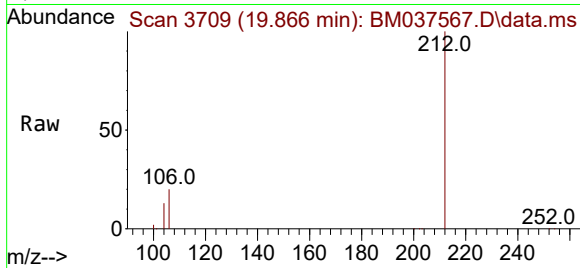

#26
Benzo(a)pyrene
Concen: 0.114 ng/ul
RT: 23.986 min Scan# 5038
Delta R.T. -0.042 min
Lab File: BM037567.D
Acq: 18 Nov 2022 16:40

Tgt Ion:252 Resp: 9729
Ion Ratio Lower Upper
252 100
253 38.3 18.8 28.2#
125 32.8 10.5 15.7#

