

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
 Data File : BM037570.D
 Acq On : 18 Nov 2022 19:08
 Operator : CG/JU
 Sample : PB149149BL
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Nov 18 23:14:21 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 18 06:51:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.136	152	5836	0.400	ng/ul	0.00
4) Naphthalene-d8	10.957	136	17531	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.756	164	11203	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.491	188	23391	0.400	ng/ul	0.00
17) Chrysene-d12	21.648	240	16883	0.400	ng/ul	# 0.00
23) Perylene-d12	24.144	264	19779	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.453	96	51606	7.606	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.536	152	9952	0.342	ng/ul	0.00
18) Fluoranthene-d10	19.499	212	21784	0.390	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.746	166	4261	0.081	ng/ul#	13
20) Pyrene	19.866	202	4288	0.051	ng/ul#	1
26) Benzo(a)pyrene	23.986	252	9696	0.124	ng/ul#	61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
Data File : BM037570.D
Acq On : 18 Nov 2022 19:08
Operator : CG/JU
Sample : PB149149BL
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :


Quant Time: Nov 18 23:14:21 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 18 06:51:41 2022
Response via : Initial Calibration

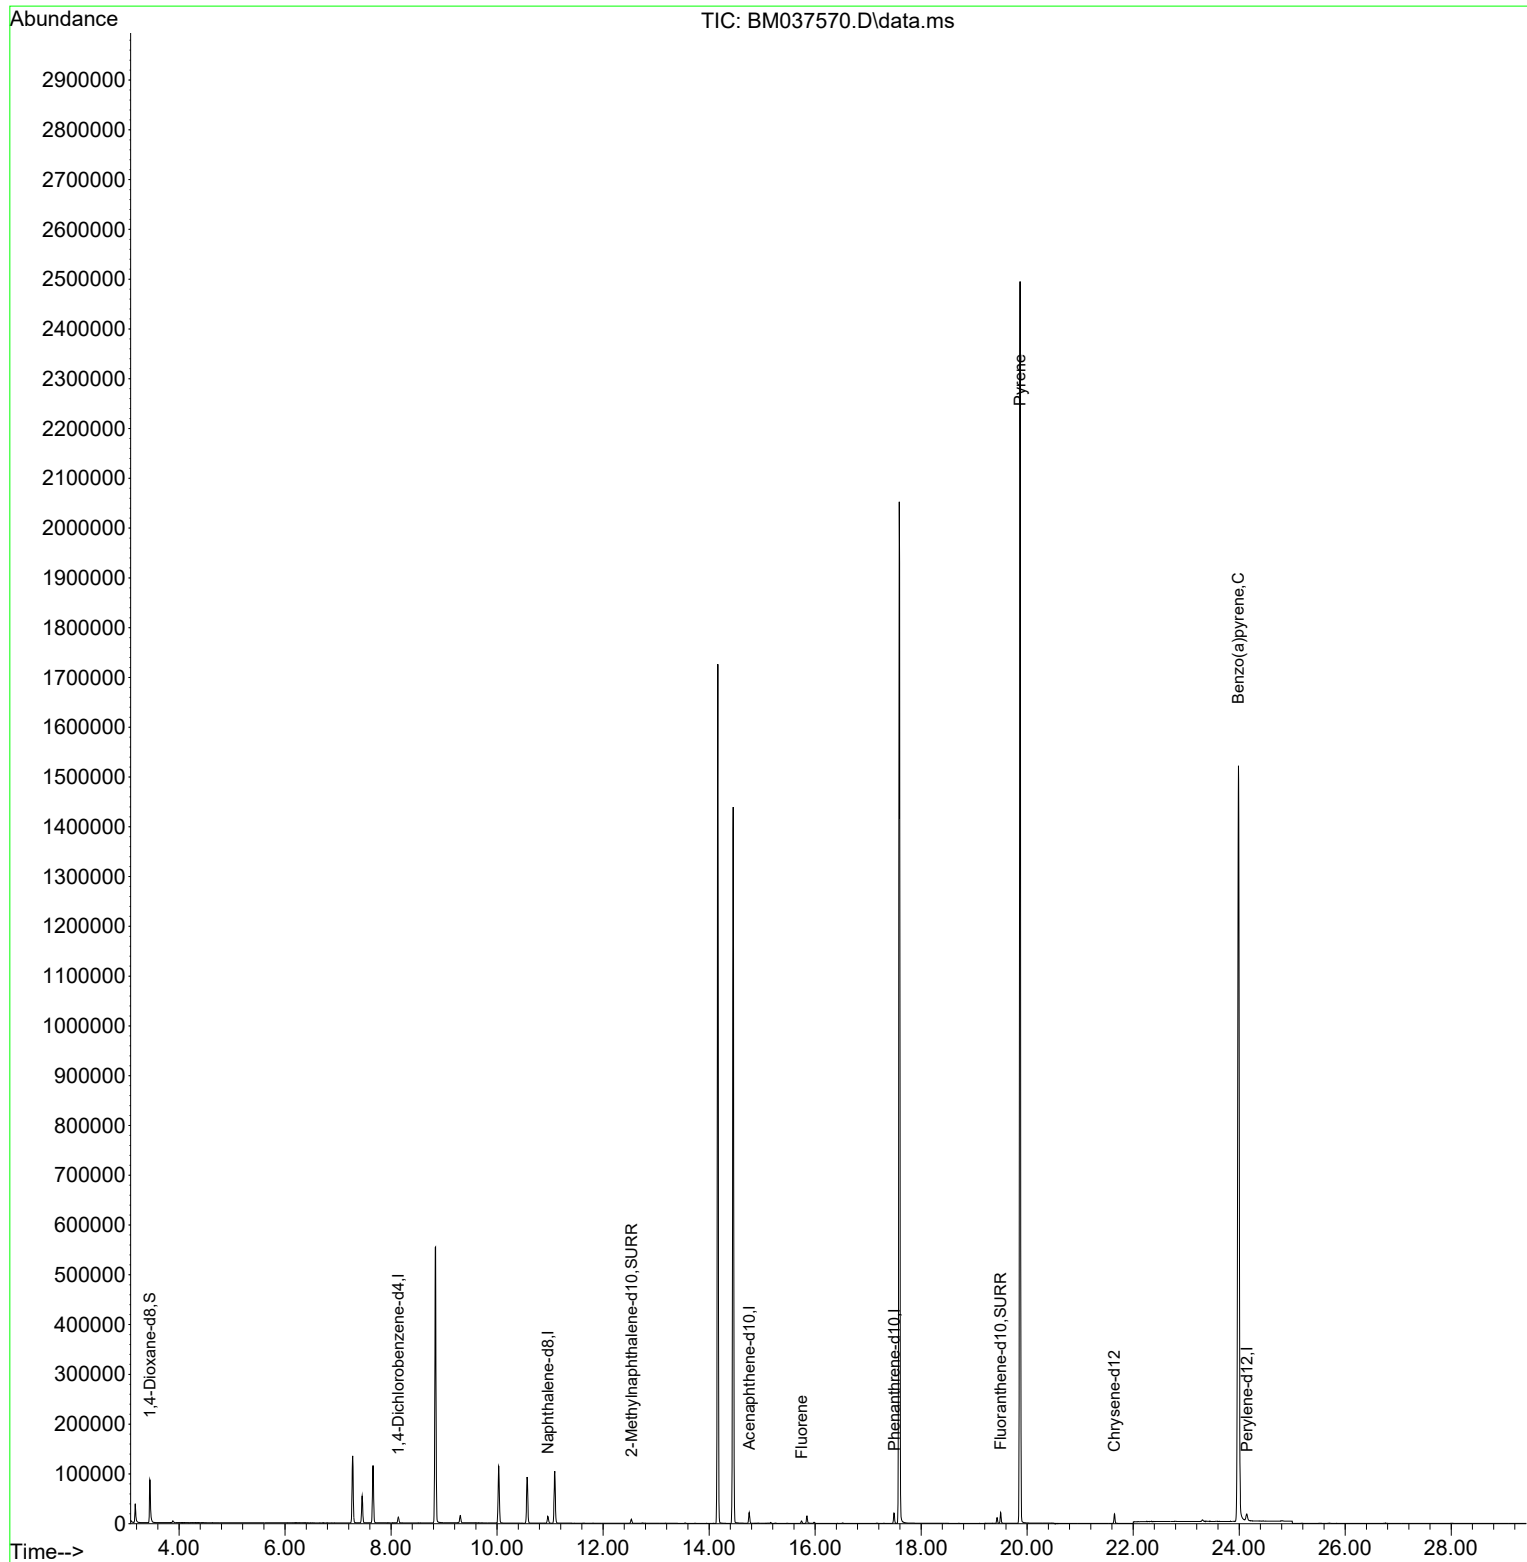



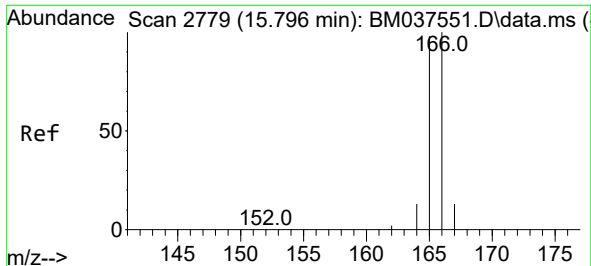


#12
Fluorene
Concen: 0.081 ng/ul
RT: 15.746 min Scan# 21
Delta R.T. -0.050 min
Lab File: BM037570.D
Acq: 18 Nov 2022 19:08

Instrument :
BNA_M
ClientSampleId :



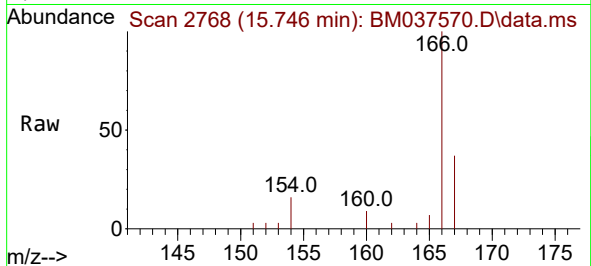



Tgt Ion:166 Resp: 4261
Ion Ratio Lower Upper
166 100
165 7.2 78.7 118.1#
167 36.8 11.3 16.9#

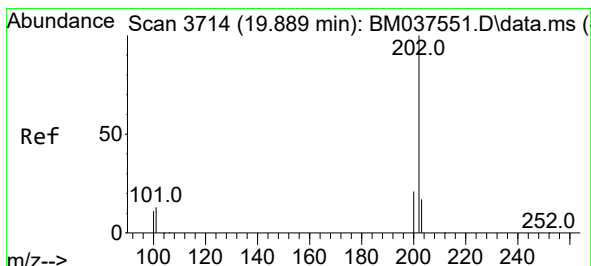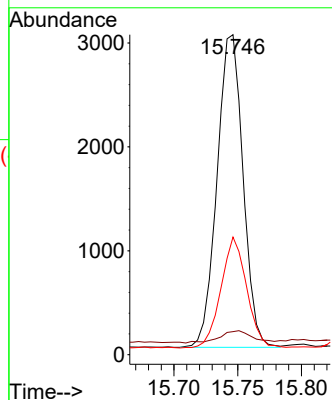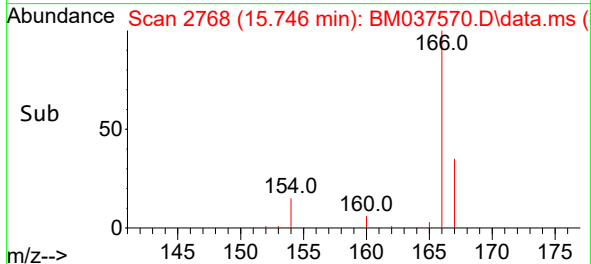

#20
Pyrene
Concen: 0.051 ng/ul
RT: 19.866 min Scan# 3709
Delta R.T. -0.022 min
Lab File: BM037570.D
Acq: 18 Nov 2022 19:08


Tgt Ion:202 Resp: 4288
Ion Ratio Lower Upper
202 100
101 156.4 10.1 15.1#
100 1187.8 8.0 12.0#

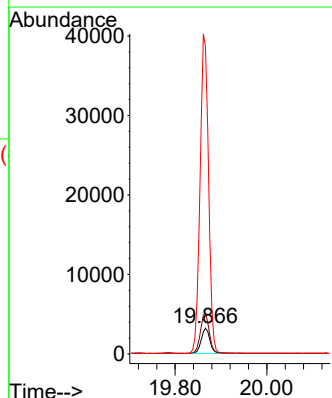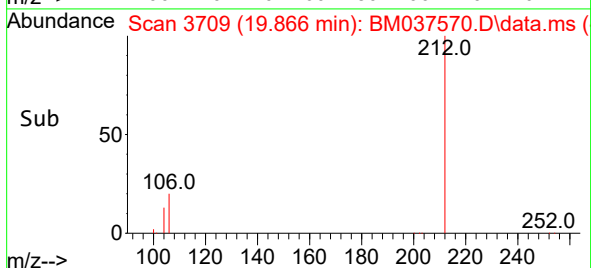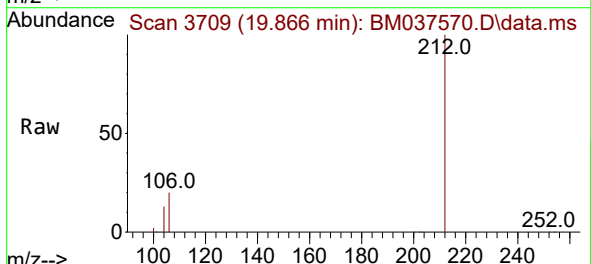

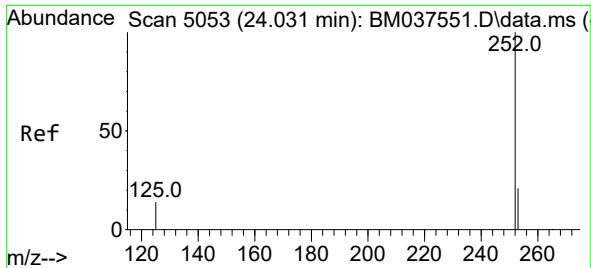

#26
Benzo(a)pyrene
Concen: 0.124 ng/ul
RT: 23.986 min Scan# 50
Delta R.T. -0.042 min
Lab File: BM037570.D
Acq: 18 Nov 2022 19:08

Instrument :
BNA_M
ClientSampleId :

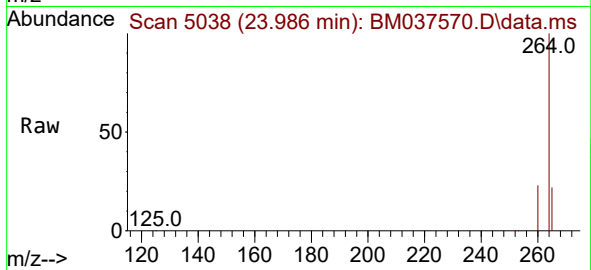

Tgt Ion:252 Resp: 9696
Ion Ratio Lower Upper
252 100
253 39.0 18.8 28.2#
125 34.2 10.5 15.7#

