




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
Data File : BM037576.D
Acq On : 18 Nov 2022 22:49
Operator : CG/JU
Sample : N5689-01
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGCC4

Manual IntegrationsAPPROVED

Quant Time: Nov 18 23:43:25 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 18 06:51:41 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/21/2022
Supervised By :mohammad ahmed 11/21/2022

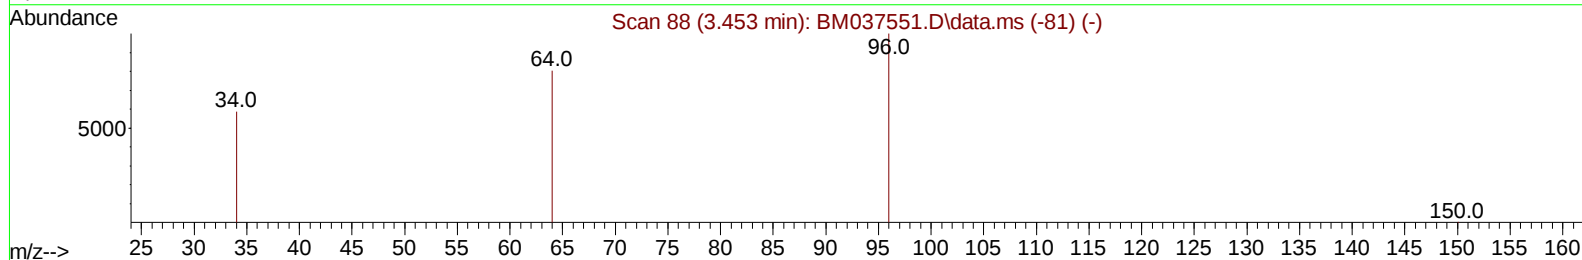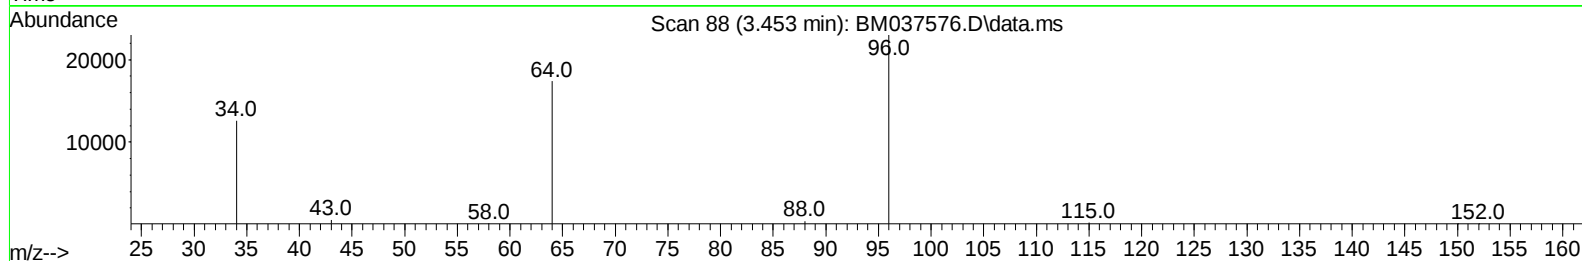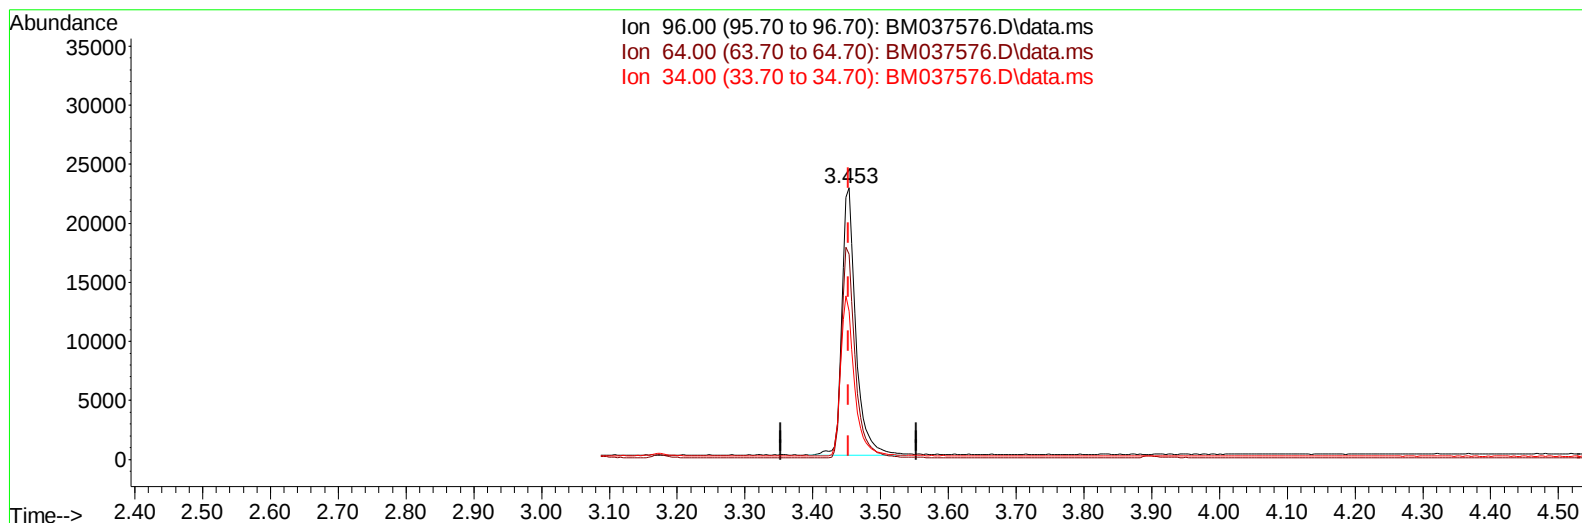

TIC: BM037576.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.453min (-0.000) 3.99 ng/u1

response 32204

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	67.60	75.51
34.00	42.40	54.58#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
Data File : BM037576.D
Acq On : 18 Nov 2022 22:49
Operator : CG/JU
Sample : N5689-01
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGCC4

Manual IntegrationsAPPROVED

Quant Time: Nov 18 23:43:25 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 18 06:51:41 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/21/2022
Supervised By :mohammad ahmed 11/21/2022

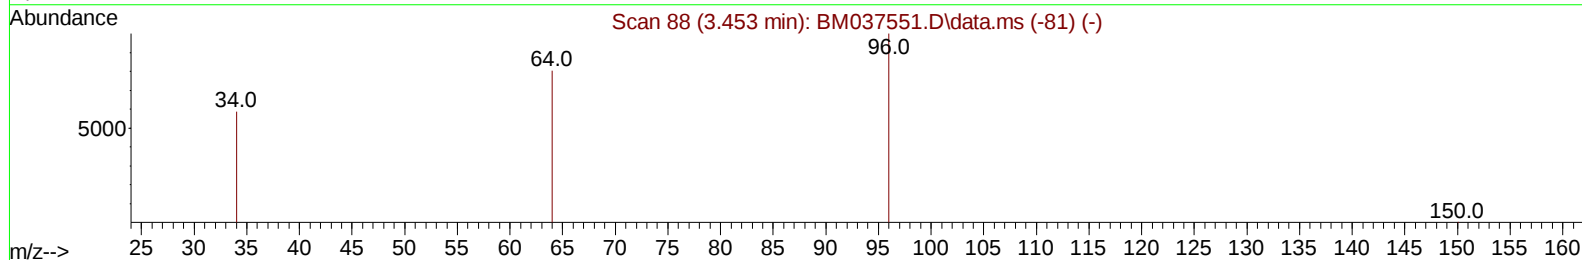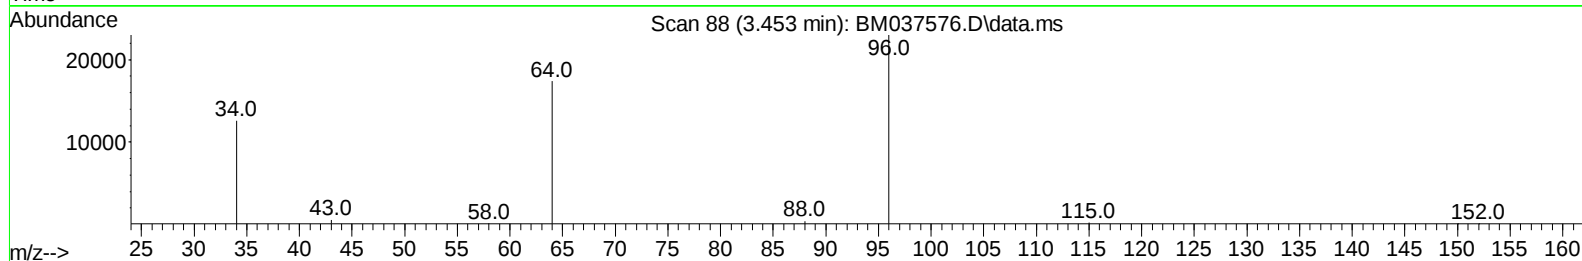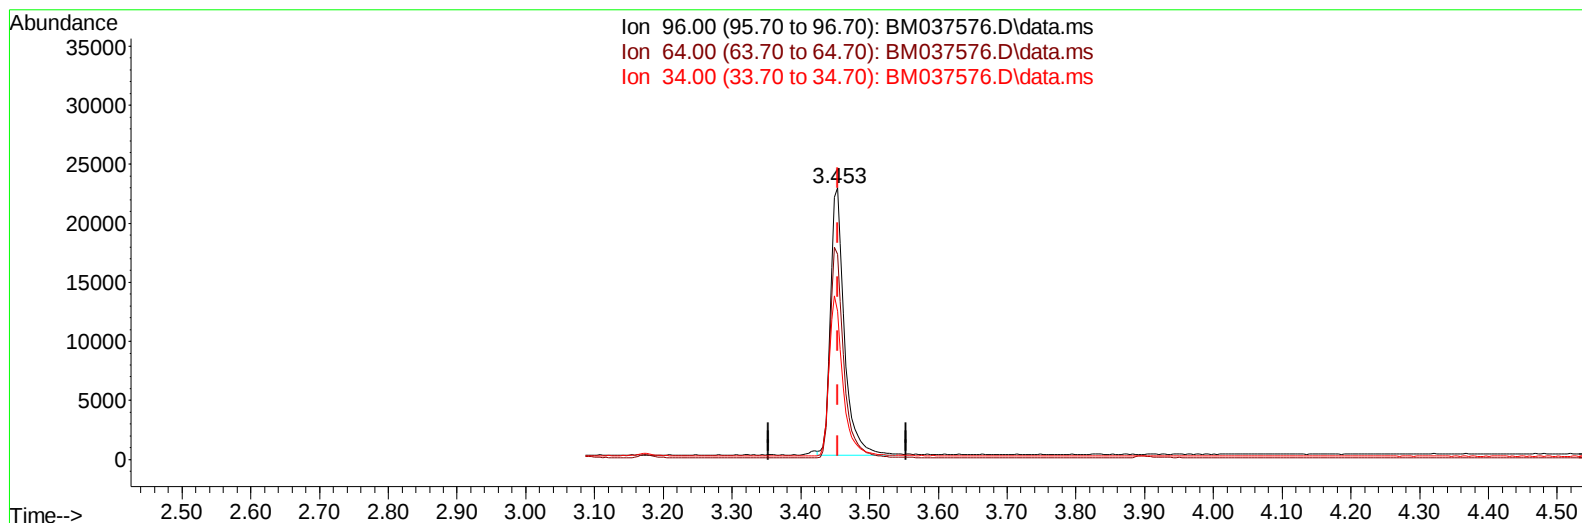

TIC: BM037576.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.453min (-0.000) 3.97 ng/u1 m

response 32009

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	67.60	75.51
34.00	42.40	54.58#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
 Data File : BM037576.D
 Acq On : 18 Nov 2022 22:49
 Operator : CG/JU
 Sample : N5689-01
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGCC4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/21/2022
 Supervised By :mohammad ahmed 11/21/2022

Quant Time: Nov 18 23:43:25 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 18 06:51:41 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	8.136	152		6939	0.400	ng/ul	0.00
4) Naphthalene-d8	10.957	136		20432	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.755	164		13071	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.486	188		27630	0.400	ng/ul	0.00
17) Chrysene-d12	21.646	240		20869	0.400	ng/ul	# 0.00
23) Perylene-d12	24.139	264		24304	0.400	ng/ul	# 0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.453	96		32009m	3.968	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.530	152		9661	0.285	ng/ul	0.00
18) Fluoranthene-d10	19.498	212		23033	0.334	ng/ul	0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	3.491	88		1704	0.203	ng/ul#	59

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
Data File : BM037576.D
Acq On : 18 Nov 2022 22:49
Operator : CG/JU
Sample : N5689-01
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGCC4

Manual IntegrationsAPPROVED

Quant Time: Nov 18 23:43:25 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 18 06:51:41 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/21/2022
Supervised By :mohammad ahmed 11/21/2022

