




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
Data File : BM037581.D
Acq On : 19 Nov 2022 01:52
Operator : CG/JU
Sample : N5689-06
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGCD1

Manual IntegrationsAPPROVED

Quant Time: Nov 19 02:53:47 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 18 06:51:41 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/21/2022
Supervised By :mohammad ahmed 11/21/2022

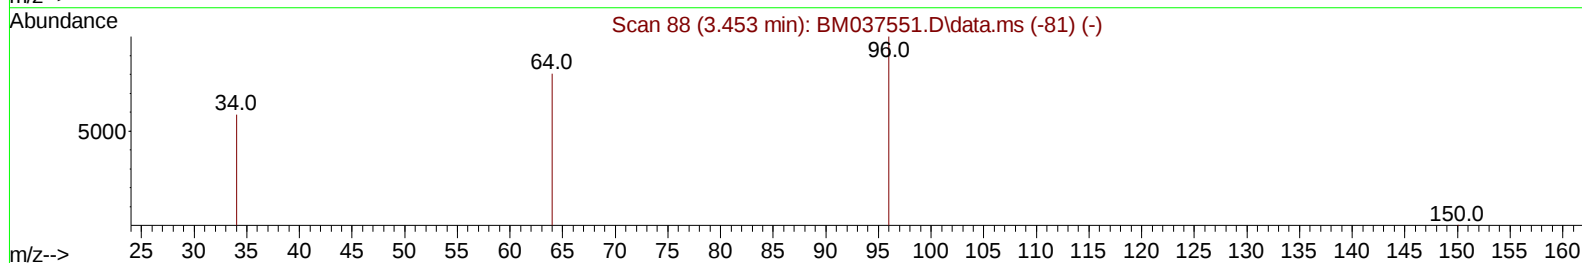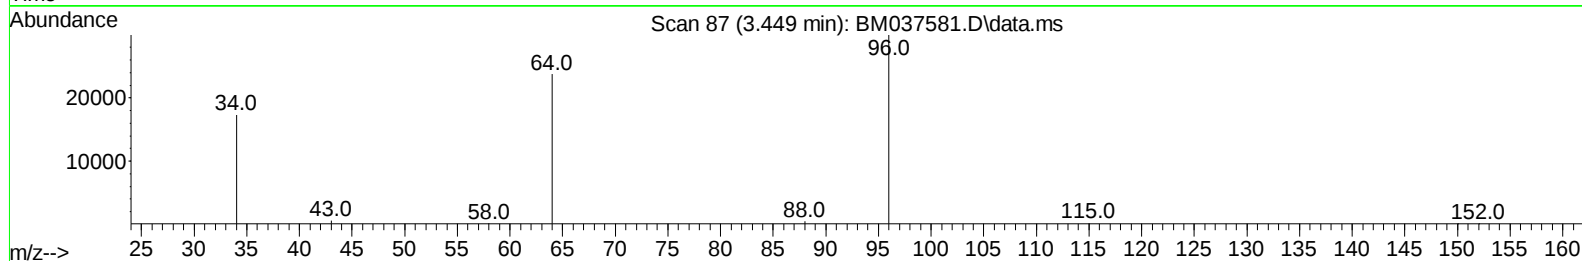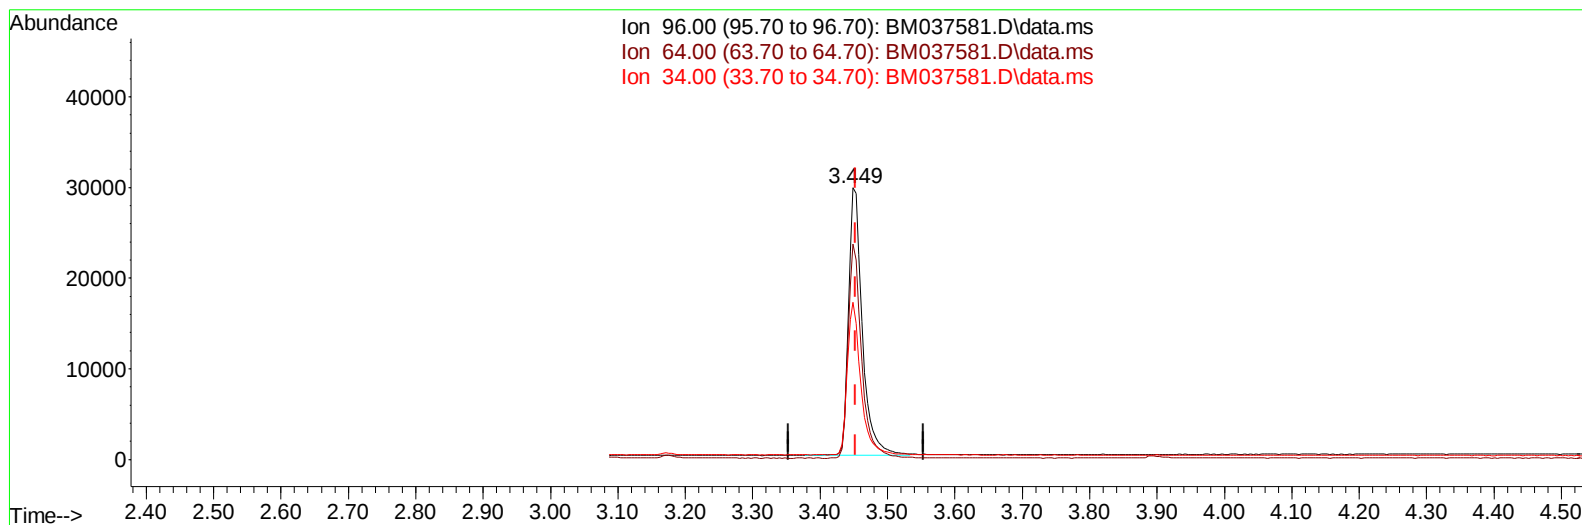

TIC: BM037581.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.449min (-0.004) 4.82 ng/u1

response 41890

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	67.60	79.25
34.00	42.40	57.80#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
 Data File : BM037581.D
 Acq On : 19 Nov 2022 01:52
 Operator : CG/JU
 Sample : N5689-06
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGCD1

Manual IntegrationsAPPROVED

Quant Time: Nov 19 02:53:47 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 18 06:51:41 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/21/2022
 Supervised By :mohammad ahmed 11/21/2022

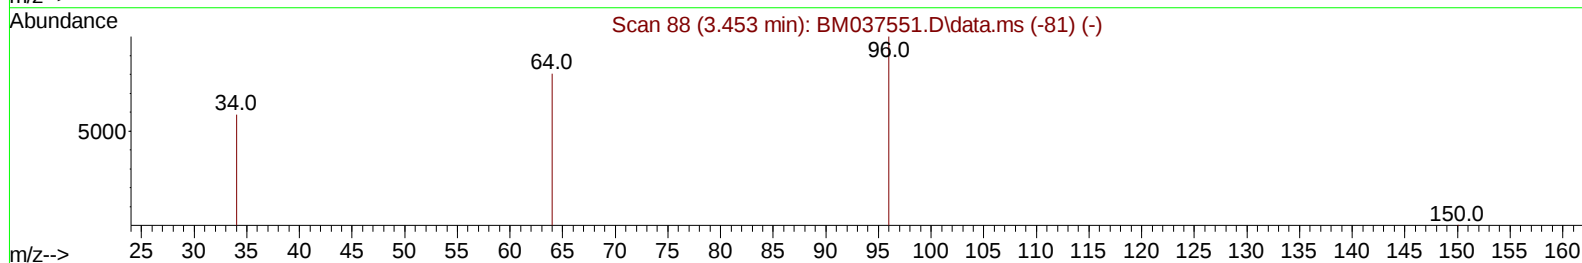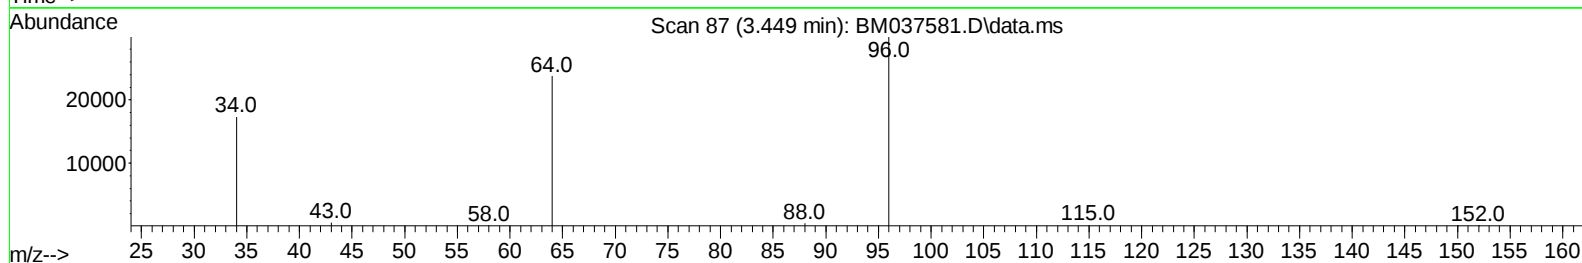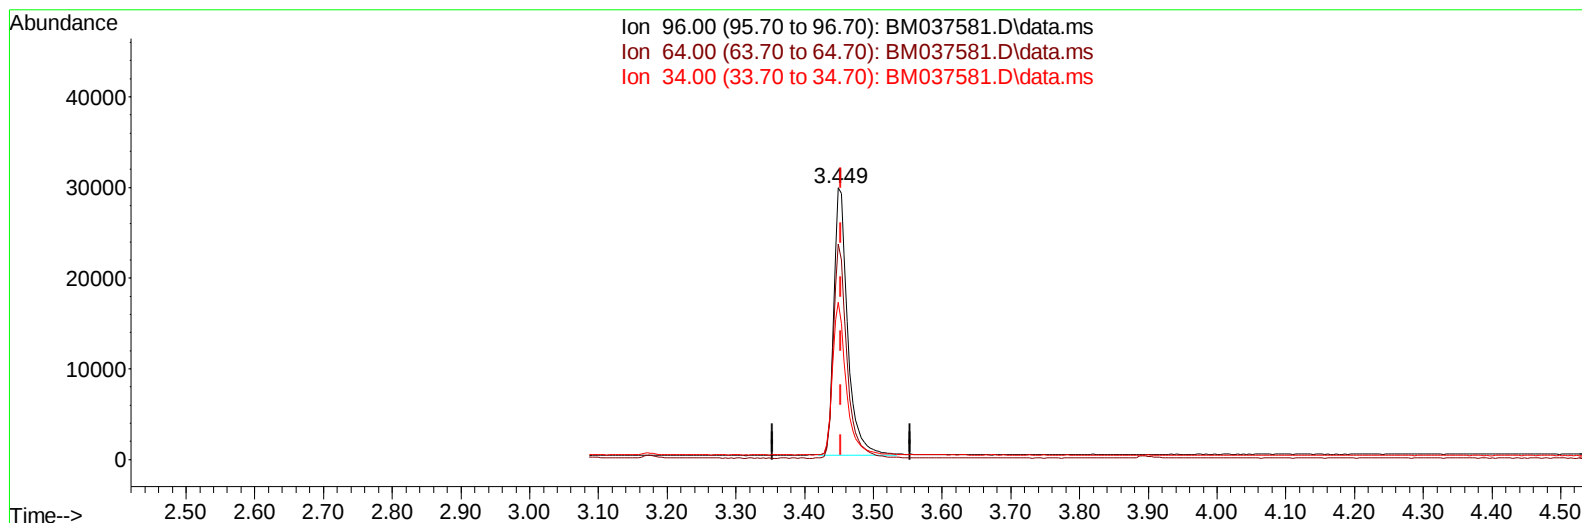

TIC: BM037581.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.449min (-0.004) 4.77 ng/ul m

response 41469

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	67.60	79.25
34.00	42.40	57.80#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
 Data File : BM037581.D
 Acq On : 19 Nov 2022 01:52
 Operator : CG/JU
 Sample : N5689-06
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGCD1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/21/2022
 Supervised By :mohammad ahmed 11/21/2022

Quant Time: Nov 19 02:53:47 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 18 06:51:41 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	8.136	152		7478	0.400	ng/ul	0.00
4) Naphthalene-d8	10.957	136		22065	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.755	164		13905	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.486	188		28877	0.400	ng/ul	0.00
17) Chrysene-d12	21.643	240		21003	0.400	ng/ul #	0.00
23) Perylene-d12	24.136	264		23544	0.400	ng/ul #	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.449	96		41469m	4.770	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.530	152		12317	0.337	ng/ul	0.00
18) Fluoranthene-d10	19.498	212		28142	0.405	ng/ul	0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	3.491	88		2230	0.246	ng/ul#	55

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
Data File : BM037581.D
Acq On : 19 Nov 2022 01:52
Operator : CG/JU
Sample : N5689-06
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGCD1

Manual IntegrationsAPPROVED

Quant Time: Nov 19 02:53:47 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 18 06:51:41 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/21/2022
Supervised By :mohammad ahmed 11/21/2022

