

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
 Data File : BM037521.D
 Acq On : 17 Nov 2022 11:33
 Operator : CG/JU
 Sample : N5622-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGCA3

Quant Time: Nov 17 12:54:09 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 17 00:46:50 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.145	152	6879	0.400	ng/ul	0.00
4) Naphthalene-d8	10.968	136	20393	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.766	164	13135	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.496	188	27738	0.400	ng/ul	0.00
17) Chrysene-d12	21.657	240	20090	0.400	ng/ul	0.00
23) Perylene-d12	24.156	264	23109	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.453	96	34071	4.260	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.541	152	9783	0.289	ng/ul	0.00
18) Fluoranthene-d10	19.508	212	23392	0.352	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.495	88	1897	0.228	ng/ul#	59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
Data File : BM037521.D
Acq On : 17 Nov 2022 11:33
Operator : CG/JU
Sample : N5622-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGCA3


Quant Time: Nov 17 12:54:09 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 17 00:46:50 2022
Response via : Initial Calibration

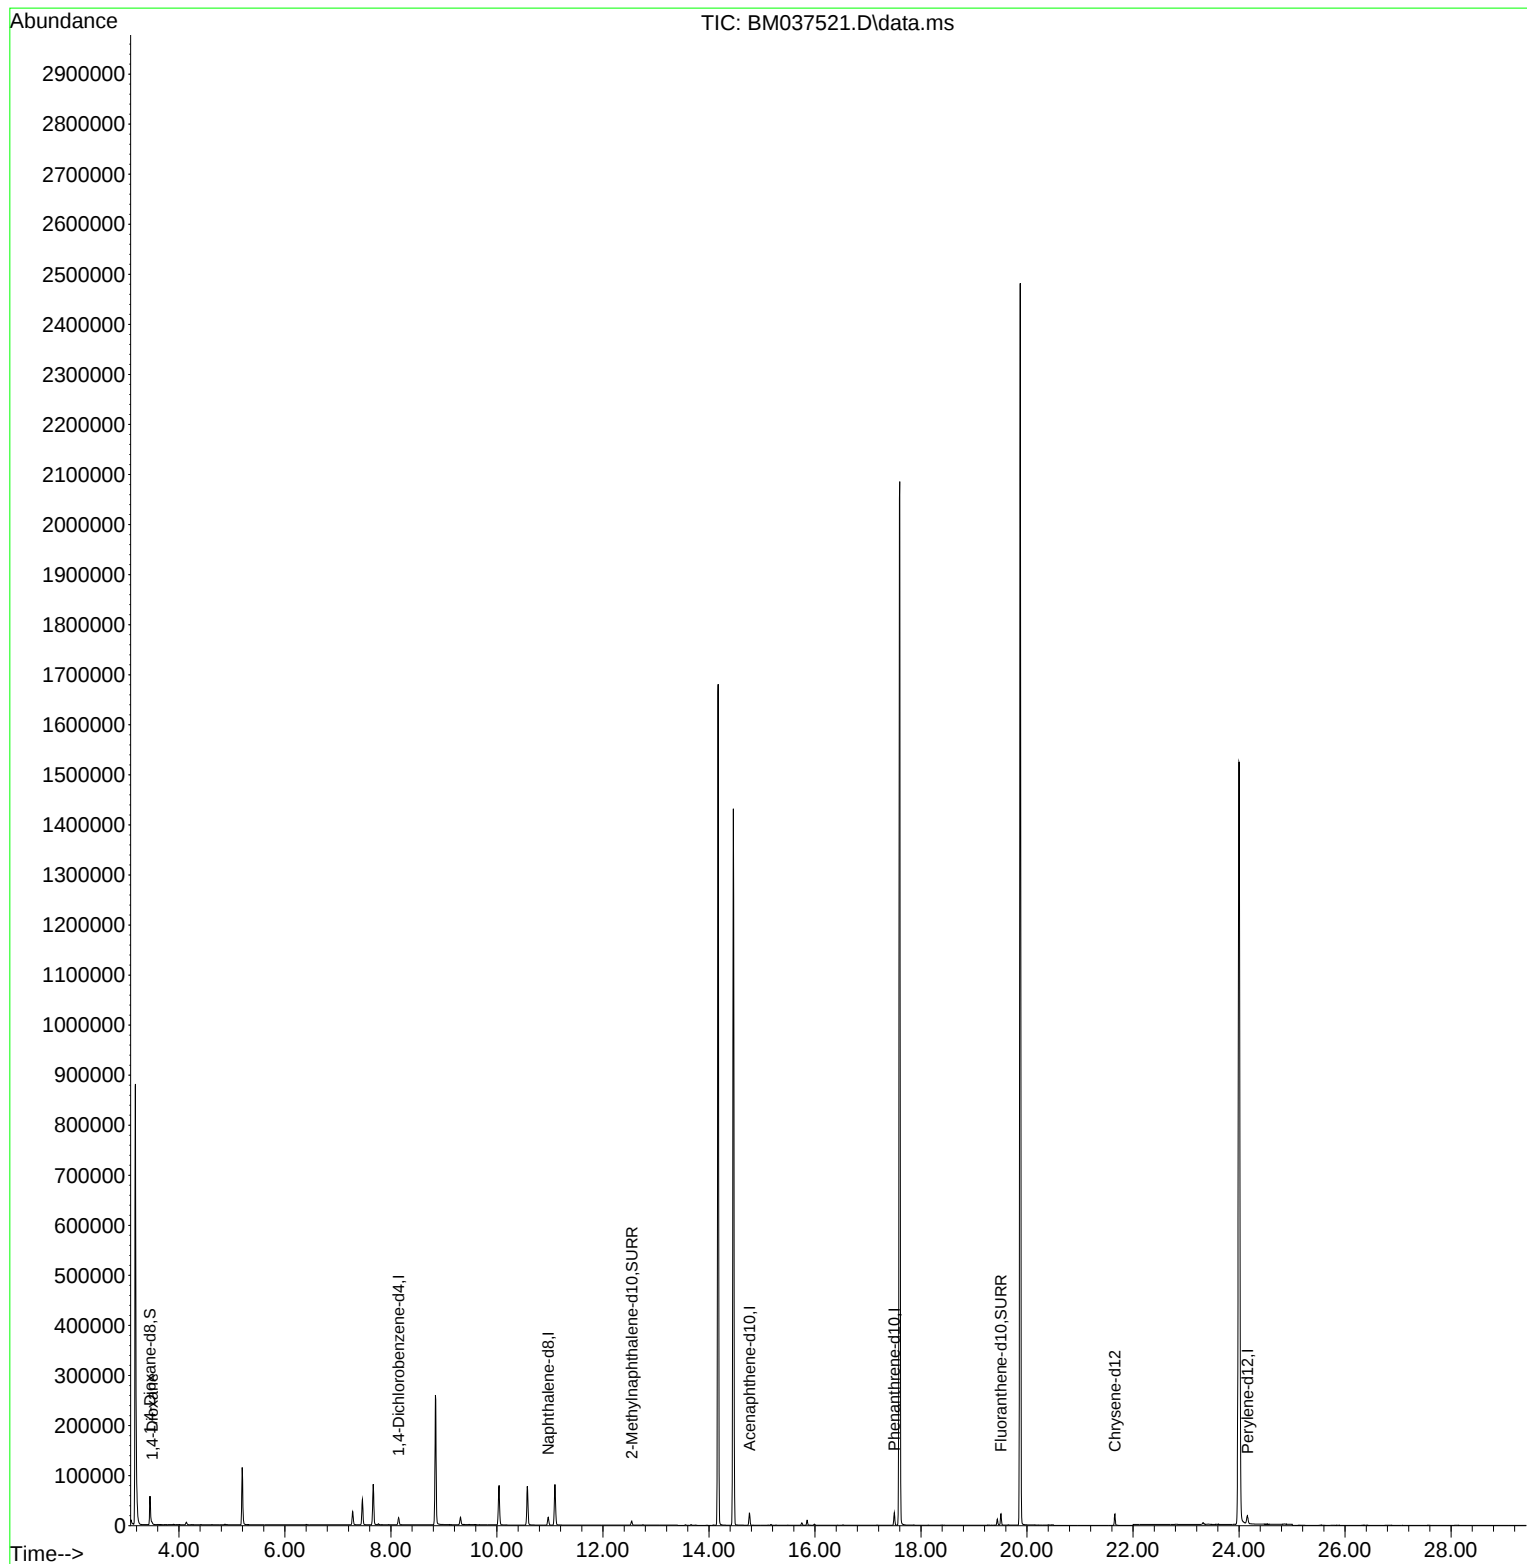

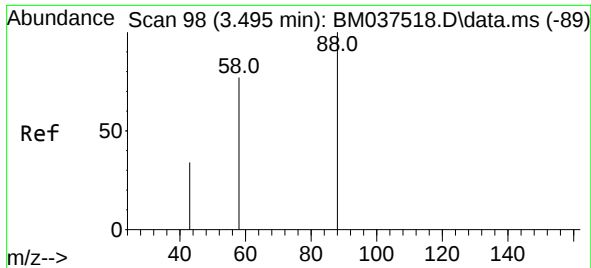

#2
 1,4-Dioxane
 Concen: 0.228 ng/ul
 RT: 3.495 min Scan# 98
 Delta R.T. 0.000 min
 Lab File: BM037521.D
 Acq: 17 Nov 2022 11:33

Instrument :
 BNA_M
 ClientSampleId :
 BGCA3

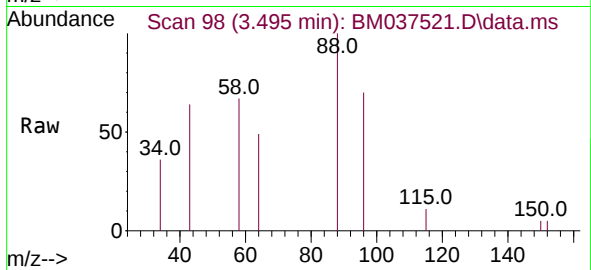

Tgt Ion:	88	Resp:	1897
Ion	Ratio	Lower	Upper
88	100		
43	64.0	102.8	154.2#
58	66.9	67.3	100.9#

