

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
 Data File : BM037523.D
 Acq On : 17 Nov 2022 12:46
 Operator : CG/JU
 Sample : N5622-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGCA5

Quant Time: Nov 17 13:48:05 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 17 00:46:50 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.145	152	6054	0.400	ng/ul	0.00
4) Naphthalene-d8	10.963	136	17813	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.761	164	11420	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.496	188	24053	0.400	ng/ul	0.00
17) Chrysene-d12	21.654	240	16850	0.400	ng/ul	0.00
23) Perylene-d12	24.153	264	19652	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.453	96	29800	4.234	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.541	152	9158	0.310	ng/ul	0.00
18) Fluoranthene-d10	19.504	212	23565	0.423	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.491	88	1552	0.212	ng/ul#	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
Data File : BM037523.D
Acq On : 17 Nov 2022 12:46
Operator : CG/JU
Sample : N5622-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGCA5

Quant Time: Nov 17 13:48:05 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 17 00:46:50 2022
Response via : Initial Calibration

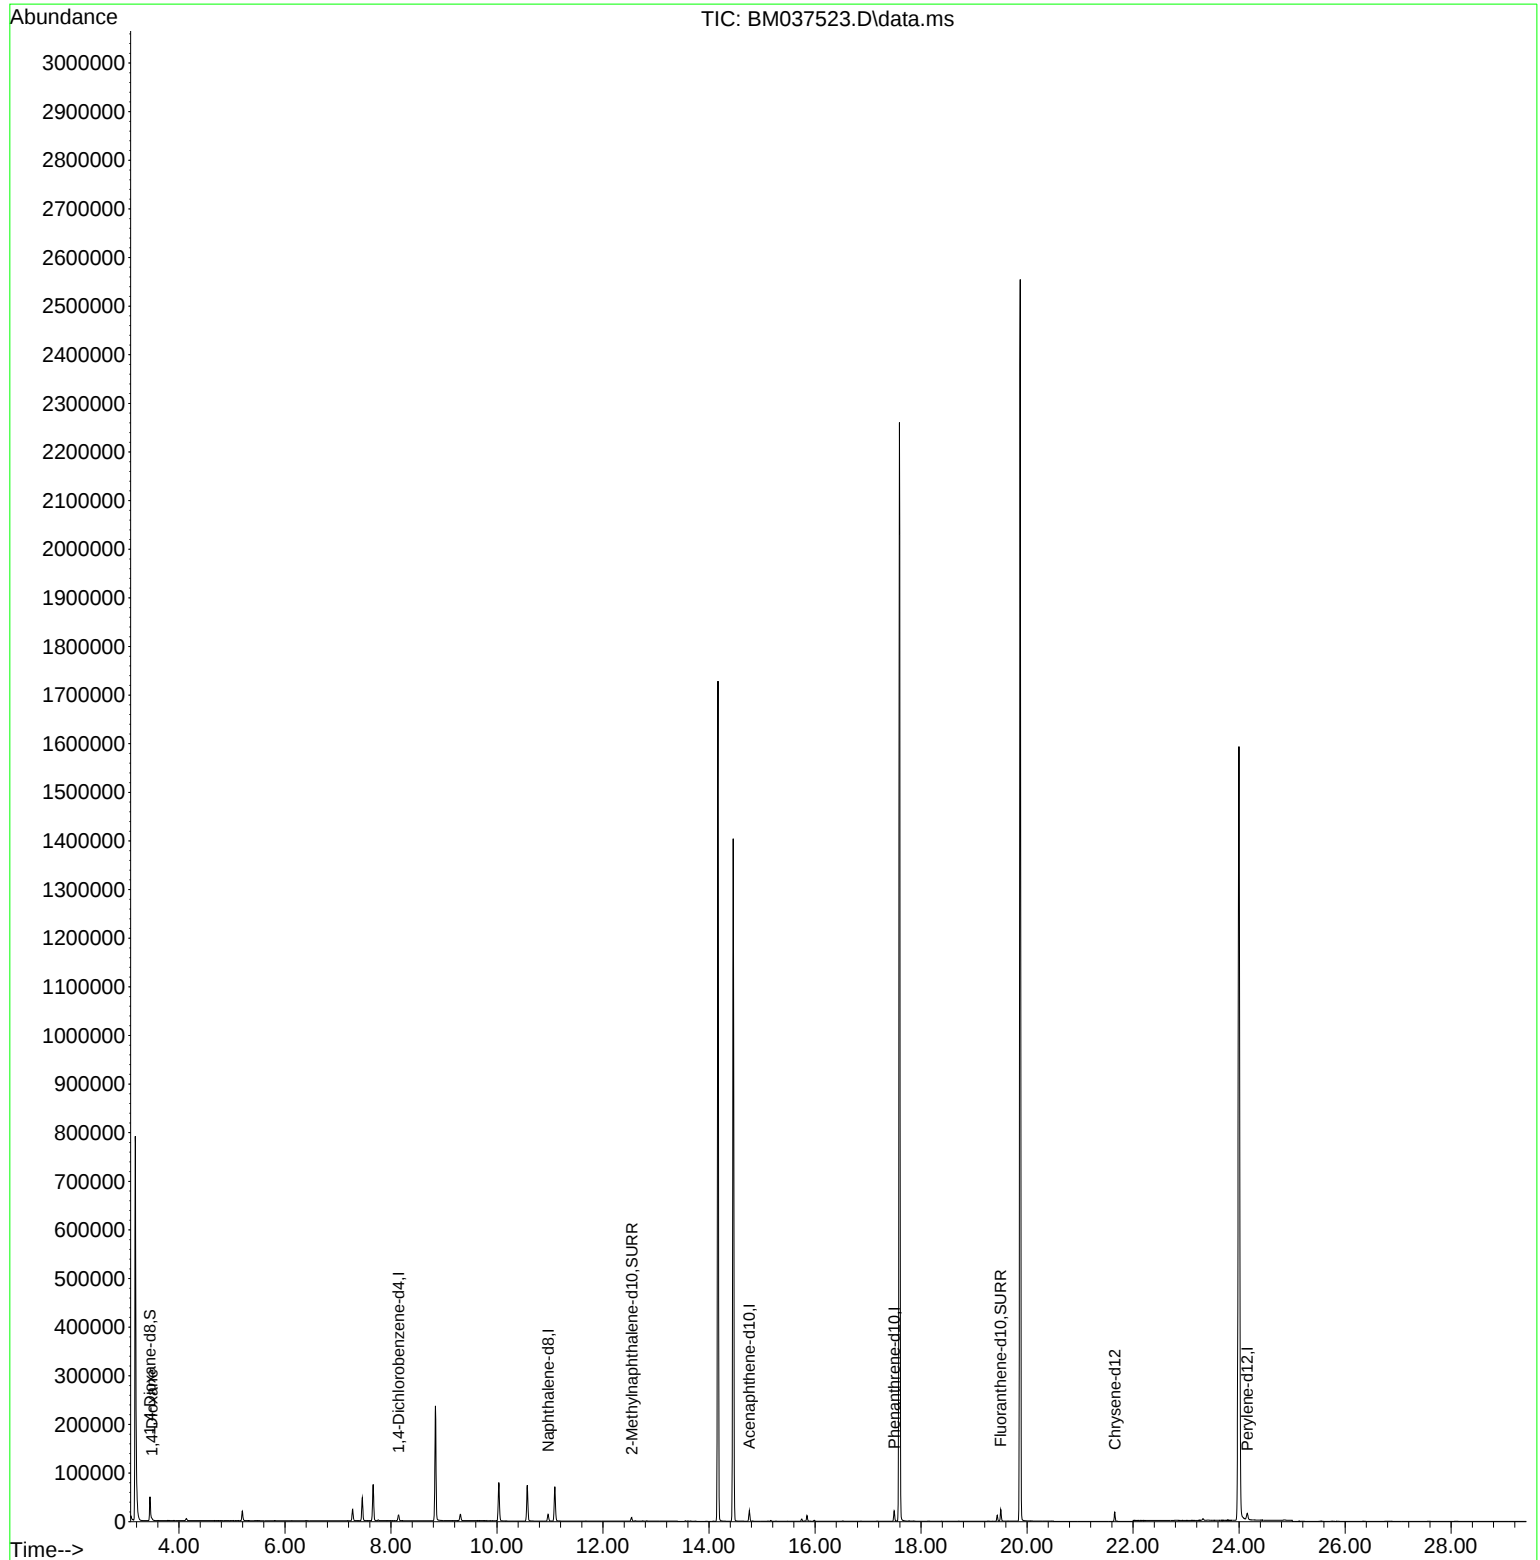

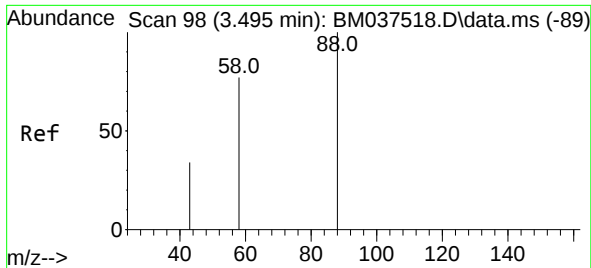

#2
 1,4-Dioxane
 Concen: 0.212 ng/ul
 RT: 3.491 min Scan# 91
 Delta R.T. -0.004 min
 Lab File: BM037523.D
 Acq: 17 Nov 2022 12:46

Instrument :
 BNA_M
 ClientSampleId :
 BGCA5

Tgt Ion: 88	Resp: 1552		
Ion Ratio	Lower	Upper	
88 100			
43 75.9	102.8	154.2#	
58 68.6	67.3	100.9	

