

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
 Data File : BM037536.D
 Acq On : 17 Nov 2022 21:17
 Operator : CG/JU
 Sample : N5622-11
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGCB3

Quant Time: Nov 17 22:52:40 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 17 00:46:50 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.141	152	5949	0.400	ng/ul	0.00
4) Naphthalene-d8	10.963	136	17410	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.760	164	11078	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.491	188	22982	0.400	ng/ul	0.00
17) Chrysene-d12	21.649	240	15986	0.400	ng/ul	# 0.00
23) Perylene-d12	24.145	264	19112	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.453	96	42351	6.123	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.536	152	10149	0.352	ng/ul	0.00
18) Fluoranthene-d10	19.503	212	22826	0.432	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.491	88	1962	0.273	ng/ul#	60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
Data File : BM037536.D
Acq On : 17 Nov 2022 21:17
Operator : CG/JU
Sample : N5622-11
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGCB3


Quant Time: Nov 17 22:52:40 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 17 00:46:50 2022
Response via : Initial Calibration

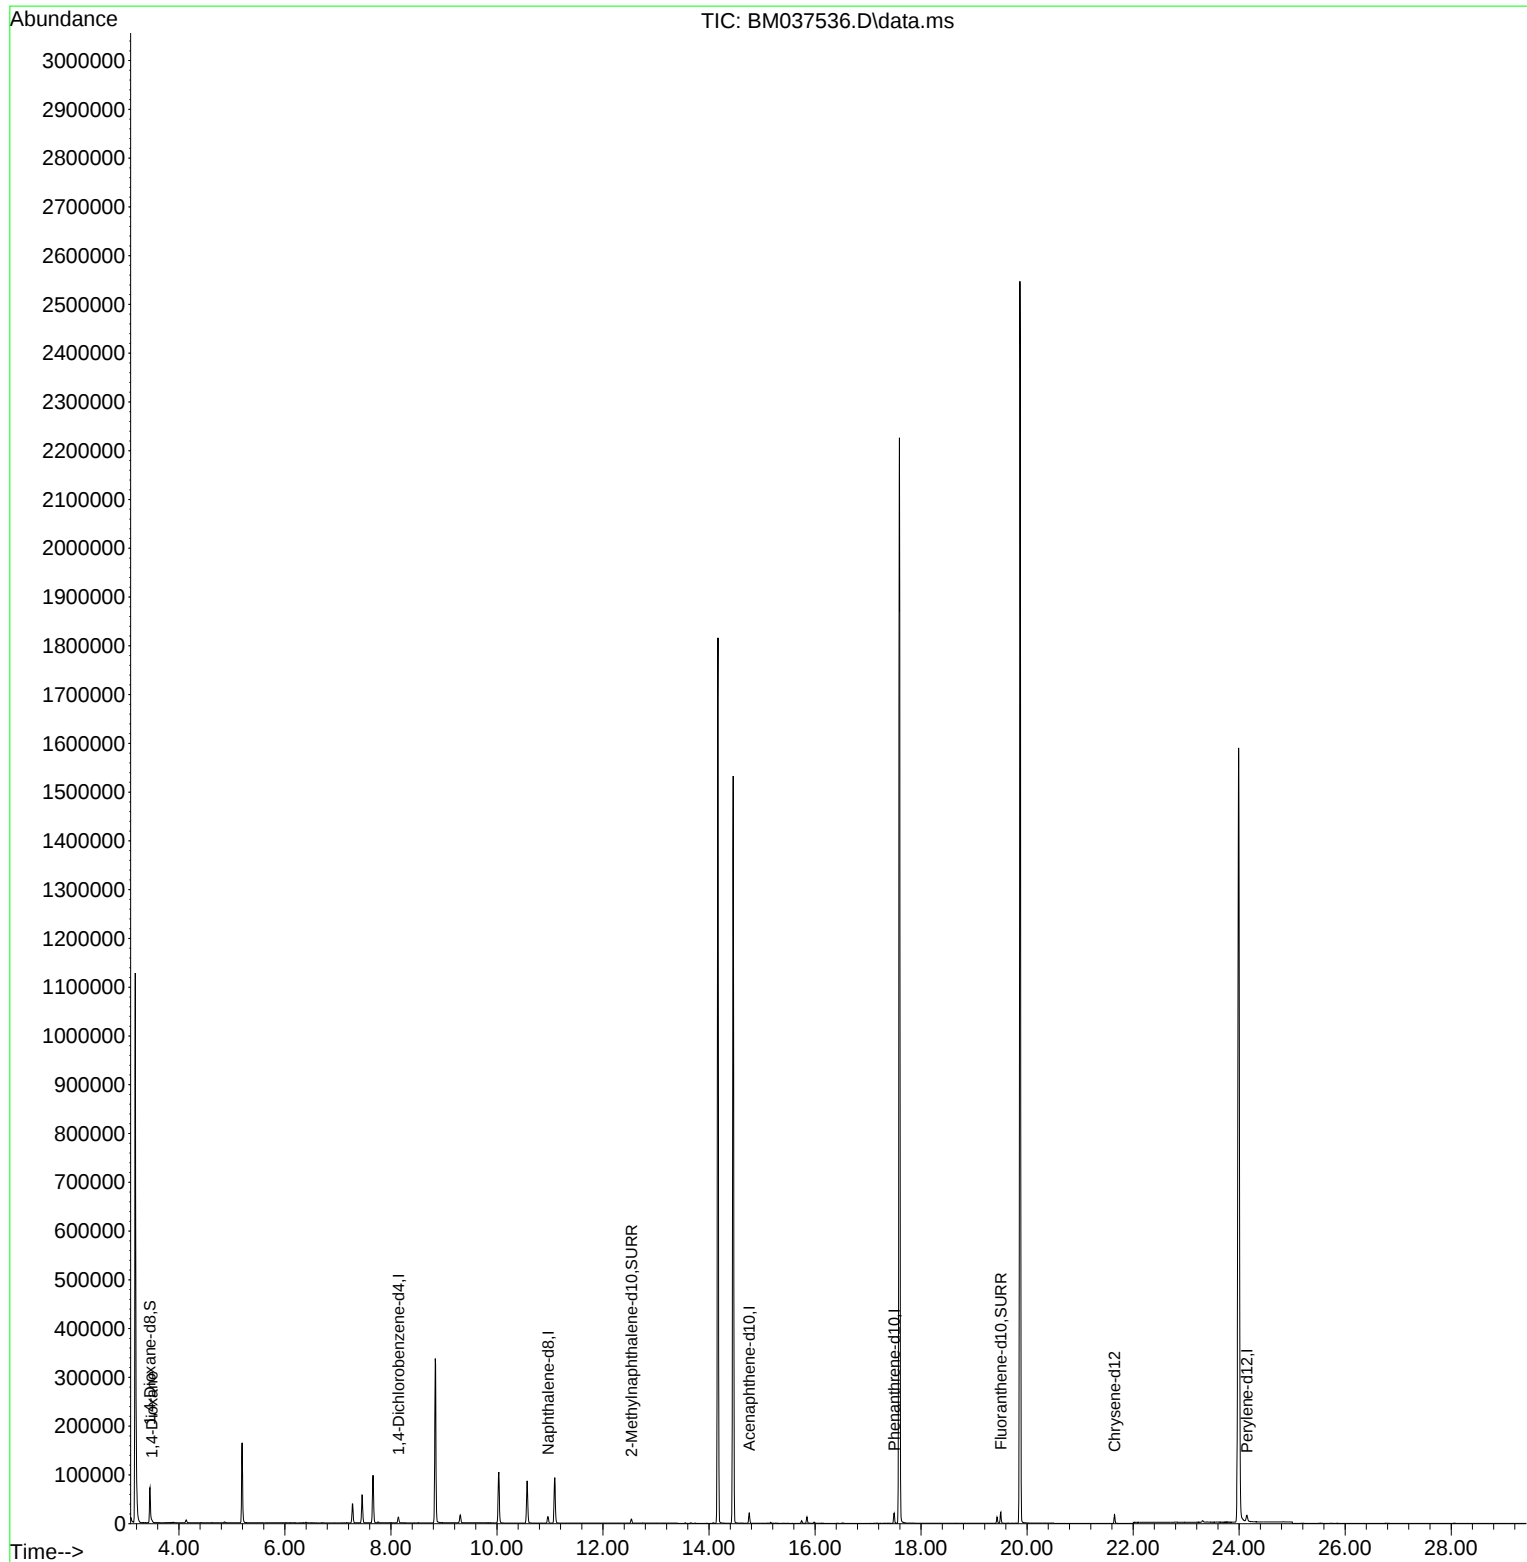

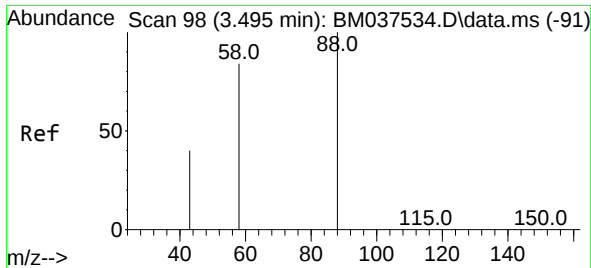

#2
 1,4-Dioxane
 Concen: 0.273 ng/ul
 RT: 3.491 min Scan# 91
 Delta R.T. -0.004 min
 Lab File: BM037536.D
 Acq: 17 Nov 2022 21:17

Instrument :
 BNA_M
 ClientSampleId :
 BGCB3

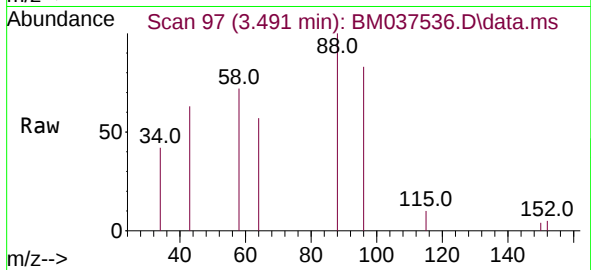

Tgt Ion: 88 Resp: 1962

Ion	Ratio	Lower	Upper
88	100		
43	62.8	102.8	154.2#
58	72.1	67.3	100.9

