

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
 Data File : BM037537.D
 Acq On : 17 Nov 2022 21:53
 Operator : CG/JU
 Sample : N5622-12
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGCB4

Quant Time: Nov 17 22:59:41 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 17 00:46:50 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.140	152	7533	0.400	ng/ul	0.00
4) Naphthalene-d8	10.963	136	21842	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.760	164	13553	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.490	188	28124	0.400	ng/ul	0.00
17) Chrysene-d12	21.652	240	19686	0.400	ng/ul	0.00
23) Perylene-d12	24.145	264	23254	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.453	96	39676	4.530	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.536	152	10883	0.301	ng/ul	0.00
18) Fluoranthene-d10	19.503	212	25501	0.392	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.495	88	2001	0.220	ng/ul#	44


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
Data File : BM037537.D
Acq On : 17 Nov 2022 21:53
Operator : CG/JU
Sample : N5622-12
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGCB4

Quant Time: Nov 17 22:59:41 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 17 00:46:50 2022
Response via : Initial Calibration

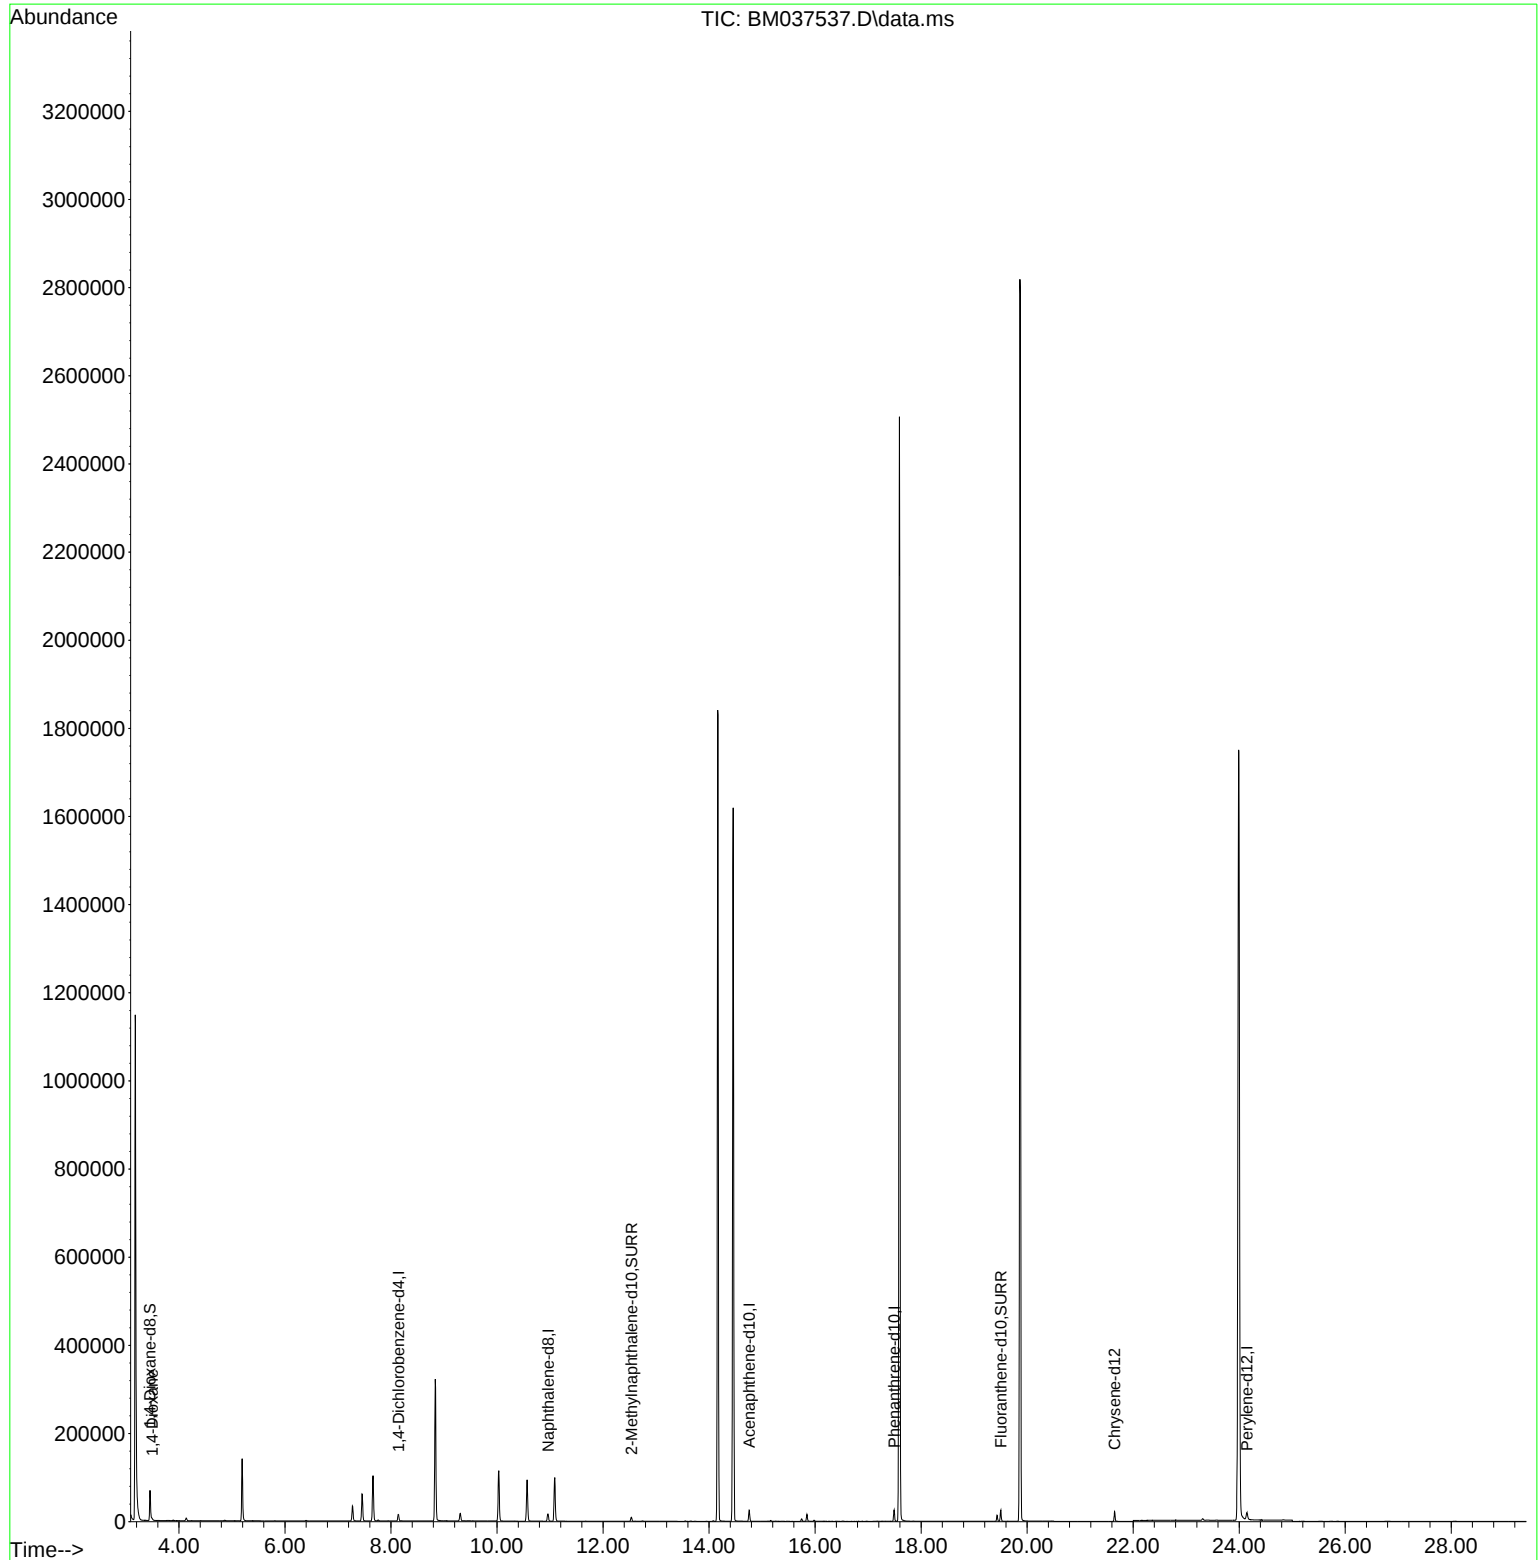

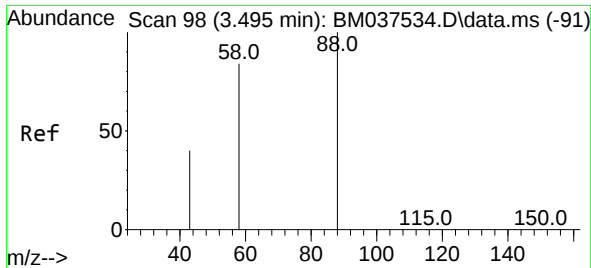

#2
 1,4-Dioxane
 Concen: 0.220 ng/ul
 RT: 3.495 min Scan# 98
 Delta R.T. 0.000 min
 Lab File: BM037537.D
 Acq: 17 Nov 2022 21:53

Instrument :
 BNA_M
 ClientSampleId :
 BGCB4

Tgt Ion:	88	Resp:	2001
Ion	Ratio	Lower	Upper
88	100		
43	48.9	102.8	154.2#
58	51.3	67.3	100.9#

