

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
 Data File : BM037541.D
 Acq On : 18 Nov 2022 00:19
 Operator : CG/JU
 Sample : N5622-16
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGCA1

Quant Time: Nov 18 02:27:05 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 17 23:00:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.140	152	8455	0.400	ng/ul	0.00
4) Naphthalene-d8	10.963	136	25052	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.755	164	15494	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.491	188	32725	0.400	ng/ul	0.00
17) Chrysene-d12	21.649	240	24008	0.400	ng/ul	0.00
23) Perylene-d12	24.142	264	28008	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.453	96	45264	4.605	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.536	152	12259	0.295	ng/ul	0.00
18) Fluoranthene-d10	19.503	212	28806	0.363	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.491	88	2433	0.238	ng/ul#	49


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
Data File : BM037541.D
Acq On : 18 Nov 2022 00:19
Operator : CG/JU
Sample : N5622-16
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGCA1

Quant Time: Nov 18 02:27:05 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 17 23:00:56 2022
Response via : Initial Calibration

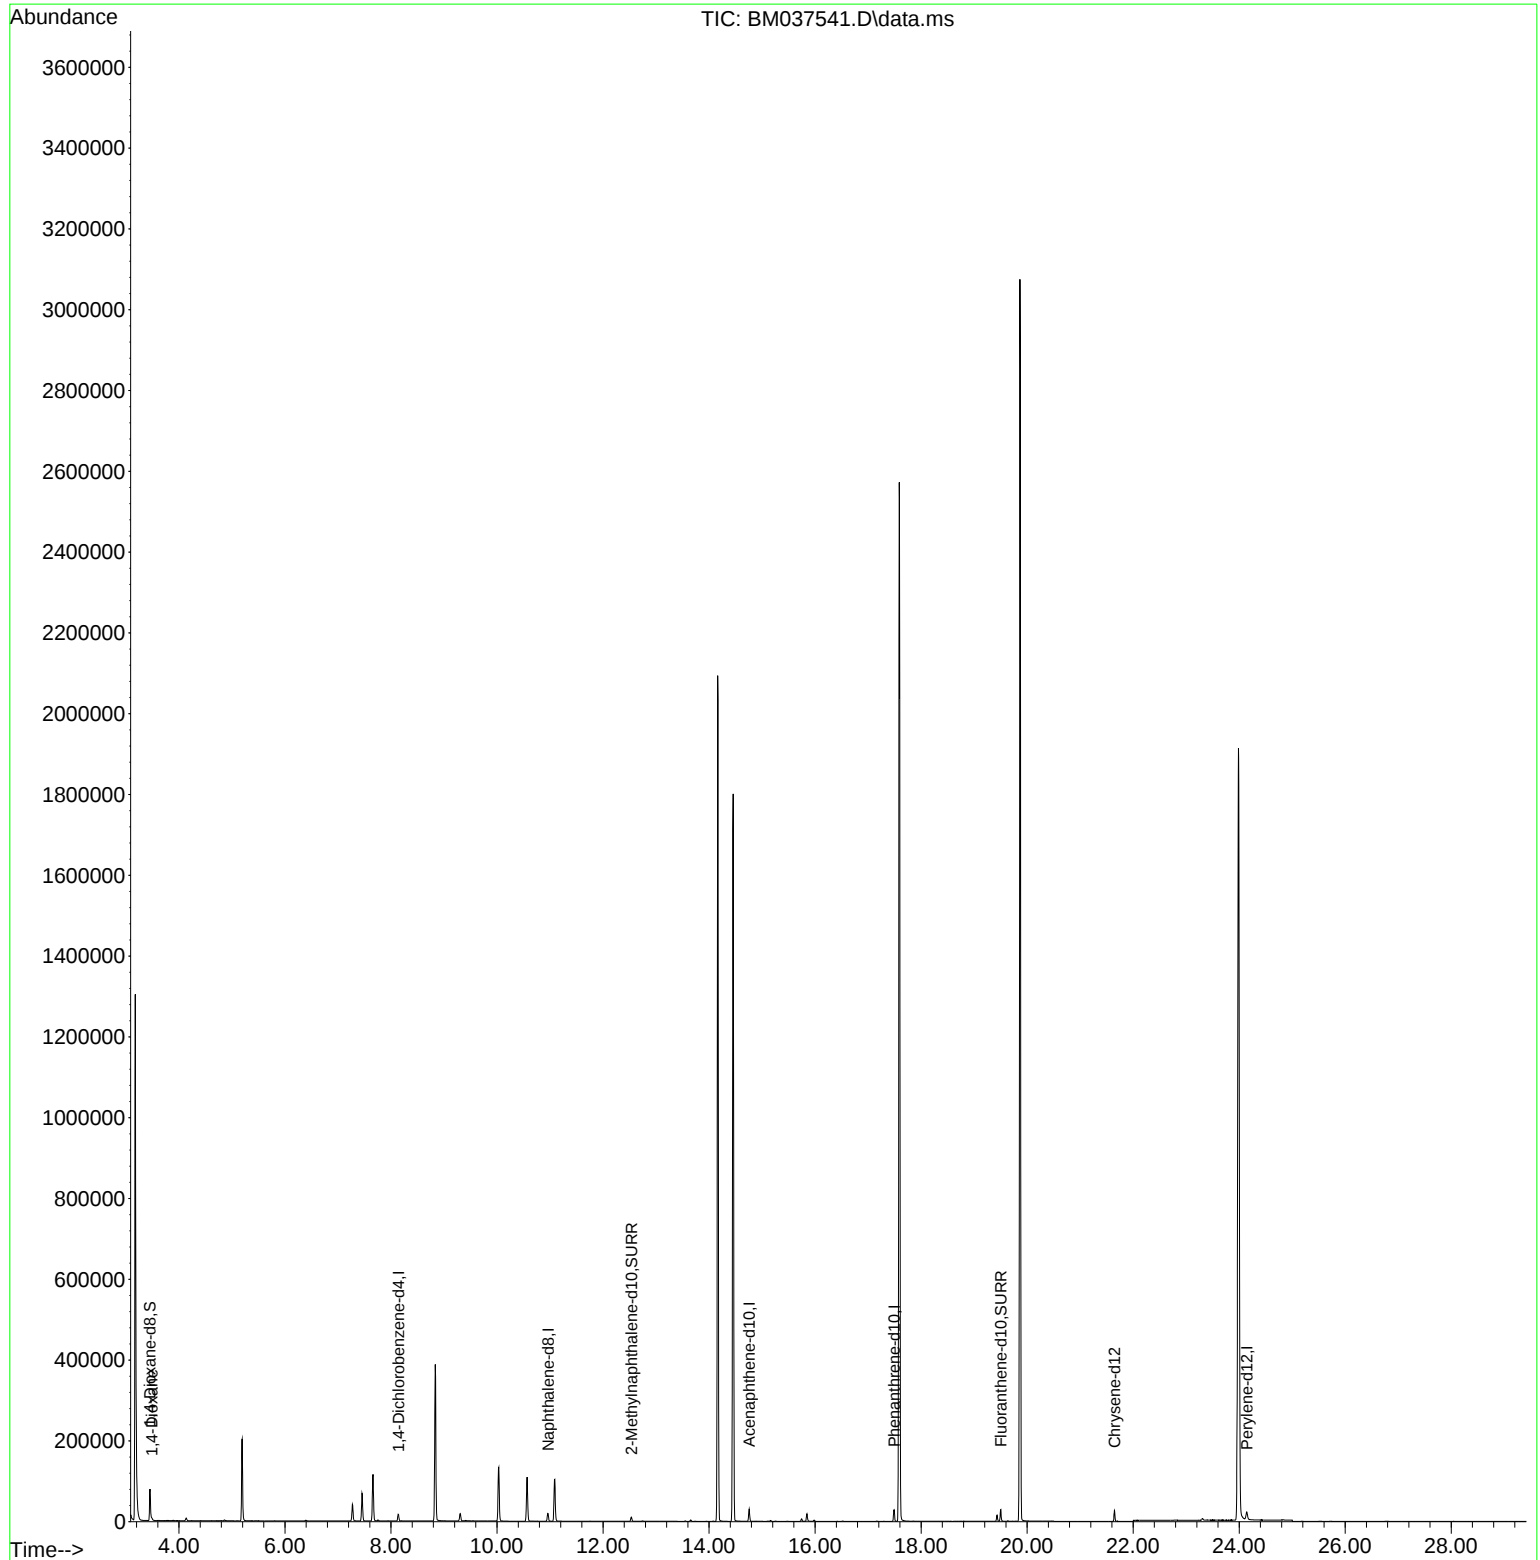

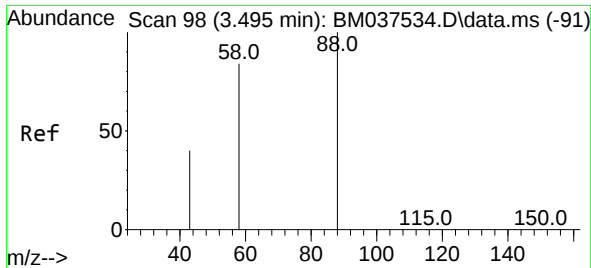

#2
 1,4-Dioxane
 Concen: 0.238 ng/ul
 RT: 3.491 min Scan# 91
 Delta R.T. -0.004 min
 Lab File: BM037541.D
 Acq: 18 Nov 2022 00:19

Instrument :
 BNA_M
 ClientSampleId :
 BGCA1

Tgt Ion: 88 Resp: 2433
 Ion Ratio Lower Upper
 88 100
 43 52.3 102.8 154.2#
 58 57.7 67.3 100.9#

