

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
 Data File : BM037542.D
 Acq On : 18 Nov 2022 00:55
 Operator : CG/JU
 Sample : N5622-17
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGCA2

Quant Time: Nov 18 02:27:51 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 17 23:00:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.141	152	9125	0.400	ng/ul	0.00
4) Naphthalene-d8	10.958	136	26704	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.756	164	16644	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.491	188	35041	0.400	ng/ul	0.00
17) Chrysene-d12	21.649	240	24143	0.400	ng/ul	0.00
23) Perylene-d12	24.142	264	28536	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.454	96	48795	4.599	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.530	152	11989	0.271	ng/ul	-0.01
18) Fluoranthene-d10	19.498	212	28186	0.353	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.491	88	2373	0.215	ng/ul#	46


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
Data File : BM037542.D
Acq On : 18 Nov 2022 00:55
Operator : CG/JU
Sample : N5622-17
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGCA2

Quant Time: Nov 18 02:27:51 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 17 23:00:56 2022
Response via : Initial Calibration

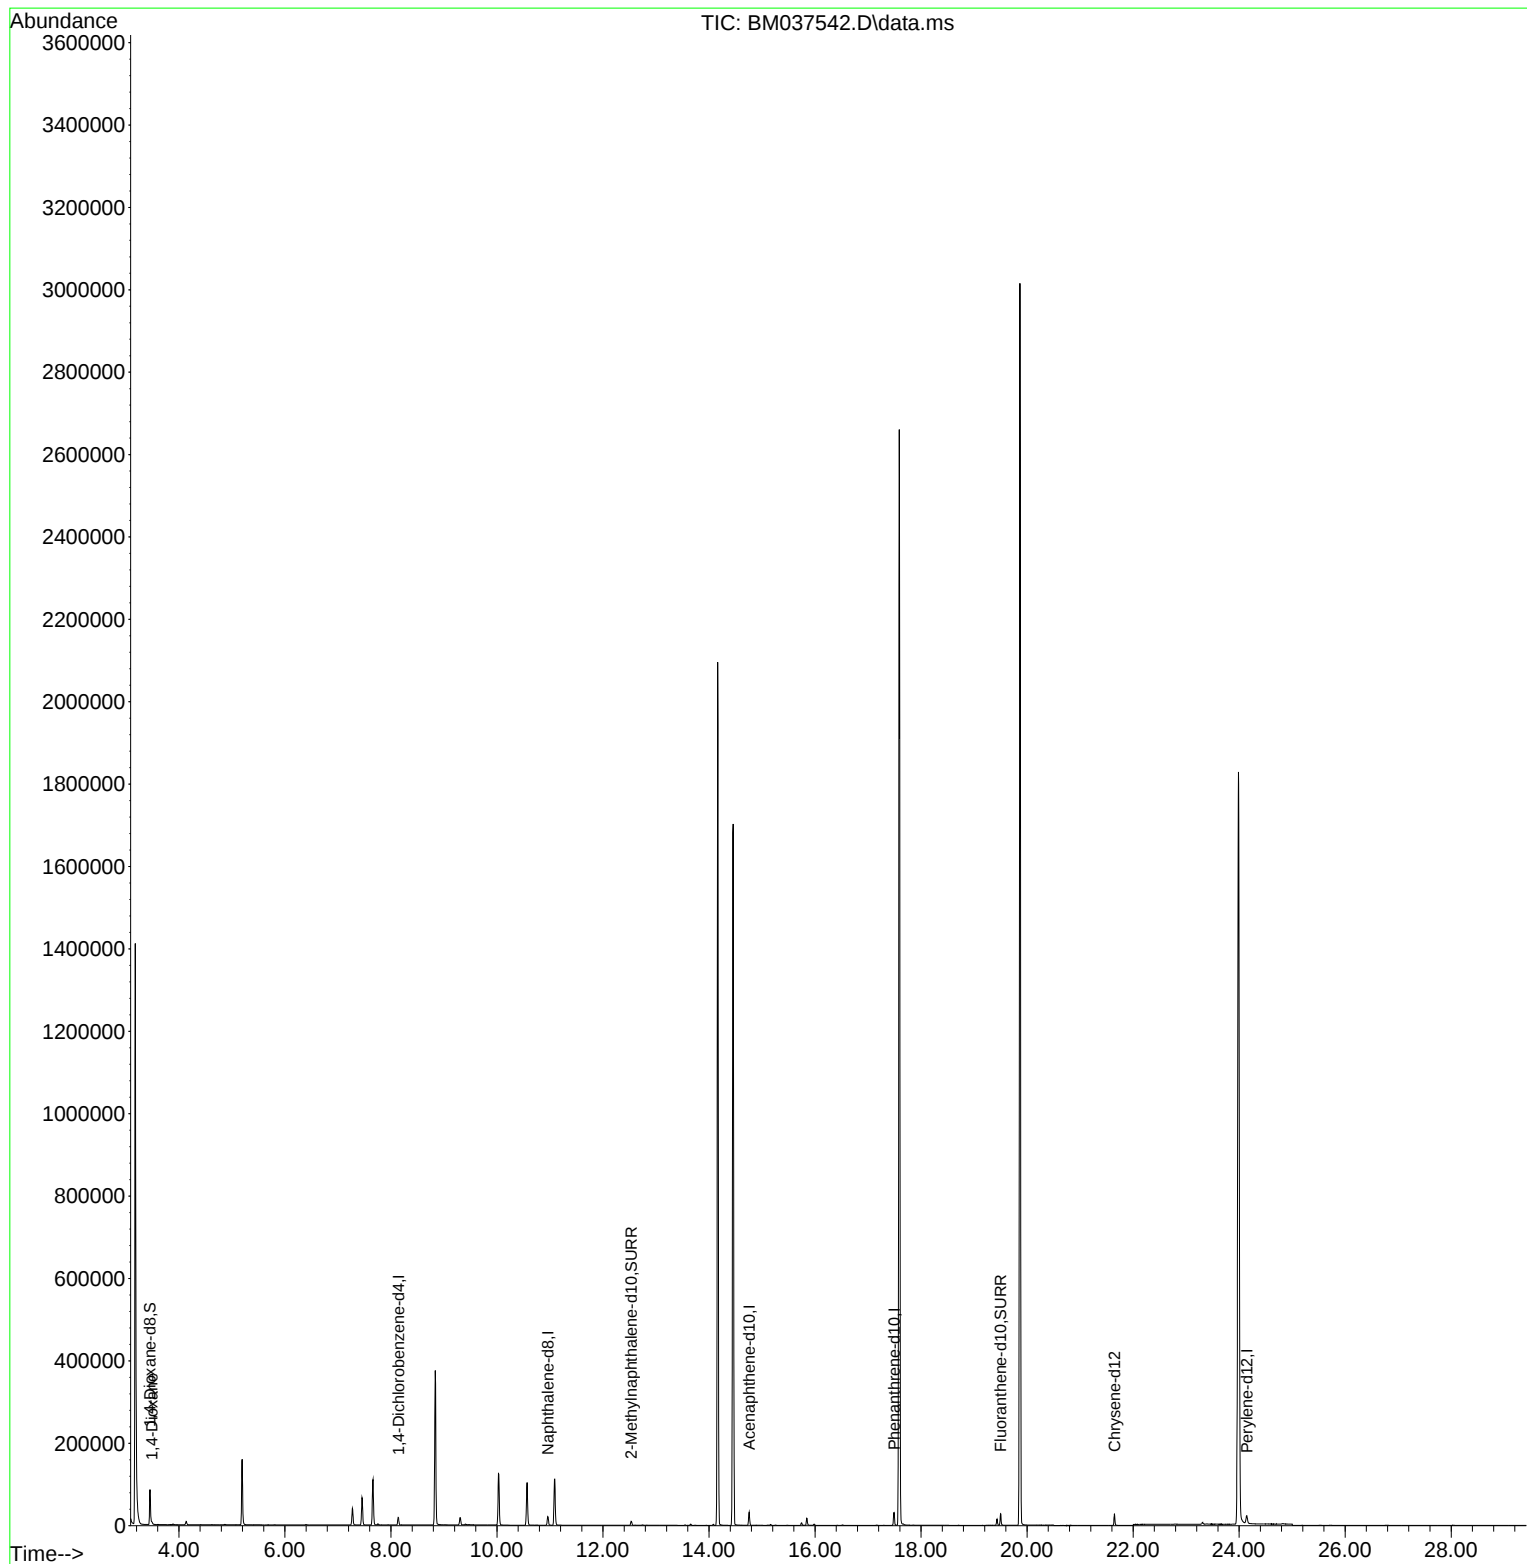

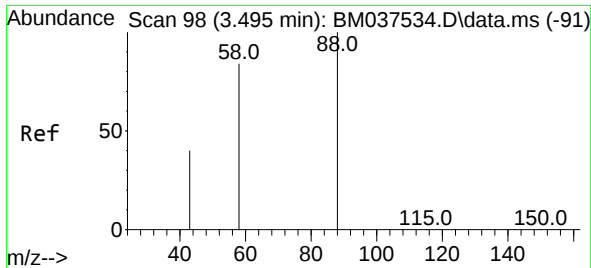

#2
 1,4-Dioxane
 Concen: 0.215 ng/ul
 RT: 3.491 min Scan# 91
 Delta R.T. -0.004 min
 Lab File: BM037542.D
 Acq: 18 Nov 2022 00:55

Instrument :
 BNA_M
 ClientSampleId :
 BGCA2

Tgt Ion:	88	Resp:	2373
Ion	Ratio	Lower	Upper
88	100		
43	50.0	102.8	154.2#
58	54.4	67.3	100.9#

