

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
 Data File : BM037543.D
 Acq On : 18 Nov 2022 01:31
 Operator : CG/JU
 Sample : N5622-18
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGCB5

Quant Time: Nov 18 02:28:34 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 17 23:00:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.136	152	8091	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.958	136	23849	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.756	164	14825	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.491	188	31428	0.400	ng/ul	0.00
17) Chrysene-d12	21.649	240	22165	0.400	ng/ul	0.00
23) Perylene-d12	24.145	264	26245	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.454	96	44922	4.775	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.530	152	11838	0.299	ng/ul	-0.01
18) Fluoranthene-d10	19.499	212	30770	0.420	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.491	88	2254	0.230	ng/ul#	44


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
Data File : BM037543.D
Acq On : 18 Nov 2022 01:31
Operator : CG/JU
Sample : N5622-18
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGCB5

Quant Time: Nov 18 02:28:34 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 17 23:00:56 2022
Response via : Initial Calibration

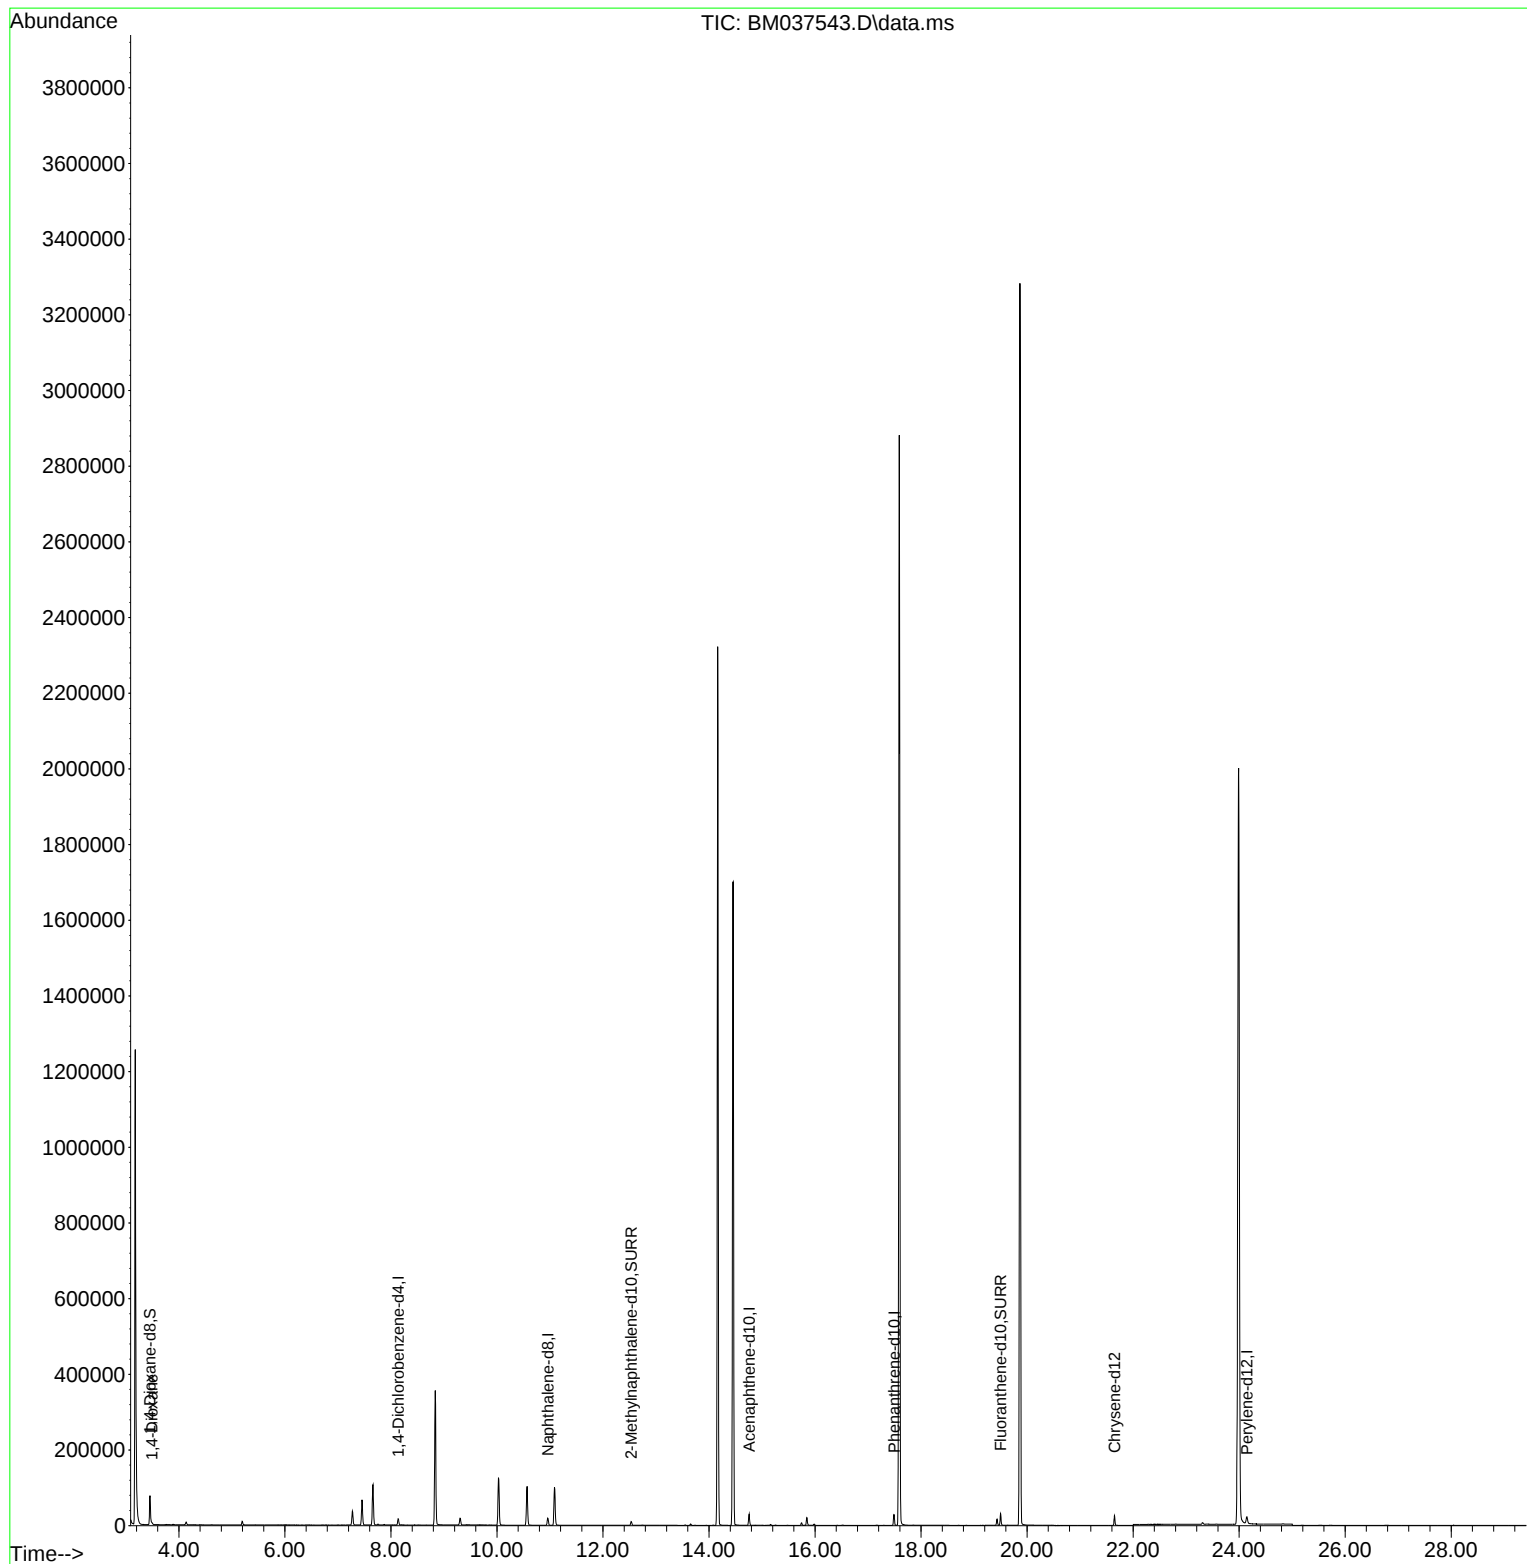

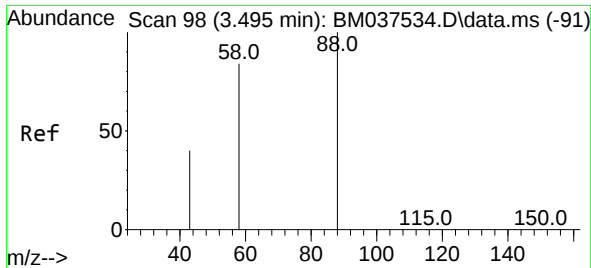

#2
 1,4-Dioxane
 Concen: 0.230 ng/ul
 RT: 3.491 min Scan# 91
 Delta R.T. -0.004 min
 Lab File: BM037543.D
 Acq: 18 Nov 2022 01:31

Instrument :
 BNA_M
 ClientSampleId :
 BGCB5

Tgt Ion: 88 Resp: 2254

Ion	Ratio	Lower	Upper
88	100		
43	47.8	102.8	154.2#
58	52.9	67.3	100.9#

