

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
 Data File : BM037546.D
 Acq On : 18 Nov 2022 03:20
 Operator : CG/JU
 Sample : N5623-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGCB8

Quant Time: Nov 18 04:16:34 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 17 23:00:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.136	152	7224	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.957	136	21064	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.755	164	13292	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.486	188	27807	0.400	ng/ul	-0.01
17) Chrysene-d12	21.646	240	19316	0.400	ng/ul	#-0.01
23) Perylene-d12	24.142	264	22210	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.453	96	40520	4.824	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.530	152	10805	0.309	ng/ul	-0.01
18) Fluoranthene-d10	19.498	212	26203	0.411	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.491	88	1874	0.214	ng/ul#	52


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
Data File : BM037546.D
Acq On : 18 Nov 2022 03:20
Operator : CG/JU
Sample : N5623-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGCB8

Quant Time: Nov 18 04:16:34 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 17 23:00:56 2022
Response via : Initial Calibration

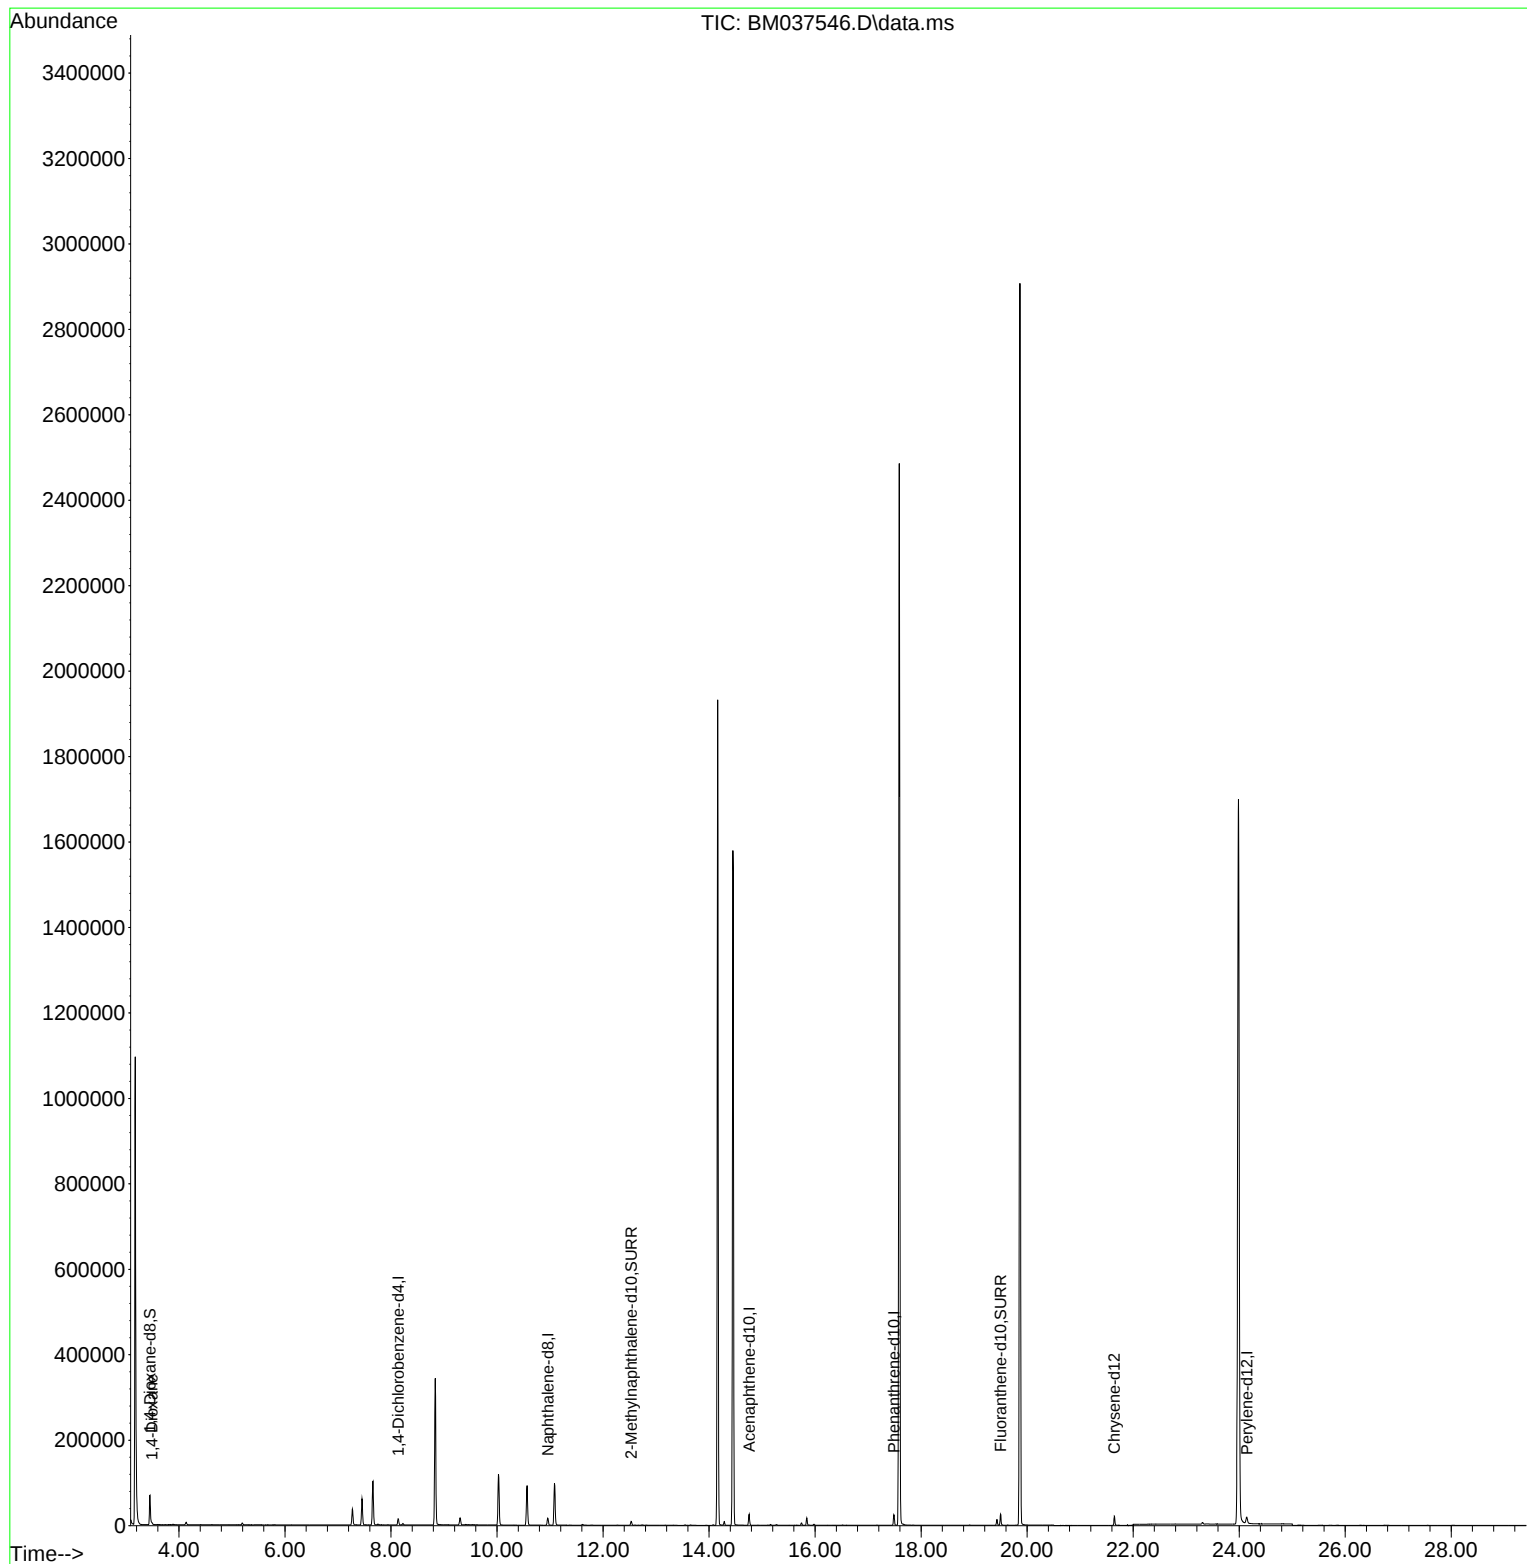

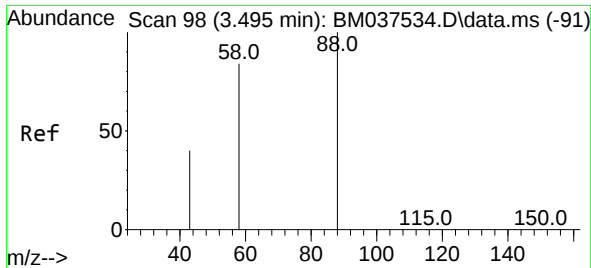

#2
 1,4-Dioxane
 Concen: 0.214 ng/ul
 RT: 3.491 min Scan# 91
 Delta R.T. -0.004 min
 Lab File: BM037546.D
 Acq: 18 Nov 2022 03:20

Instrument :
 BNA_M
 ClientSampleId :
 BGCB8

Tgt Ion:	88	Resp:	1874
Ion	Ratio	Lower	Upper
88	100		
43	54.9	102.8	154.2#
58	61.3	67.3	100.9#

