

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
 Data File : BM037547.D
 Acq On : 18 Nov 2022 03:56
 Operator : CG/JU
 Sample : N5623-02
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGCB9

Quant Time: Nov 18 04:54:55 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 17 23:00:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.136	152	8632	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.957	136	25125	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.755	164	15543	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.490	188	33110	0.400	ng/ul	0.00
17) Chrysene-d12	21.649	240	23136	0.400	ng/ul	0.00
23) Perylene-d12	24.145	264	26272	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.453	96	47132	4.696	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.530	152	13025	0.313	ng/ul	-0.01
18) Fluoranthene-d10	19.498	212	33976	0.444	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.491	88	2768	0.265	ng/ul#	46


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
Data File : BM037547.D
Acq On : 18 Nov 2022 03:56
Operator : CG/JU
Sample : N5623-02
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGCB9


Quant Time: Nov 18 04:54:55 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 17 23:00:56 2022
Response via : Initial Calibration

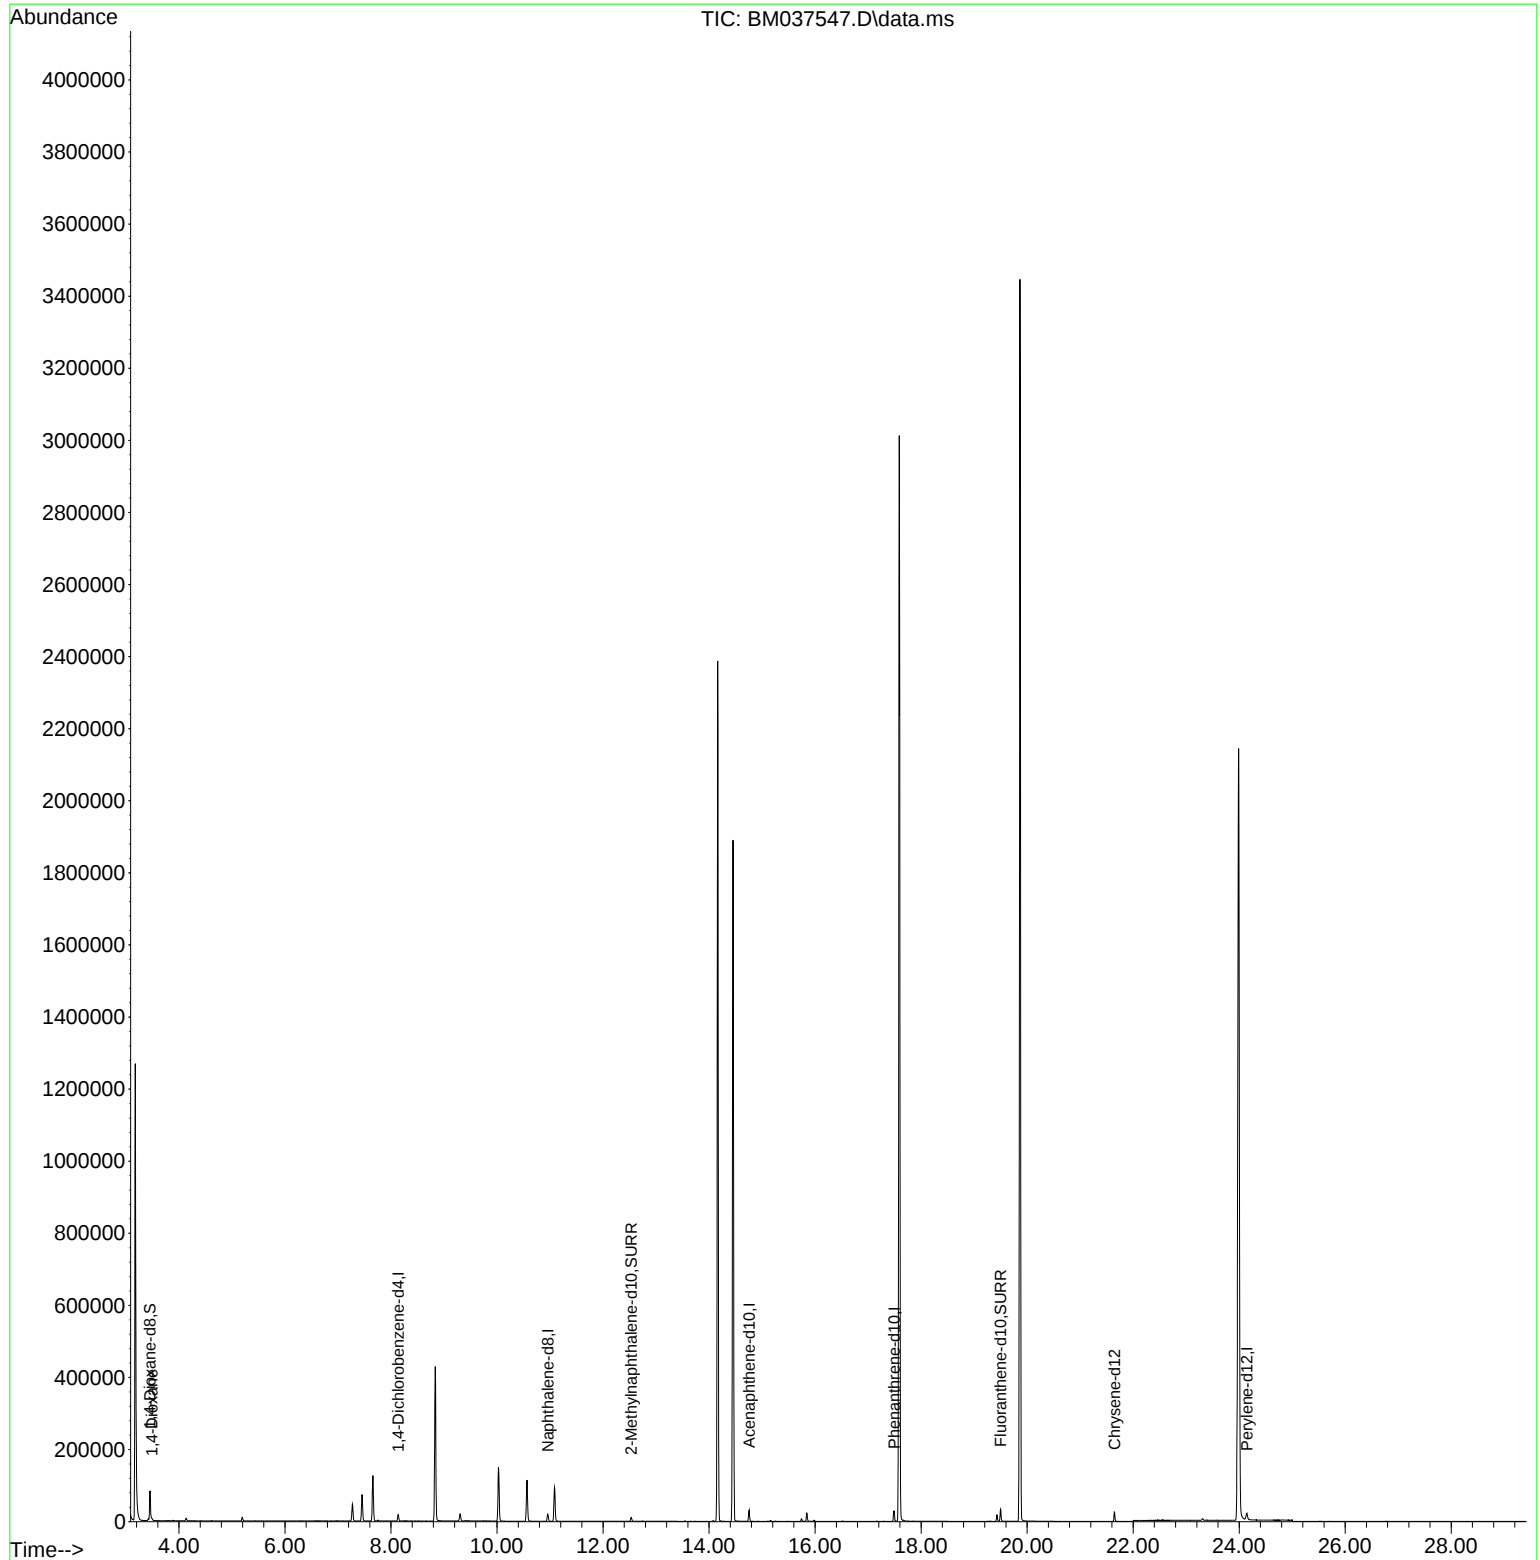

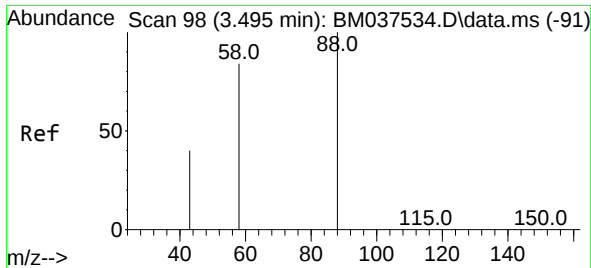

#2
 1,4-Dioxane
 Concen: 0.265 ng/ul
 RT: 3.491 min Scan# 91
 Delta R.T. -0.004 min
 Lab File: BM037547.D
 Acq: 18 Nov 2022 03:56

Instrument :
 BNA_M
 ClientSampleId :
 BGCB9

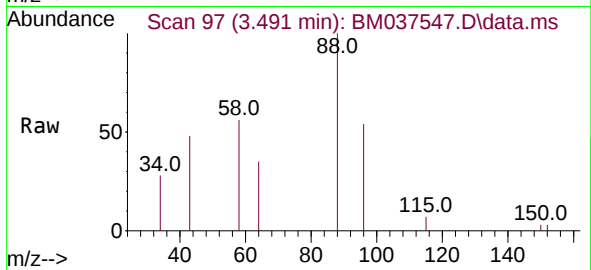

Tgt Ion: 88 Resp: 2768

Ion	Ratio	Lower	Upper
88	100		
43	47.7	102.8	154.2#
58	56.4	67.3	100.9#

