

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
 Data File : BM037548.D
 Acq On : 18 Nov 2022 04:32
 Operator : CG/JU
 Sample : N5623-03
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGCC0

Quant Time: Nov 18 05:21:37 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 17 23:00:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.136	152	6757	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.958	136	19396	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.756	164	12245	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.487	188	25769	0.400	ng/ul	-0.01
17) Chrysene-d12	21.648	240	18245	0.400	ng/ul	# 0.00
23) Perylene-d12	24.141	264	22002	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.453	96	31291	3.983	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.530	152	9186	0.286	ng/ul	-0.01
18) Fluoranthene-d10	19.499	212	23160	0.384	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.491	88	2027	0.248	ng/ul#	54


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
Data File : BM037548.D
Acq On : 18 Nov 2022 04:32
Operator : CG/JU
Sample : N5623-03
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGCC0

Quant Time: Nov 18 05:21:37 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 17 23:00:56 2022
Response via : Initial Calibration

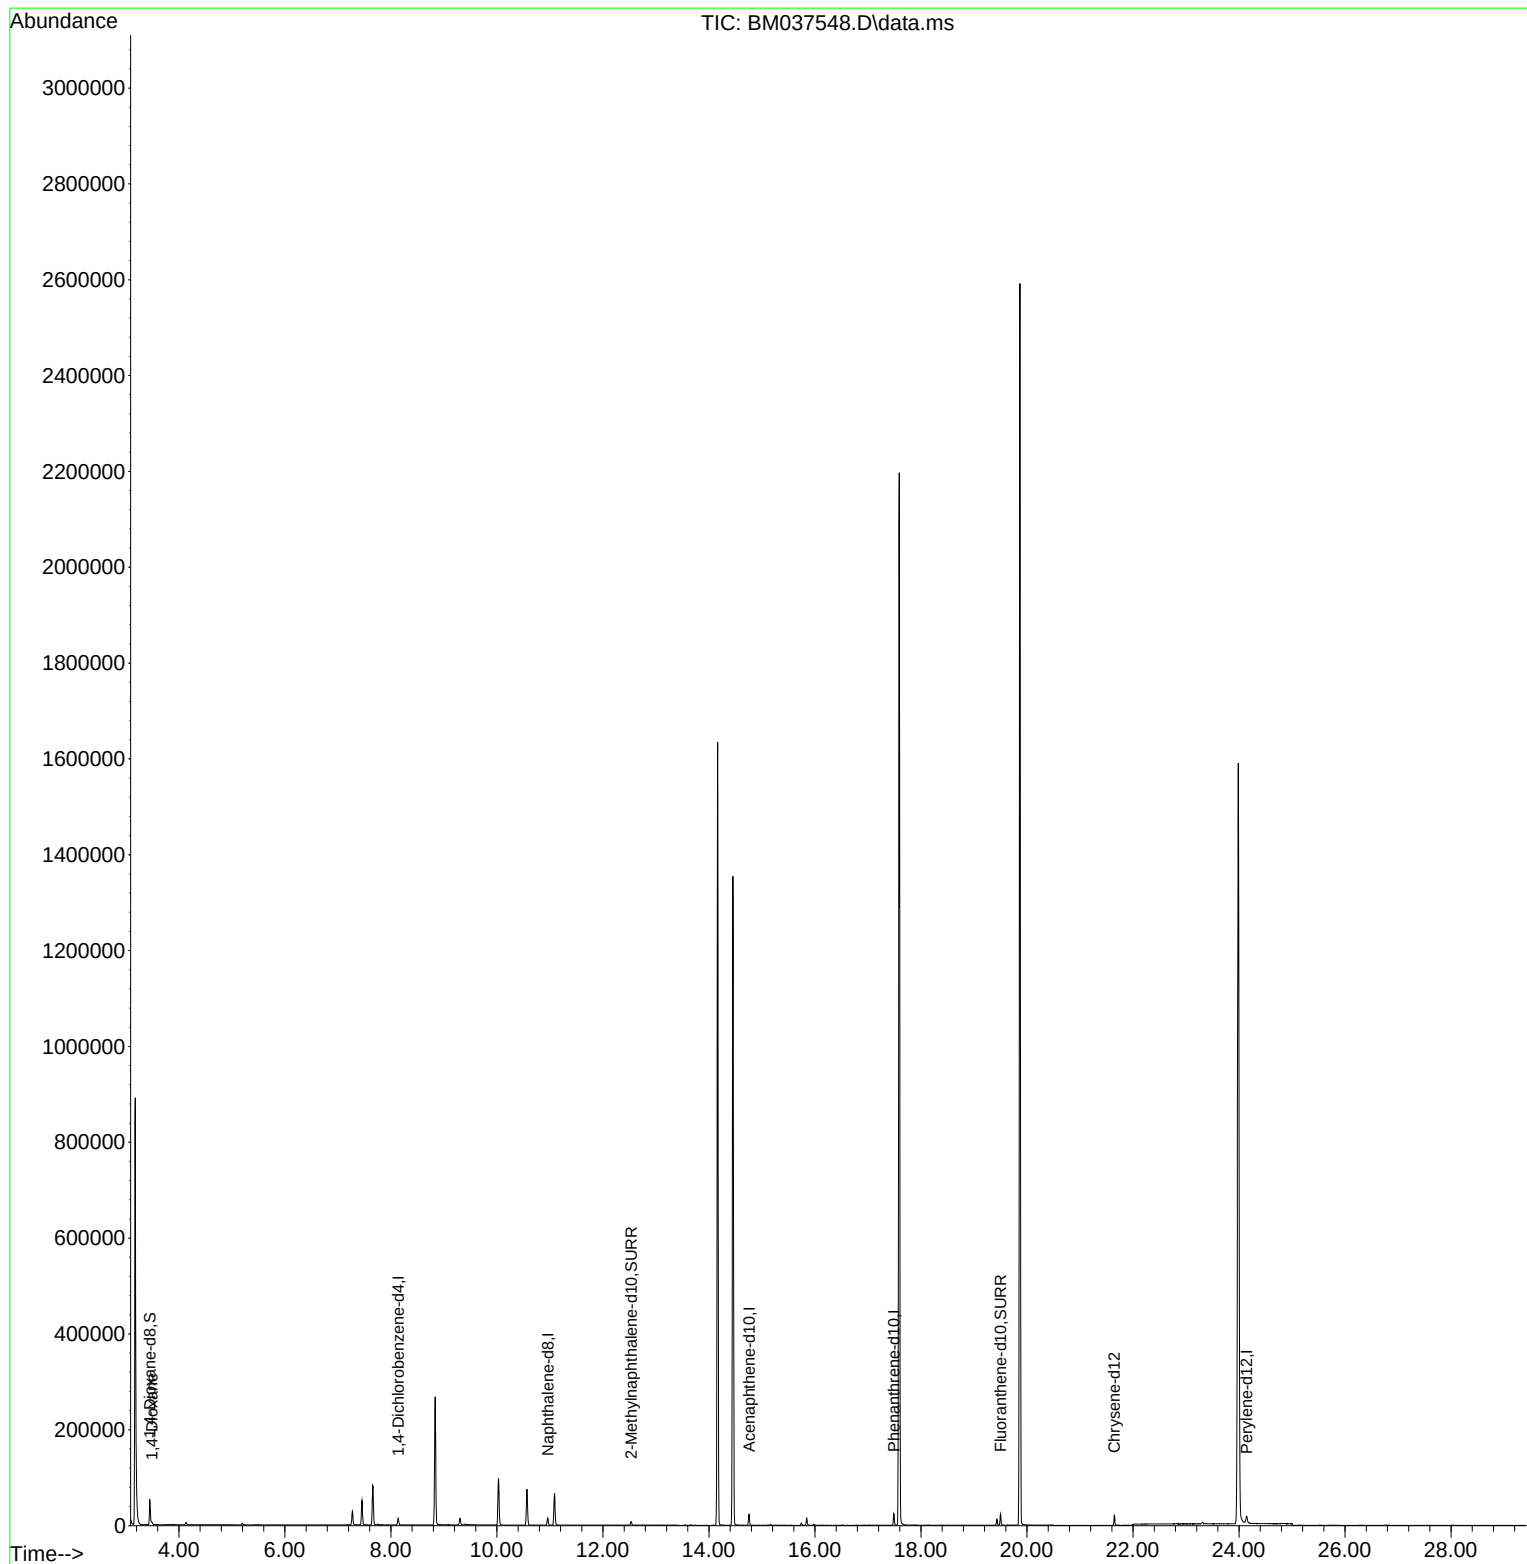

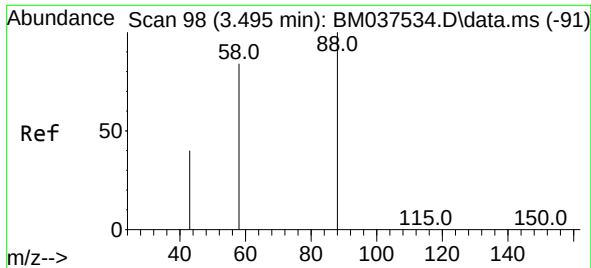

#2
 1,4-Dioxane
 Concen: 0.248 ng/ul
 RT: 3.491 min Scan# 91
 Delta R.T. -0.004 min
 Lab File: BM037548.D
 Acq: 18 Nov 2022 04:32

Instrument :
 BNA_M
 ClientSampleId :
 BGCC0

Tgt Ion: 88 Resp: 2027
 Ion Ratio Lower Upper
 88 100
 43 55.4 102.8 154.2#
 58 67.0 67.3 100.9#

