

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
 Data File : BM037554.D
 Acq On : 18 Nov 2022 08:44
 Operator : CG/JU
 Sample : N5577-01
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C9811

Quant Time: Nov 18 23:12:13 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 18 06:51:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.136	152	8903	0.400	ng/ul	0.00
4) Naphthalene-d8	10.957	136	25494	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.756	164	15994	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.487	188	35955	0.400	ng/ul	0.00
17) Chrysene-d12	21.648	240	27064	0.400	ng/ul	# 0.00
23) Perylene-d12	24.141	264	30064	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.453	96	40325	3.896	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.530	152	10540	0.249	ng/ul	0.00
18) Fluoranthene-d10	19.499	212	31286	0.350	ng/ul	0.00
Target Compounds						
						Qvalue
15) Phenanthrene	17.529	178	3024	0.025	ng/ul#	87
19) Fluoranthene	19.527	202	2677	0.021	ng/ul#	70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
Data File : BM037554.D
Acq On : 18 Nov 2022 08:44
Operator : CG/JU
Sample : N5577-01
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C9811

Quant Time: Nov 18 23:12:13 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 18 06:51:41 2022
Response via : Initial Calibration




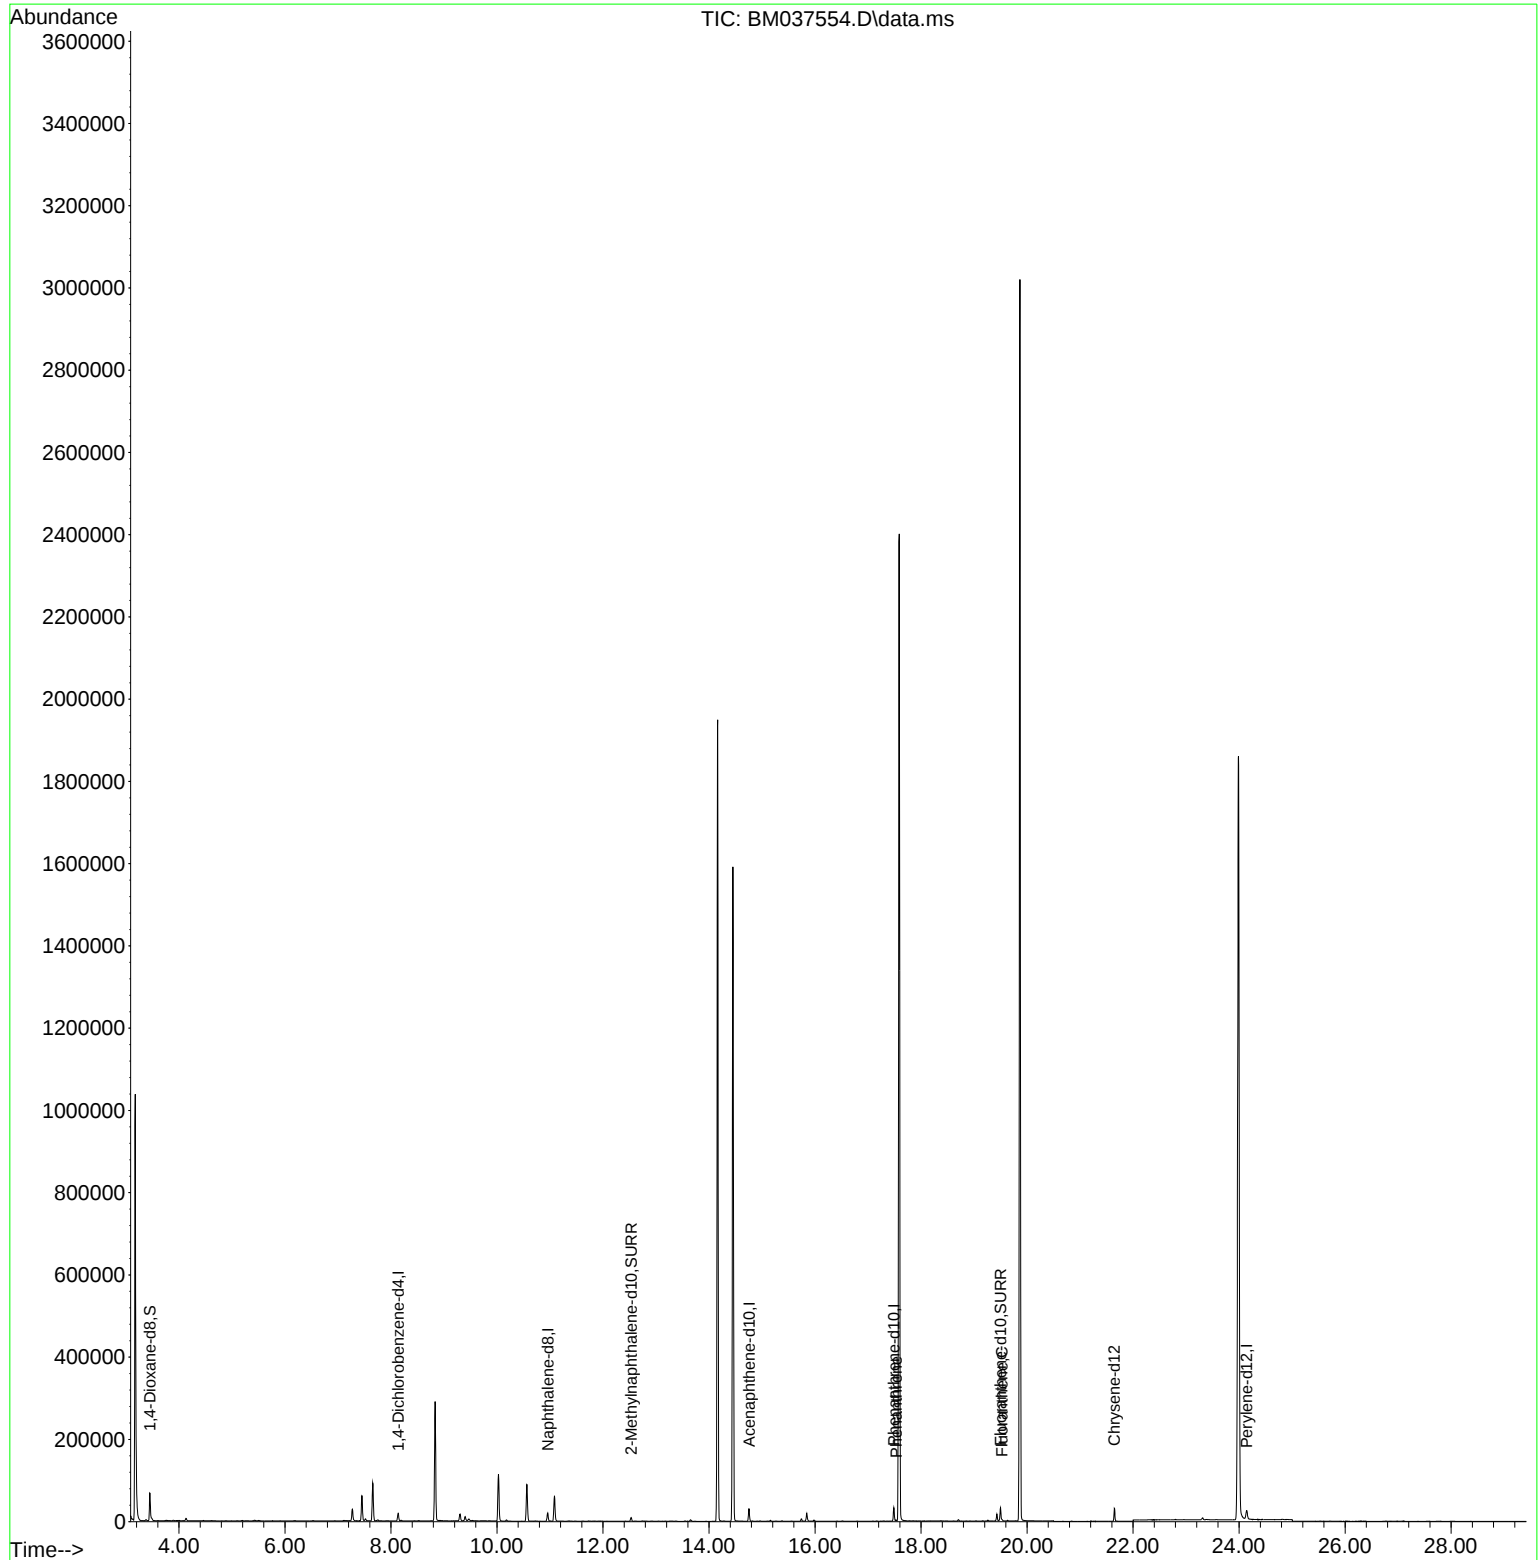


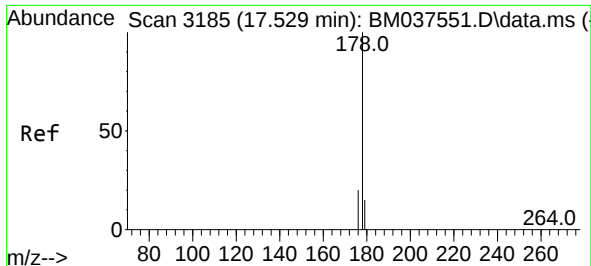

#15
Phenanthrene
Concen: 0.025 ng/ul
RT: 17.529 min Scan# 3185
Delta R.T. 0.001 min
Lab File: BM037554.D
Acq: 18 Nov 2022 08:44

Instrument :
BNA_M
ClientSampleId :
C9811

Tgt Ion:178 Resp: 3024
Ion Ratio Lower Upper
178 100
179 23.0 12.6 18.8#
176 24.4 16.0 24.0#

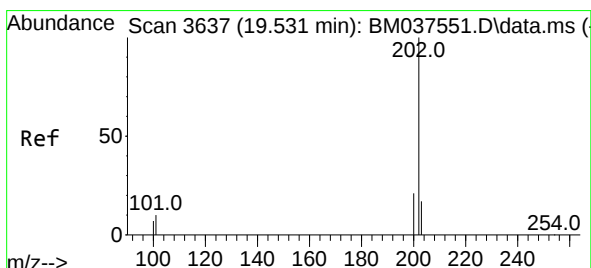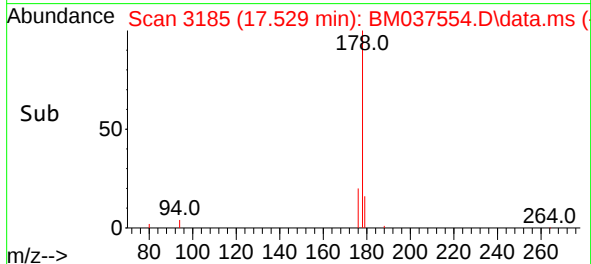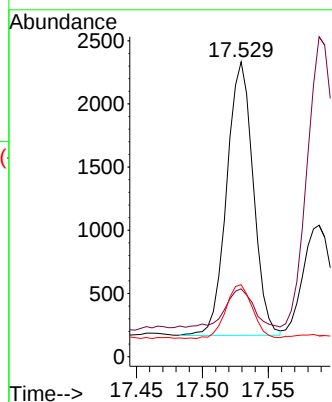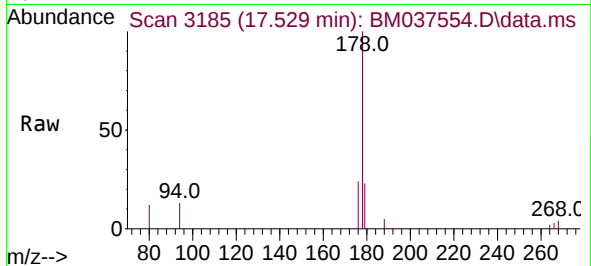

#19
Fluoranthene
Concen: 0.021 ng/ul
RT: 19.527 min Scan# 3636
Delta R.T. -0.004 min
Lab File: BM037554.D
Acq: 18 Nov 2022 08:44

Tgt Ion:202 Resp: 2677
Ion Ratio Lower Upper
202 100
101 21.1 8.2 12.2#
100 18.0 6.1 9.1#

