

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
 Data File : BM037557.D
 Acq On : 18 Nov 2022 10:33
 Operator : CG/JU
 Sample : N5577-04
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C9816

Quant Time: Nov 18 23:12:40 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 18 06:51:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.141	152	8508	0.400	ng/ul	0.00
4) Naphthalene-d8	10.957	136	25633	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.756	164	16249	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.491	188	35923	0.400	ng/ul	0.00
17) Chrysene-d12	21.651	240	26966	0.400	ng/ul	0.00
23) Perylene-d12	24.141	264	28782	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.453	96	43164	4.364	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.536	152	12331	0.290	ng/ul	0.00
18) Fluoranthene-d10	19.504	212	35808	0.402	ng/ul	0.00
Target Compounds						
						Qvalue
15) Phenanthrene	17.534	178	3180	0.026	ng/ul#	85
19) Fluoranthene	19.532	202	2759	0.021	ng/ul#	71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
Data File : BM037557.D
Acq On : 18 Nov 2022 10:33
Operator : CG/JU
Sample : N5577-04
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C9816

Quant Time: Nov 18 23:12:40 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 18 06:51:41 2022
Response via : Initial Calibration




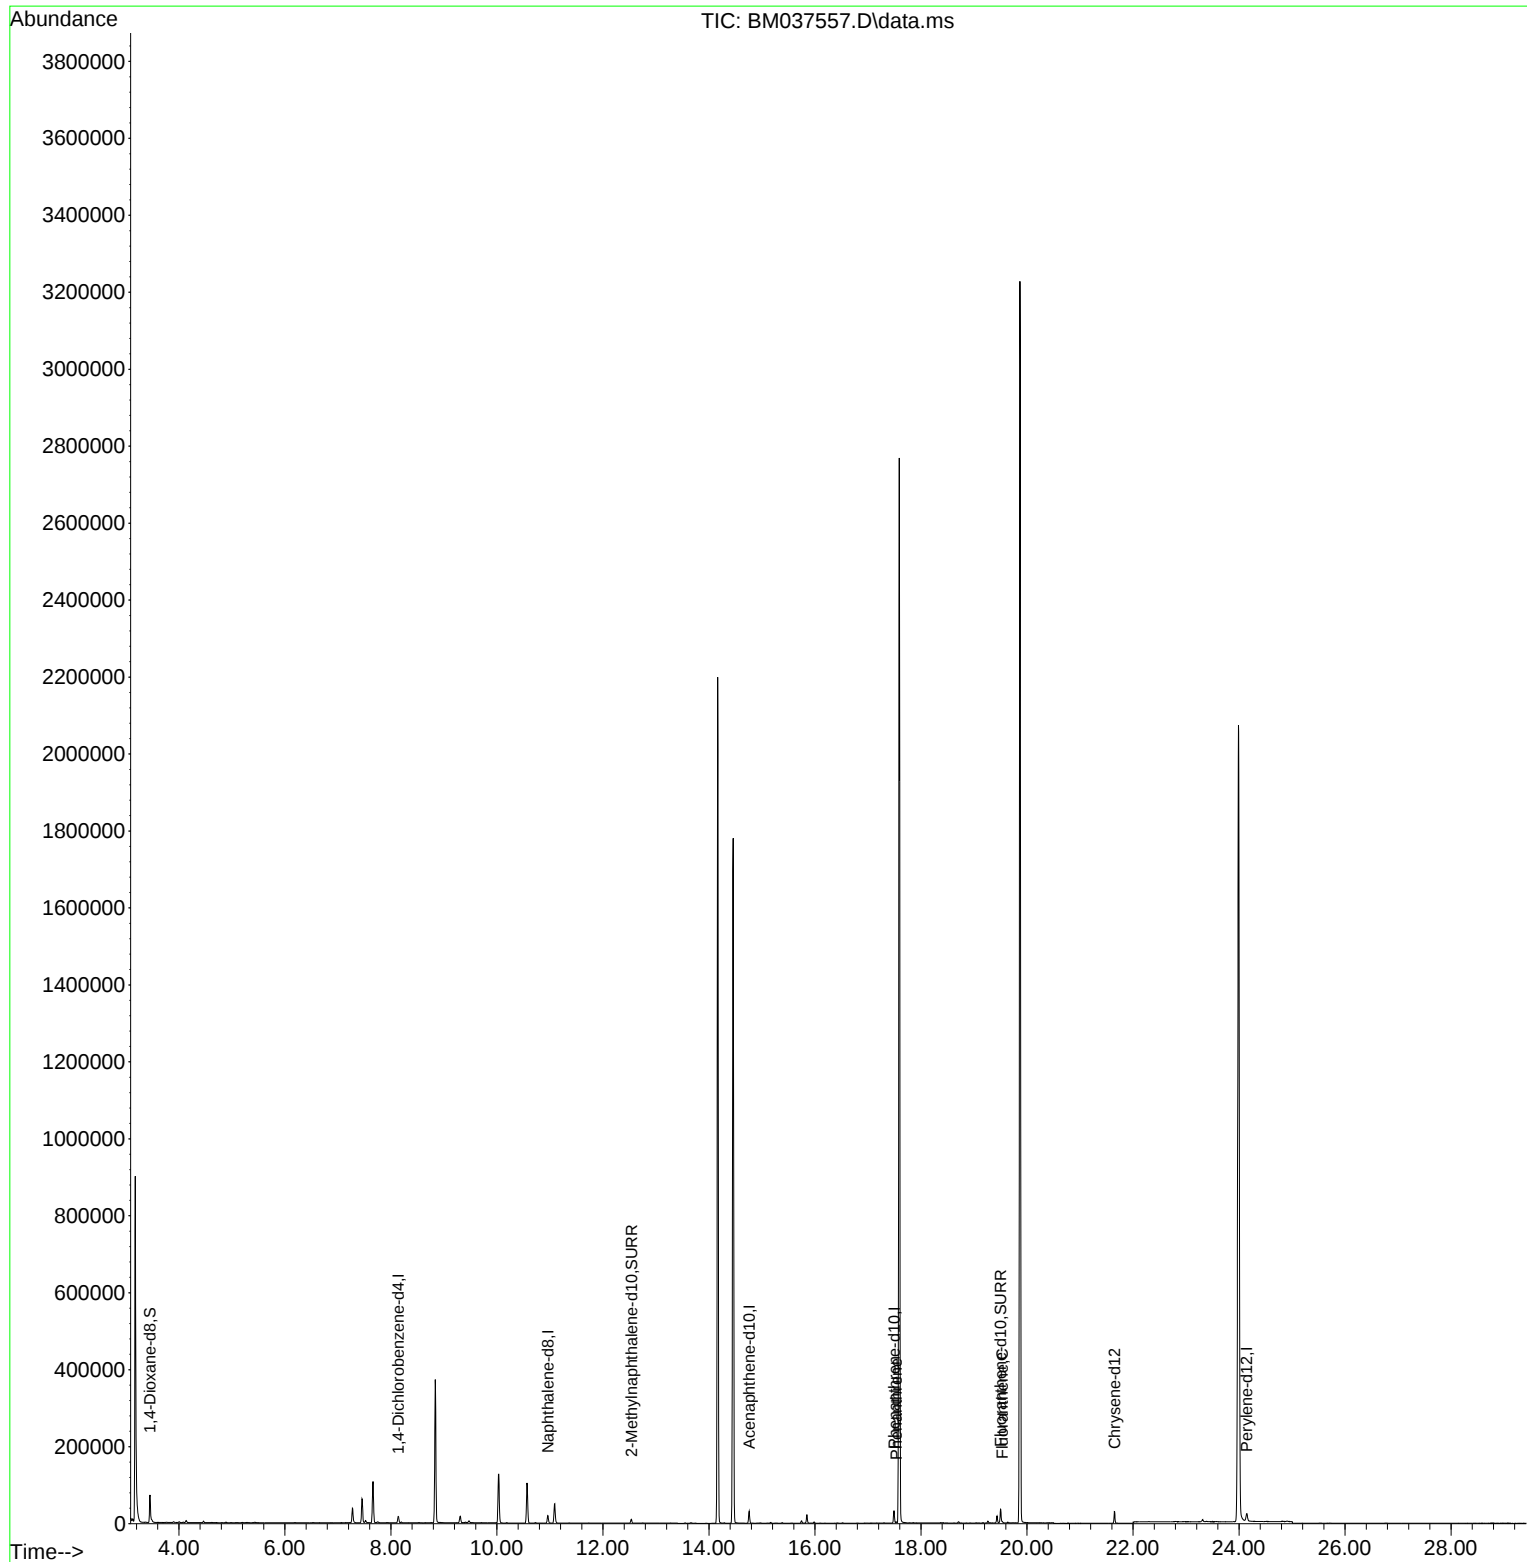


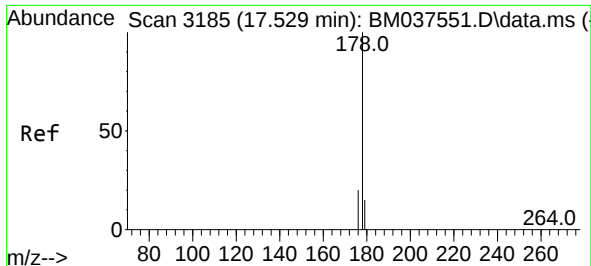

#15
Phenanthrene
Concen: 0.026 ng/ul
RT: 17.534 min Scan# 3185
Delta R.T. 0.005 min
Lab File: BM037557.D
Acq: 18 Nov 2022 10:33

Instrument :
BNA_M
ClientSampleId :
C9816

Tgt Ion:178	Resp:	3180
Ion Ratio	Lower	Upper
178	100	
179	25.7	12.6 18.8#
176	23.5	16.0 24.0

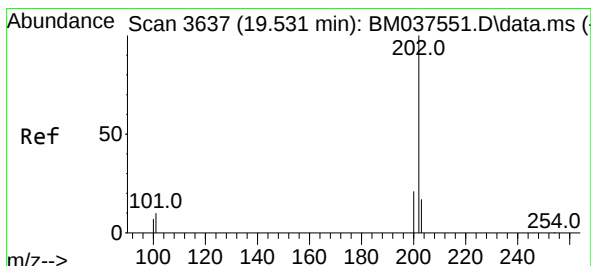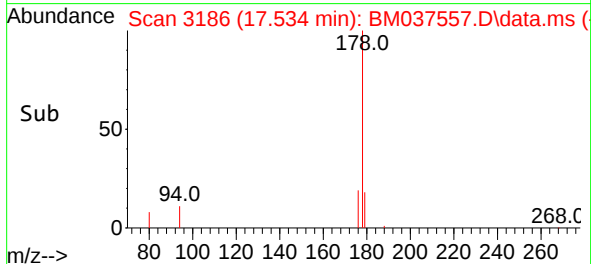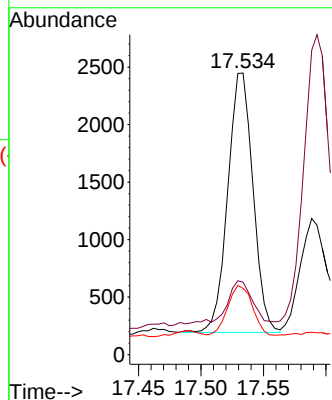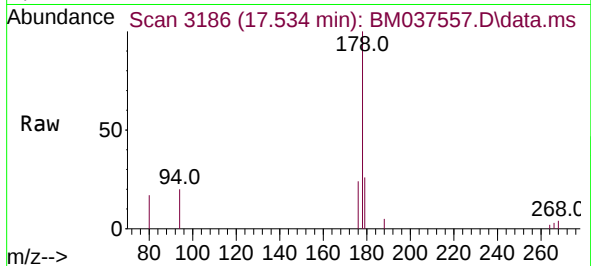

#19
Fluoranthene
Concen: 0.021 ng/ul
RT: 19.532 min Scan# 3637
Delta R.T. 0.001 min
Lab File: BM037557.D
Acq: 18 Nov 2022 10:33

Tgt Ion:202	Resp:	2759
Ion Ratio	Lower	Upper
202	100	
101	21.0	8.2 12.2#
100	17.8	6.1 9.1#

