

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
 Data File : BM037560.D
 Acq On : 18 Nov 2022 12:23
 Operator : CG/JU
 Sample : N5577-07
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C9820

Quant Time: Nov 18 23:12:59 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 18 06:51:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.136	152	7893	0.400	ng/ul	0.00
4) Naphthalene-d8	10.957	136	23473	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.756	164	14804	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.487	188	32770	0.400	ng/ul	0.00
17) Chrysene-d12	21.648	240	24498	0.400	ng/ul	0.00
23) Perylene-d12	24.144	264	26811	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.453	96	33744	3.677	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.530	152	10847	0.279	ng/ul	0.00
18) Fluoranthene-d10	19.499	212	33618	0.415	ng/ul	0.00
Target Compounds						
						Qvalue
15) Phenanthrene	17.529	178	3254	0.029	ng/ul#	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
Data File : BM037560.D
Acq On : 18 Nov 2022 12:23
Operator : CG/JU
Sample : N5577-07
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C9820


Quant Time: Nov 18 23:12:59 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 18 06:51:41 2022
Response via : Initial Calibration

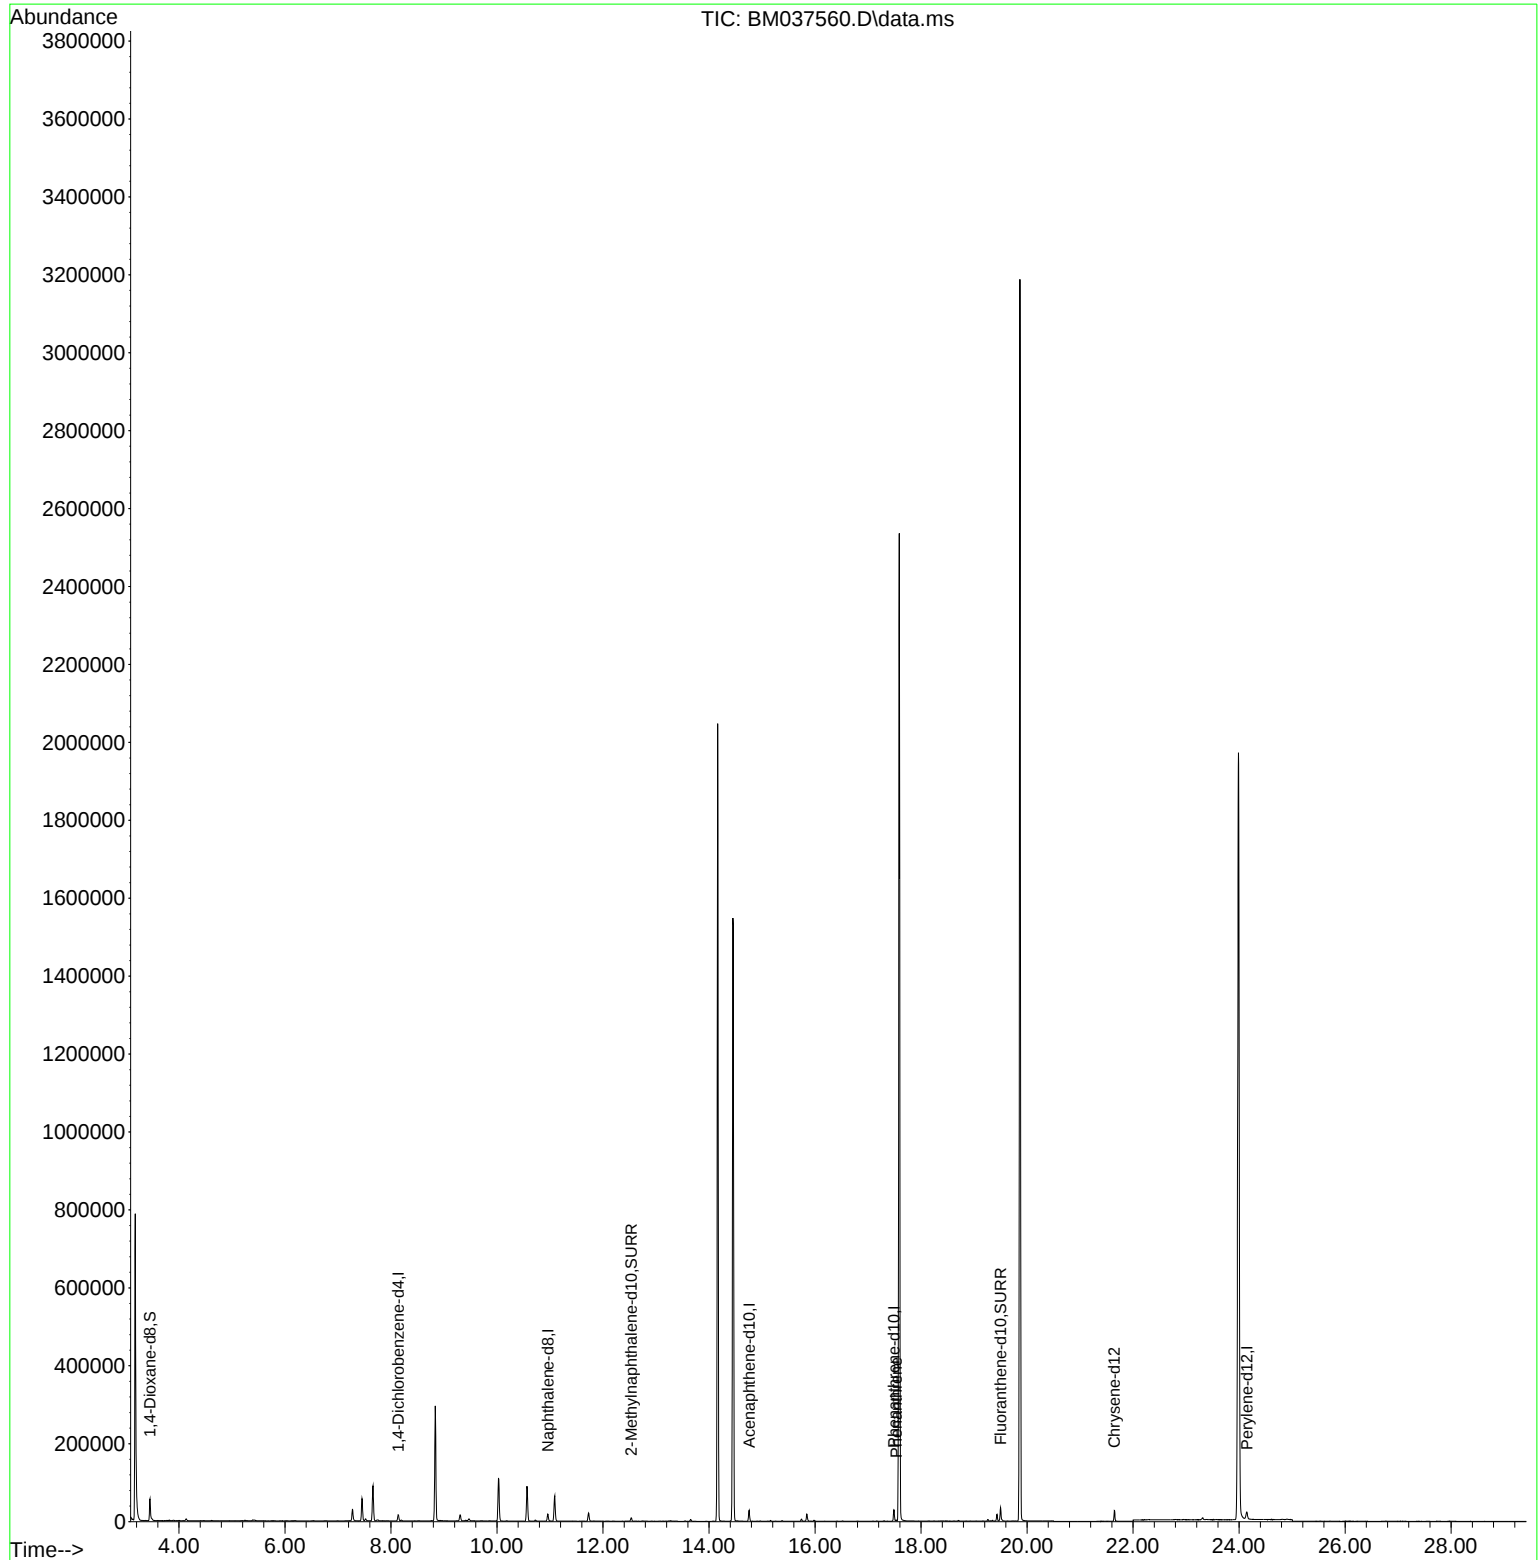

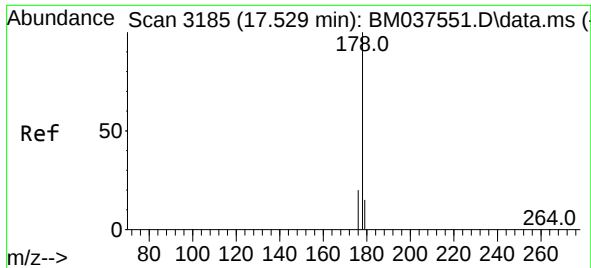

#15
 Phenanthrene
 Concen: 0.029 ng/ul
 RT: 17.529 min Scan# 31
 Delta R.T. 0.001 min
 Lab File: BM037560.D
 Acq: 18 Nov 2022 12:23

Instrument :
 BNA_M
 ClientSampleId :
 C9820

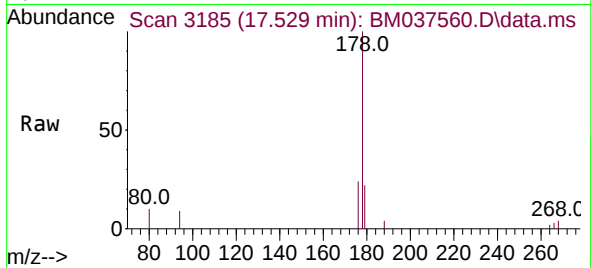

Tgt Ion:	178	Resp:	3254
Ion	Ratio	Lower	Upper
178	100		
179	22.2	12.6	18.8#
176	23.9	16.0	24.0

