

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
 Data File : BM037562.D
 Acq On : 18 Nov 2022 13:36
 Operator : CG/JU
 Sample : N5589-01
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C9813

Quant Time: Nov 18 23:13:11 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 18 06:51:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.140	152	7922	0.400	ng/ul	0.00
4) Naphthalene-d8	10.957	136	23487	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.756	164	14708	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.491	188	32601	0.400	ng/ul	0.00
17) Chrysene-d12	21.648	240	25006	0.400	ng/ul	0.00
23) Perylene-d12	24.144	264	26487	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.453	96	39587	4.298	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.536	152	10902	0.280	ng/ul	0.00
18) Fluoranthene-d10	19.499	212	36033	0.436	ng/ul	0.00
Target Compounds						
15) Phenanthrene	17.529	178	3293	0.030	ng/ul#	Qvalue 83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
Data File : BM037562.D
Acq On : 18 Nov 2022 13:36
Operator : CG/JU
Sample : N5589-01
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C9813


Quant Time: Nov 18 23:13:11 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 18 06:51:41 2022
Response via : Initial Calibration

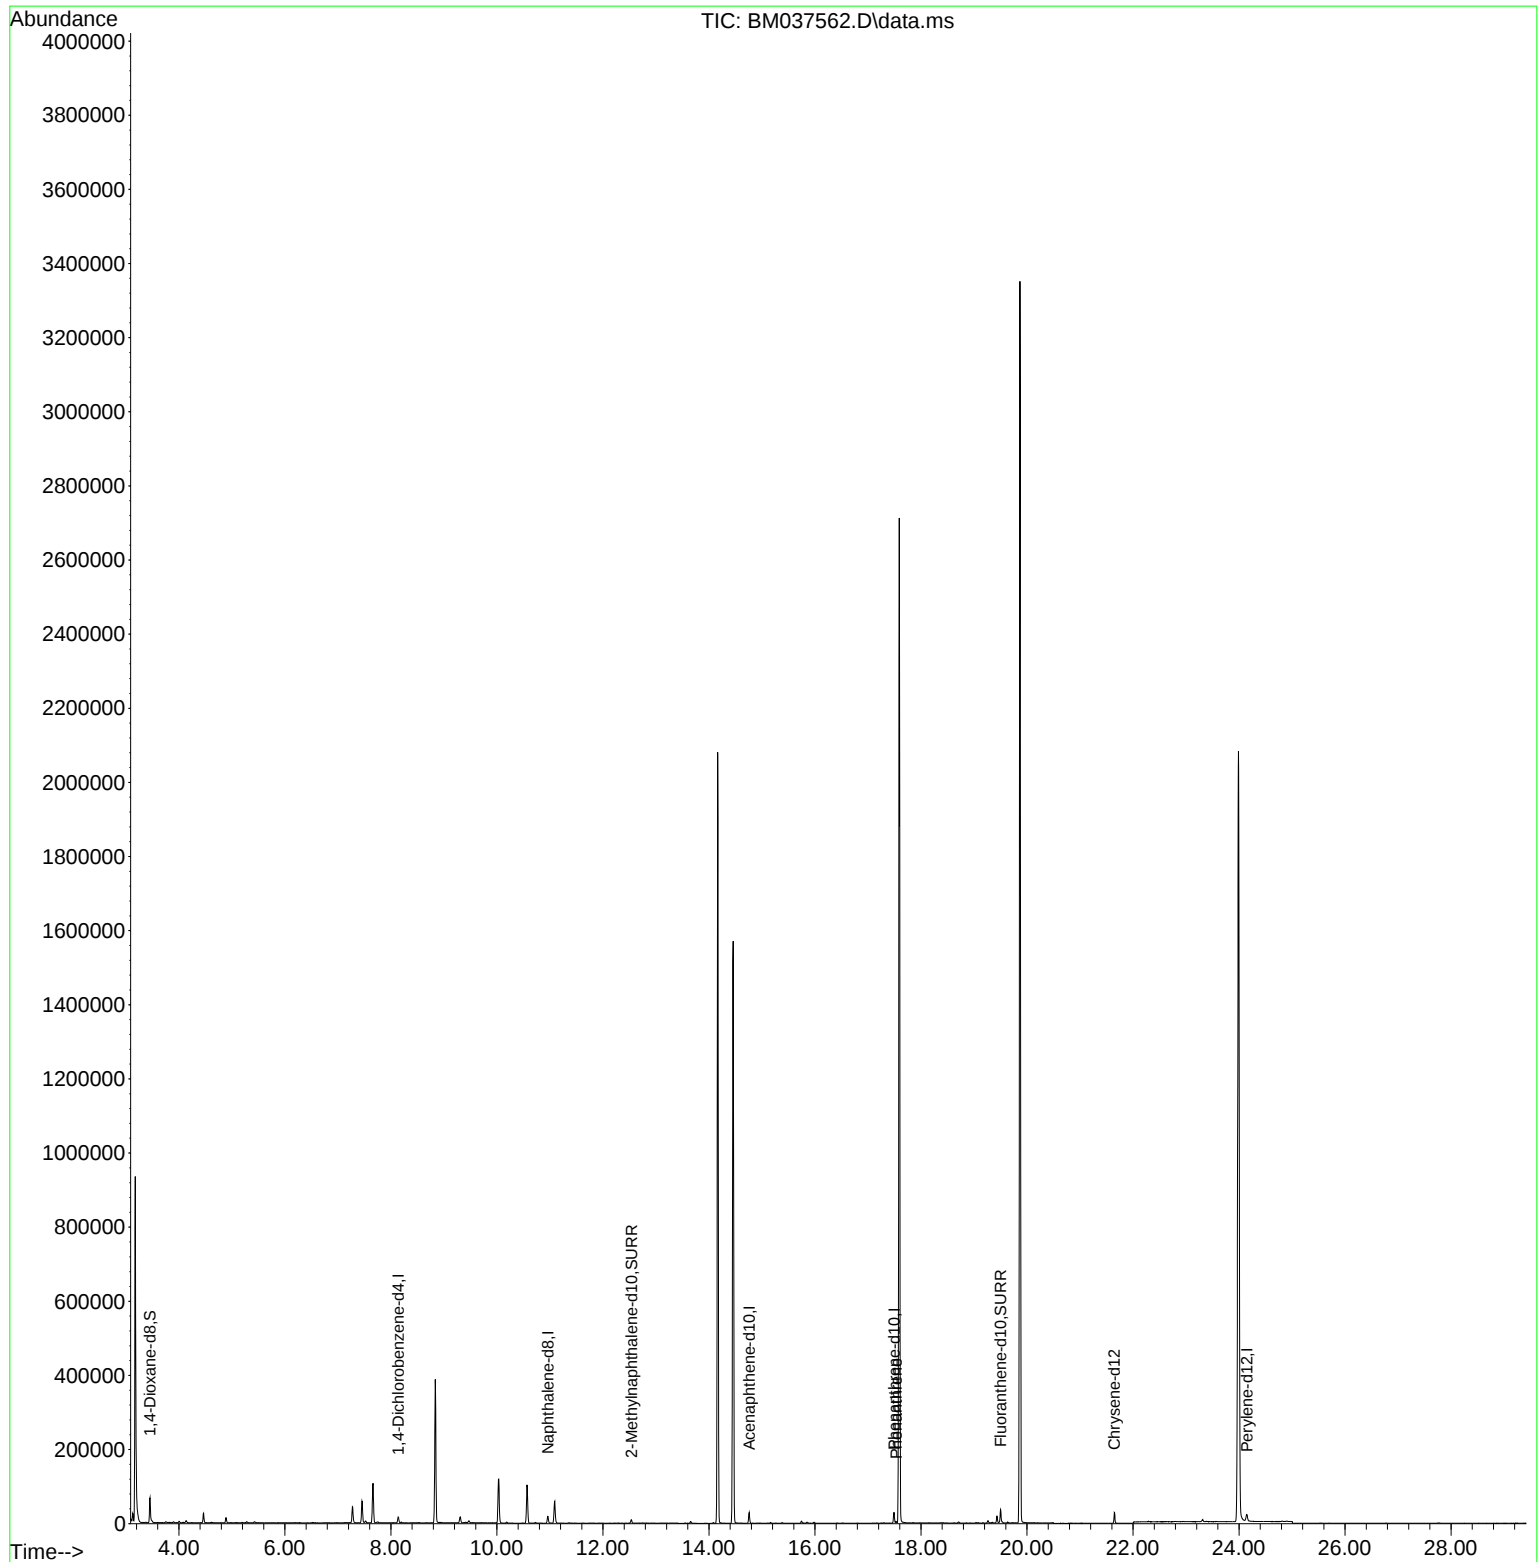

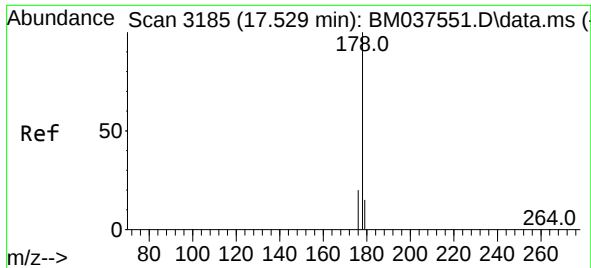

#15
 Phenanthrene
 Concen: 0.030 ng/ul
 RT: 17.529 min Scan# 31
 Delta R.T. 0.001 min
 Lab File: BM037562.D
 Acq: 18 Nov 2022 13:36

Instrument :
 BNA_M
 ClientSampleId :
 C9813

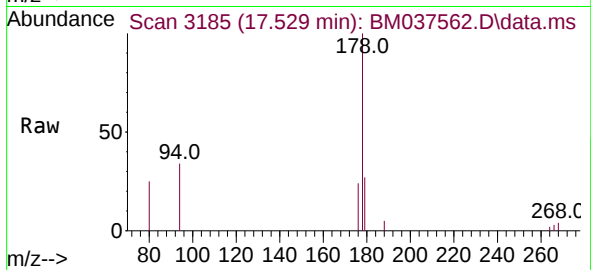

Tgt Ion:	178	Resp:	3293
Ion Ratio	Lower	Upper	
178	100		
179	27.1	12.6	18.8#
176	24.3	16.0	24.0#

