

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
 Data File : BM037576.D
 Acq On : 18 Nov 2022 22:49
 Operator : CG/JU
 Sample : N5689-01
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGCC4

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 11/21/2022
 Supervised By :mohammad ahmed 11/21/2022

Quant Time: Nov 18 23:43:25 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 18 06:51:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.136	152	6939	0.400	ng/u1	0.00
4) Naphthalene-d8	10.957	136	20432	0.400	ng/u1	# 0.00
9) Acenaphthene-d10	14.755	164	13071	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.486	188	27630	0.400	ng/u1	0.00
17) Chrysene-d12	21.646	240	20869	0.400	ng/u1	# 0.00
23) Perylene-d12	24.139	264	24304	0.400	ng/u1	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.453	96	32009m	3.968	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.530	152	9661	0.285	ng/u1	0.00
18) Fluoranthene-d10	19.498	212	23033	0.334	ng/u1	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.491	88	1704	0.203	ng/u1#	59

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
Data File : BM037576.D
Acq On : 18 Nov 2022 22:49
Operator : CG/JU
Sample : N5689-01
Misc :
ALS Vial : 62 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BGCC4

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 11/21/2022
Supervised By :mohammad ahmed 11/21/2022


Quant Time: Nov 18 23:43:25 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 18 06:51:41 2022
Response via : Initial Calibration

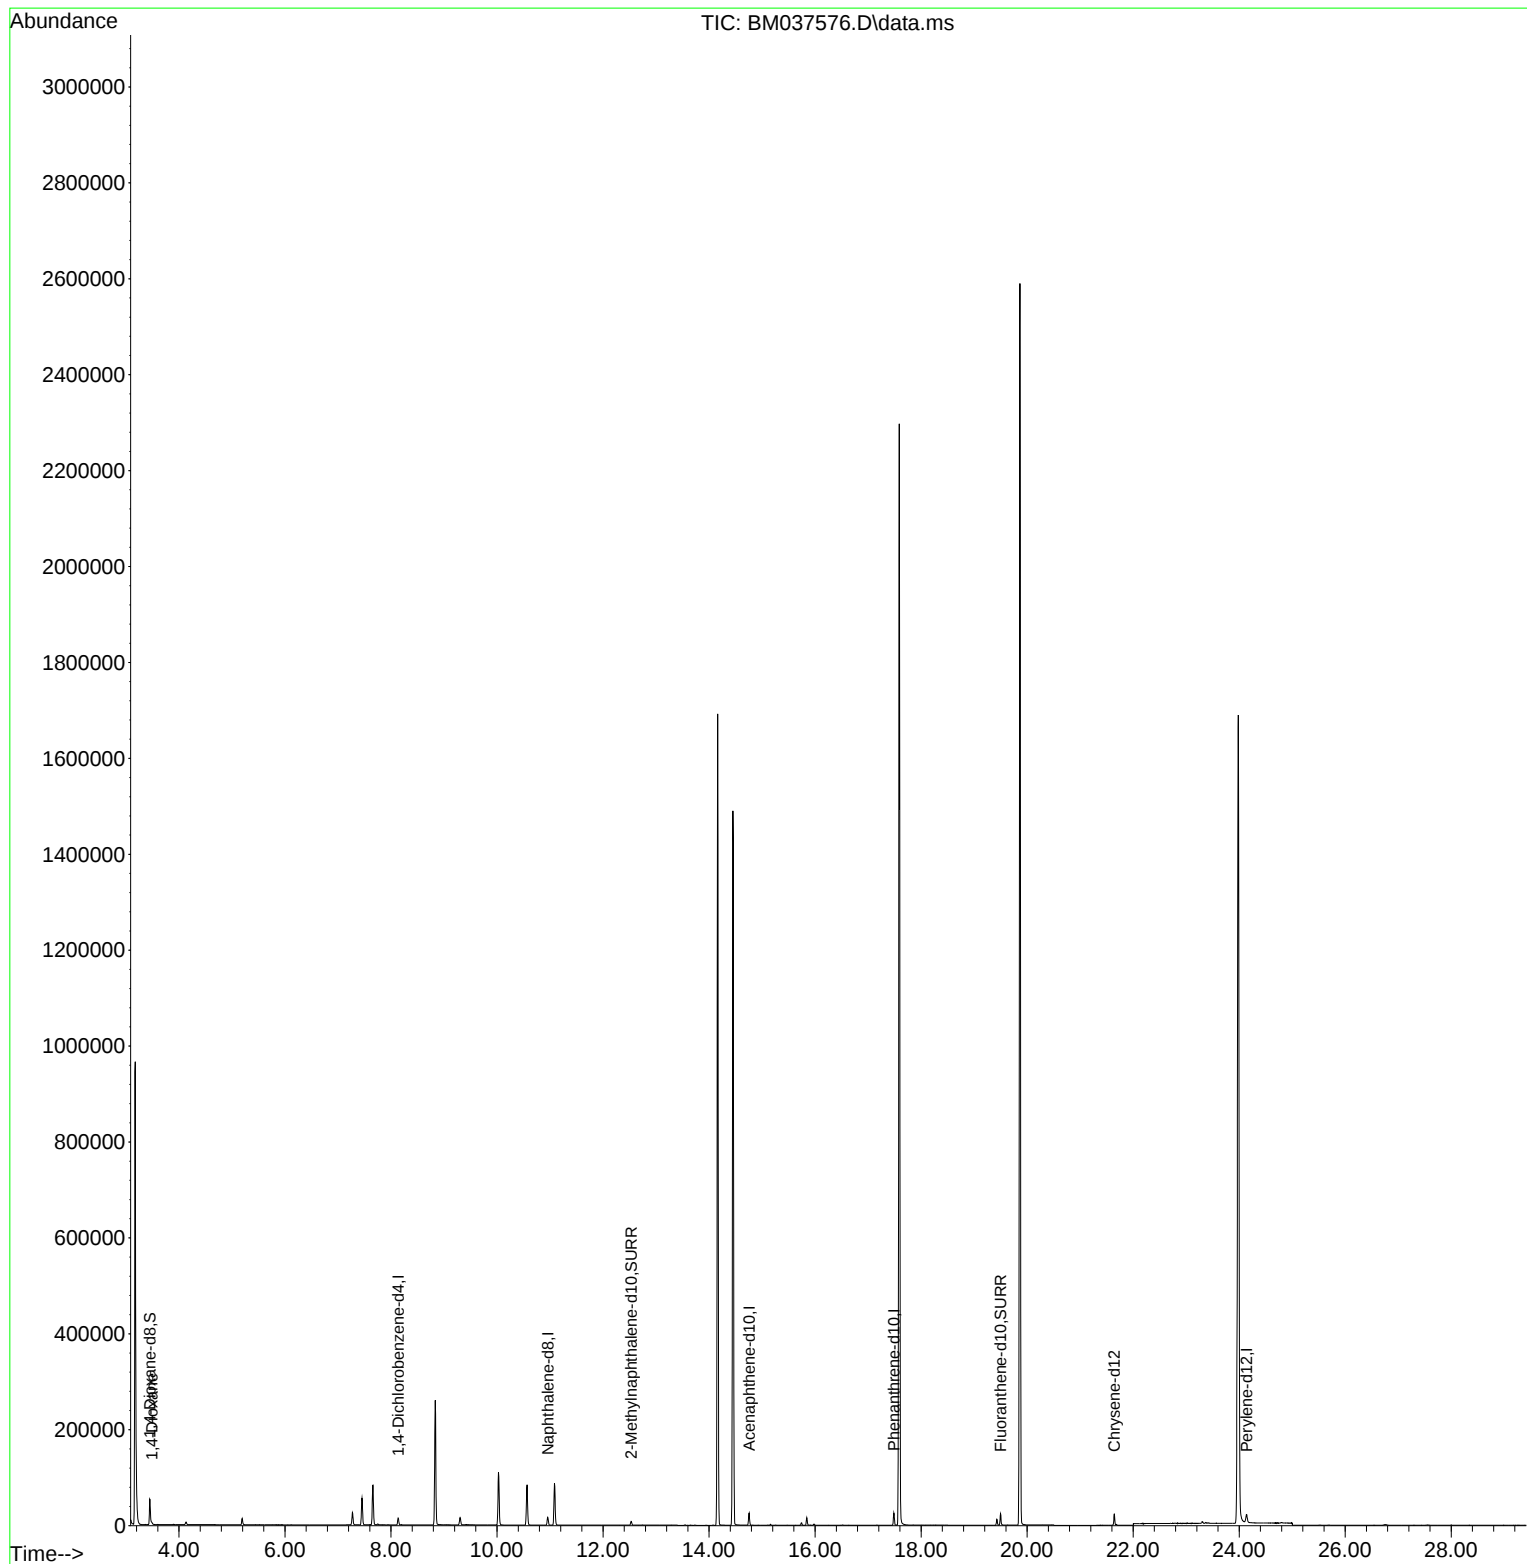

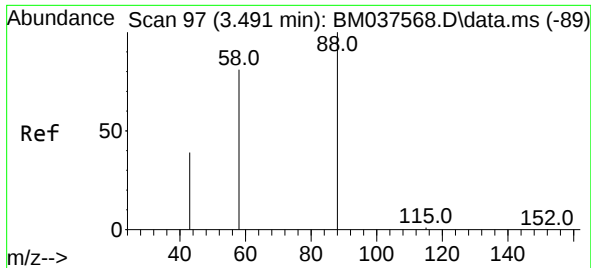

#2
 1,4-Dioxane
 Concen: 0.203 ng/ul
 RT: 3.491 min Scan# 91
 Delta R.T. -0.000 min
 Lab File: BM037576.D
 Acq: 18 Nov 2022 22:49

Instrument :
 BNA_M
 ClientSampleId :
 BGCC4

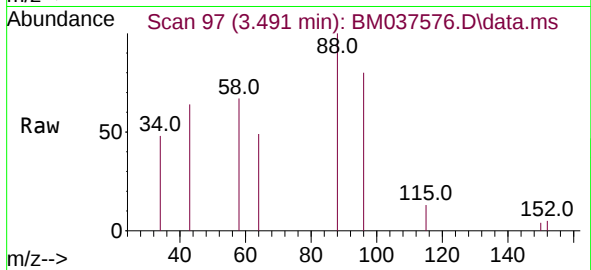

Tgt Ion: 88 Resp: 1704
 Ion Ratio Lower Upper
 88 100
 43 64.1 102.8 154.2
 58 66.9 67.3 100.9

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 11/21/2022
 Supervised By :mohammad ahmed 11/21/2022

