

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM111722\  
 Data File : BM037578.D  
 Acq On : 19 Nov 2022 00:02  
 Operator : CG/JU  
 Sample : N5689-03  
 Misc :  
 ALS Vial : 64 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 BGCC6

Quant Time: Nov 19 00:54:14 2022  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SFAM-EPA-SIM-BM111622.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Nov 18 06:51:41 2022  
 Response via : Initial Calibration


| Compound                    | R.T.   | QIon | Response | Conc  | Units  | Dev(Min) |
|-----------------------------|--------|------|----------|-------|--------|----------|
| -----                       |        |      |          |       |        |          |
| Internal Standards          |        |      |          |       |        |          |
| 1) 1,4-Dichlorobenzene-d4   | 8.136  | 152  | 7162     | 0.400 | ng/ul  | 0.00     |
| 4) Naphthalene-d8           | 10.958 | 136  | 20763    | 0.400 | ng/ul  | # 0.00   |
| 9) Acenaphthene-d10         | 14.756 | 164  | 13107    | 0.400 | ng/ul  | 0.00     |
| 13) Phenanthrene-d10        | 17.486 | 188  | 27534    | 0.400 | ng/ul  | 0.00     |
| 17) Chrysene-d12            | 21.643 | 240  | 20463    | 0.400 | ng/ul  | # 0.00   |
| 23) Perylene-d12            | 24.137 | 264  | 23091    | 0.400 | ng/ul  | # 0.00   |
| System Monitoring Compounds |        |      |          |       |        |          |
| 3) 1,4-Dioxane-d8           | 3.449  | 96   | 41379    | 4.969 | ng/ul  | 0.00     |
| 6) 2-Methylnaphthalene-d10  | 12.530 | 152  | 11012    | 0.320 | ng/ul  | 0.00     |
| 18) Fluoranthene-d10        | 19.498 | 212  | 26013    | 0.385 | ng/ul  | 0.00     |
| Target Compounds            |        |      |          |       |        |          |
|                             |        |      |          |       |        | Qvalue   |
| 2) 1,4-Dioxane              | 3.491  | 88   | 2817     | 0.325 | ng/ul# | 56       |
| -----                       |        |      |          |       |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM111722\  
Data File : BM037578.D  
Acq On : 19 Nov 2022 00:02  
Operator : CG/JU  
Sample : N5689-03  
Misc :  
ALS Vial : 64 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
BGCC6

Quant Time: Nov 19 00:54:14 2022  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SFAM-EPA-SIM-BM111622.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Nov 18 06:51:41 2022  
Response via : Initial Calibration

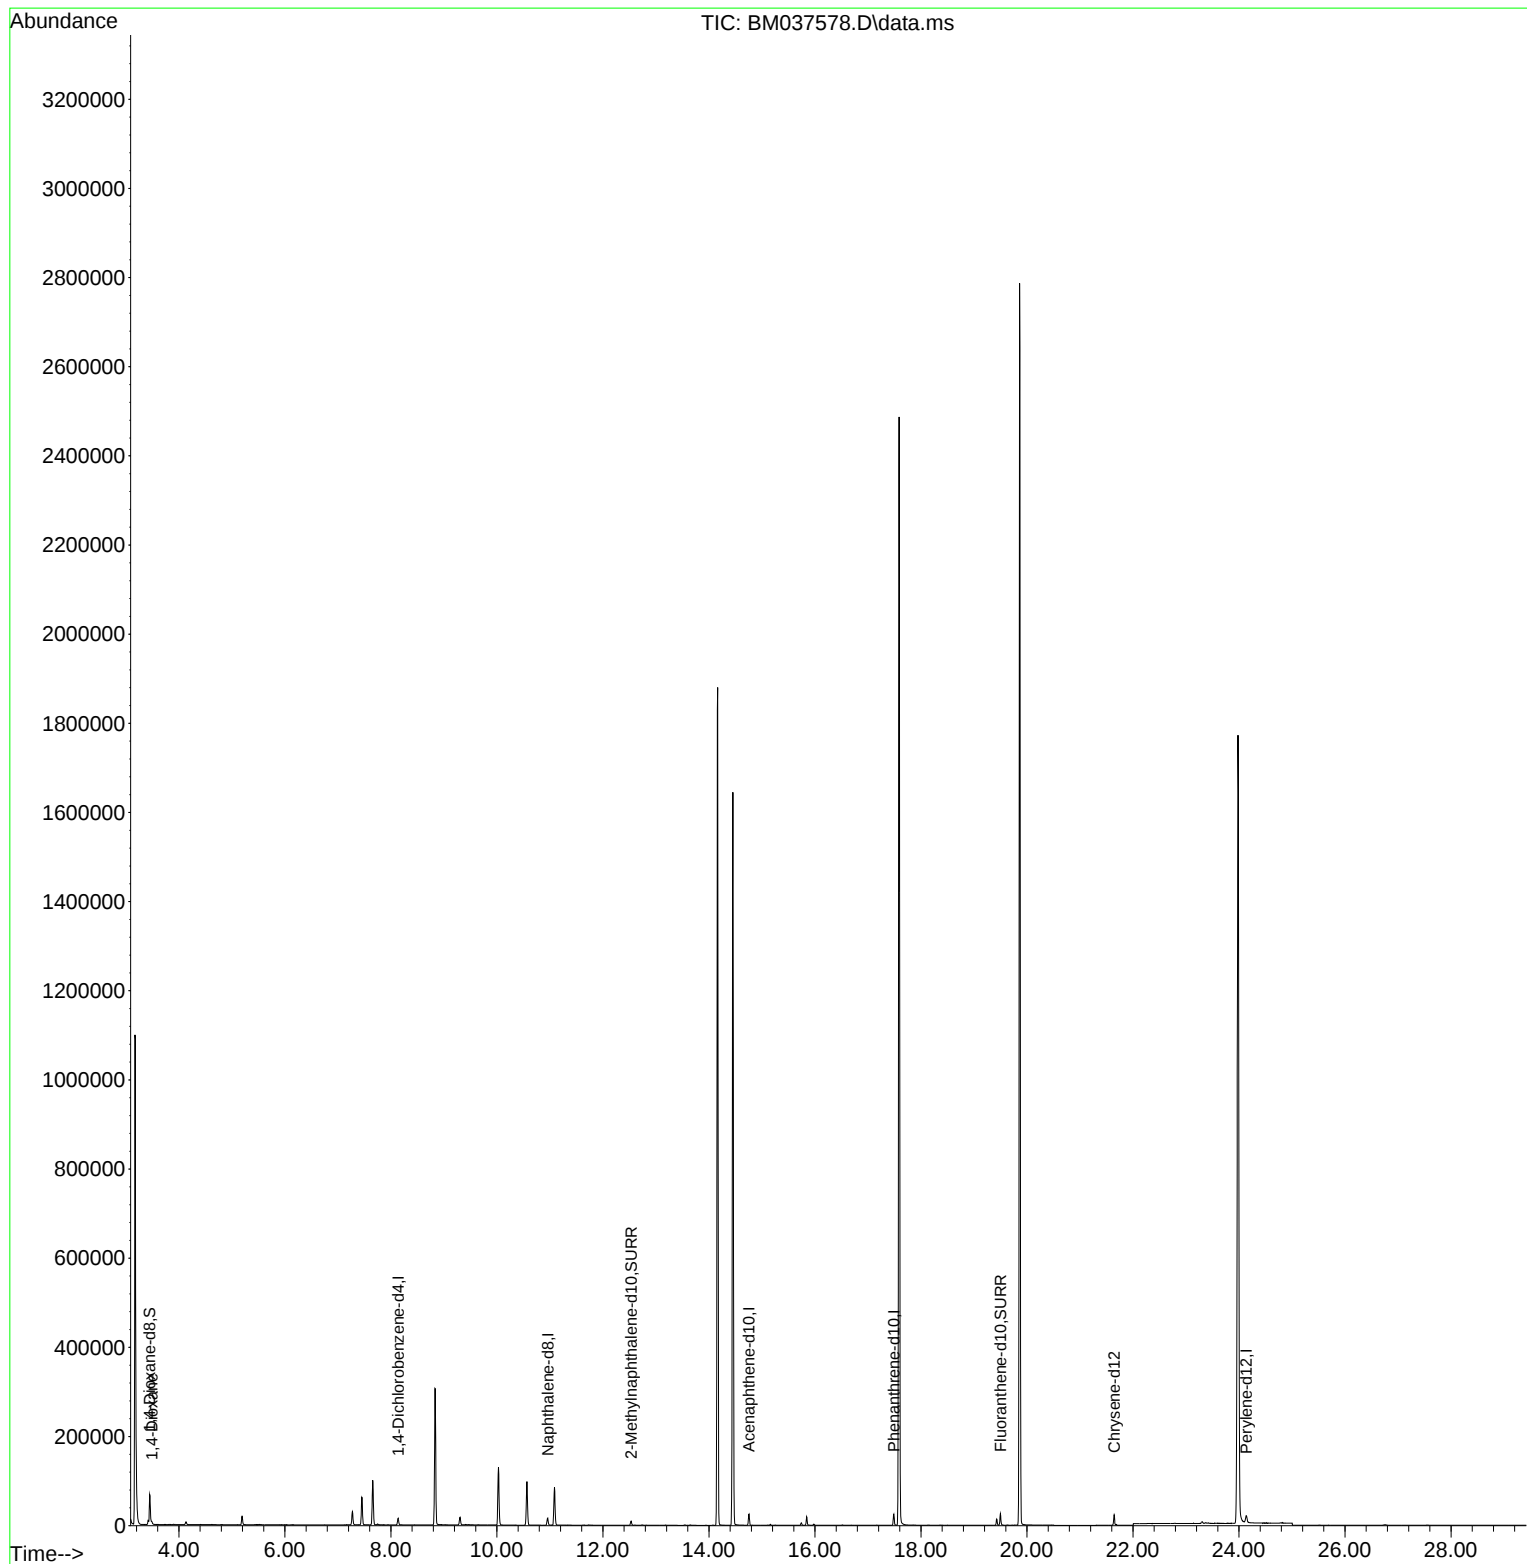

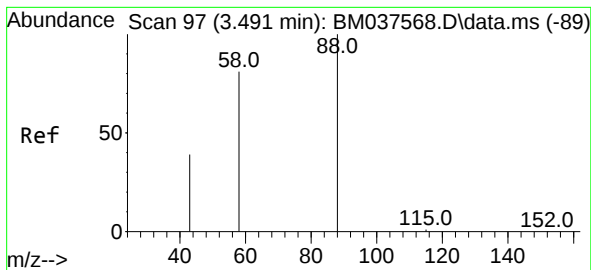

#2

1,4-Dioxane

Concen: 0.325 ng/ul

RT: 3.491 min Scan# 91

Delta R.T. 0.000 min

Lab File: BM037578.D


Acq: 19 Nov 2022 00:02

Instrument :

BNA\_M

ClientSampleId :

BGCC6

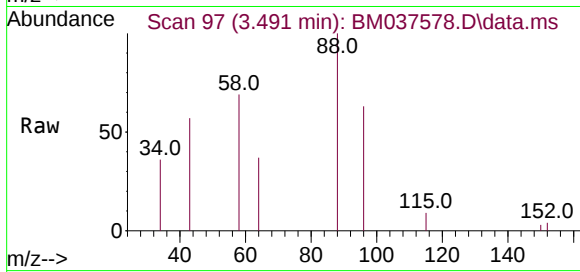

Tgt Ion: 88 Resp: 2817

Ion Ratio Lower Upper

88 100

43 57.0 102.8 154.2#

58 68.5 67.3 100.9

