

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
 Data File : BM037580.D
 Acq On : 19 Nov 2022 01:15
 Operator : CG/JU
 Sample : N5689-05
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGCC8

Quant Time: Nov 19 01:48:01 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 18 06:51:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.136	152	7480	0.400	ng/ul	0.00
4) Naphthalene-d8	10.957	136	22035	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.752	164	13953	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.487	188	28963	0.400	ng/ul	0.00
17) Chrysene-d12	21.642	240	20985	0.400	ng/ul	# 0.00
23) Perylene-d12	24.136	264	23089	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.453	96	44012	5.061	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.530	152	12269	0.336	ng/ul	0.00
18) Fluoranthene-d10	19.499	212	28106	0.405	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.491	88	2540	0.281	ng/ul#	53


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
Data File : BM037580.D
Acq On : 19 Nov 2022 01:15
Operator : CG/JU
Sample : N5689-05
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGCC8

Quant Time: Nov 19 01:48:01 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 18 06:51:41 2022
Response via : Initial Calibration

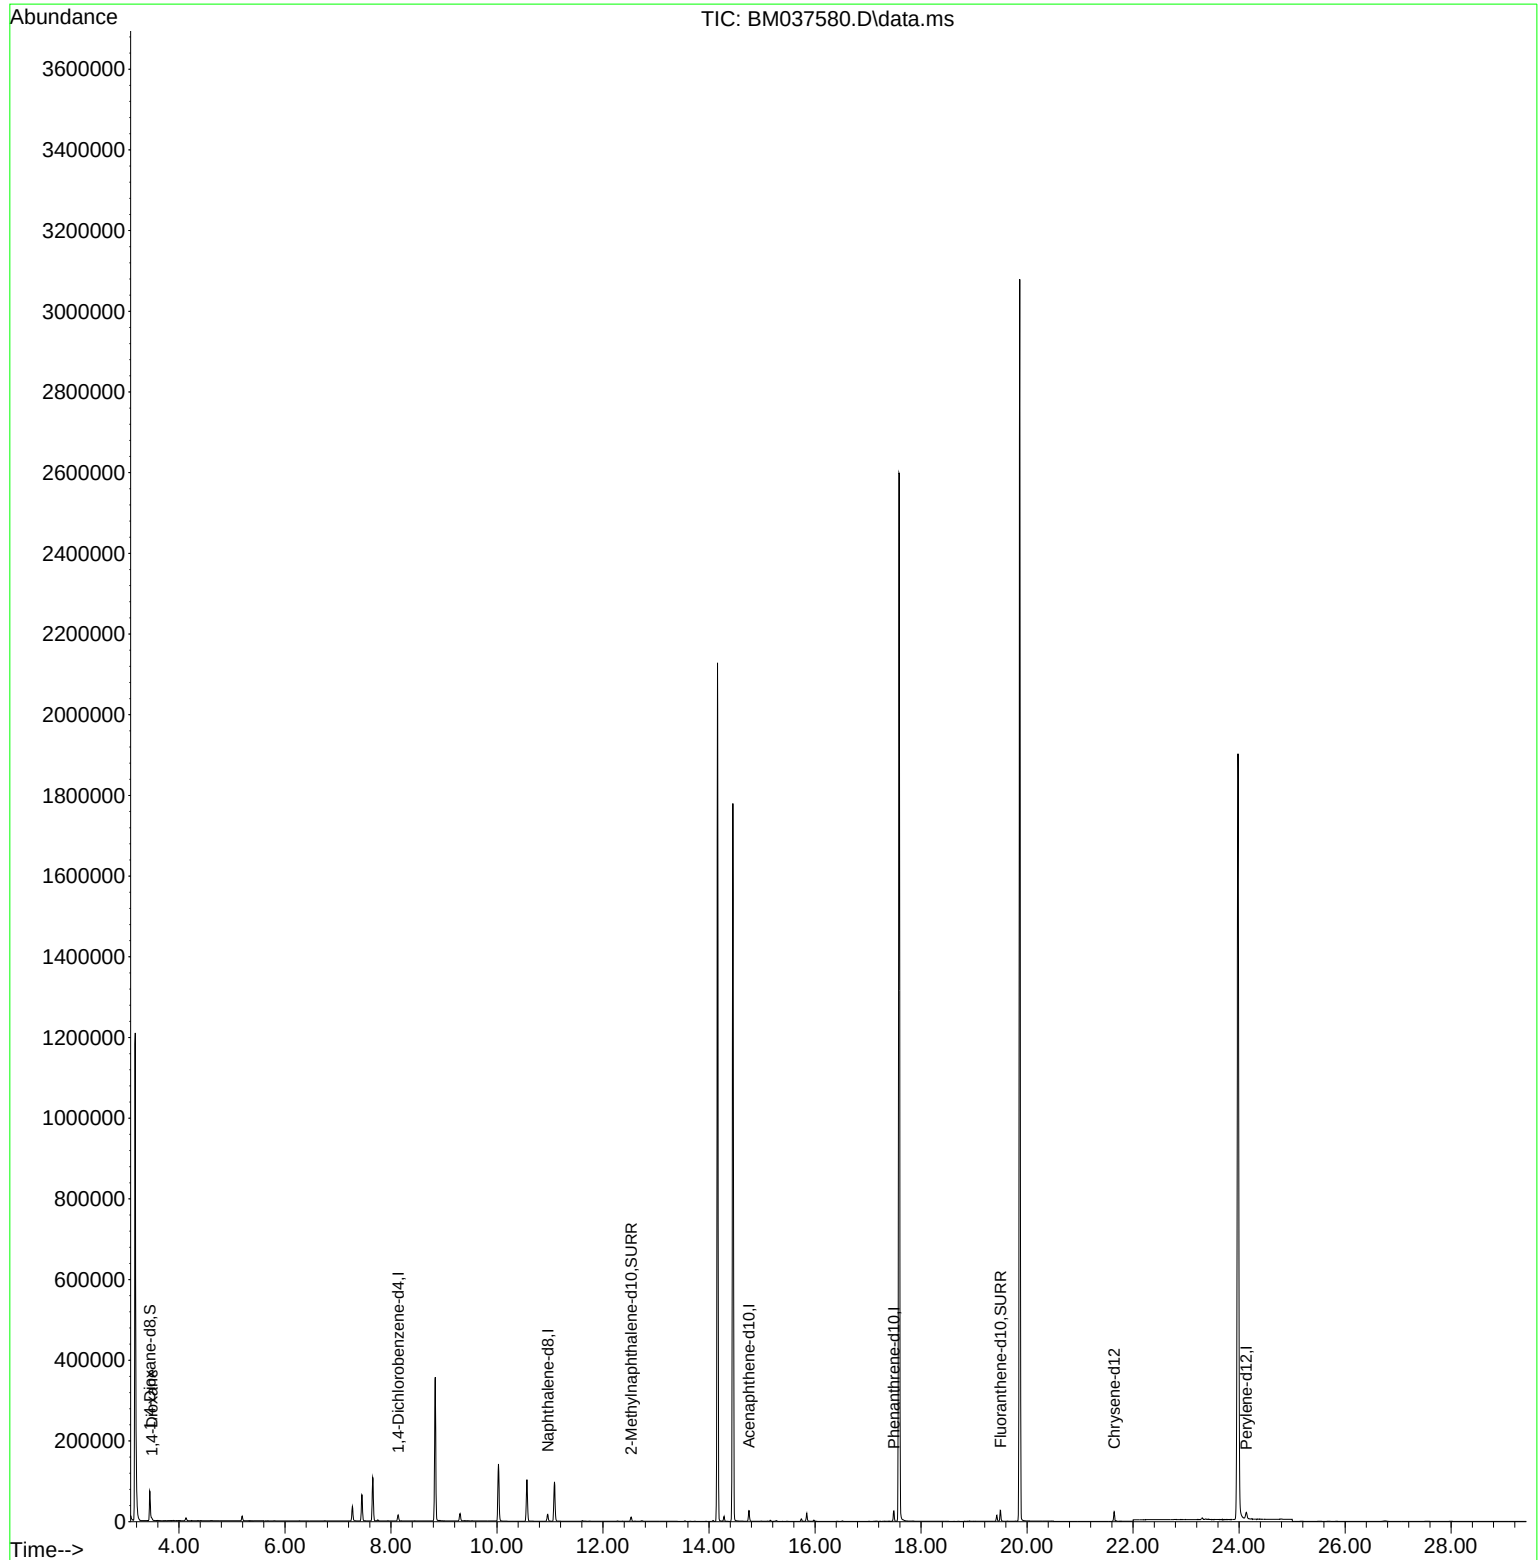

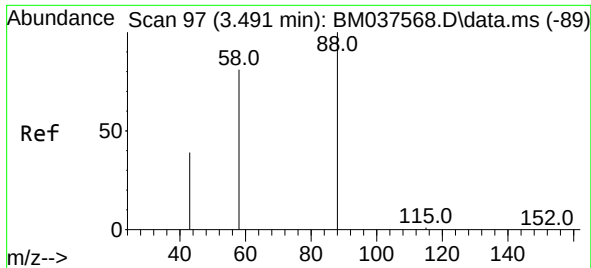

#2
 1,4-Dioxane
 Concen: 0.281 ng/ul
 RT: 3.491 min Scan# 91
 Delta R.T. -0.000 min
 Lab File: BM037580.D
 Acq: 19 Nov 2022 01:15

Instrument :
 BNA_M
 ClientSampleId :
 BGCC8

Tgt Ion: 88 Resp: 2540
 Ion Ratio Lower Upper
 88 100
 43 53.4 102.8 154.2#
 58 67.3 67.3 100.9#

