

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
 Data File : BM037583.D
 Acq On : 19 Nov 2022 03:04
 Operator : CG/JU
 Sample : N5689-08
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGCF6

Quant Time: Nov 19 03:37:34 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 18 06:51:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.136	152	7282	0.400	ng/ul	0.00
4) Naphthalene-d8	10.957	136	21706	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.751	164	13619	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.486	188	28289	0.400	ng/ul	0.00
17) Chrysene-d12	21.643	240	20590	0.400	ng/ul	# 0.00
23) Perylene-d12	24.136	264	23457	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.449	96	41452	4.896	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.530	152	13172	0.366	ng/ul	0.00
18) Fluoranthene-d10	19.498	212	28365	0.417	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.487	88	2189	0.248	ng/ul#	58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
Data File : BM037583.D
Acq On : 19 Nov 2022 03:04
Operator : CG/JU
Sample : N5689-08
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGCF6

Quant Time: Nov 19 03:37:34 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 18 06:51:41 2022
Response via : Initial Calibration

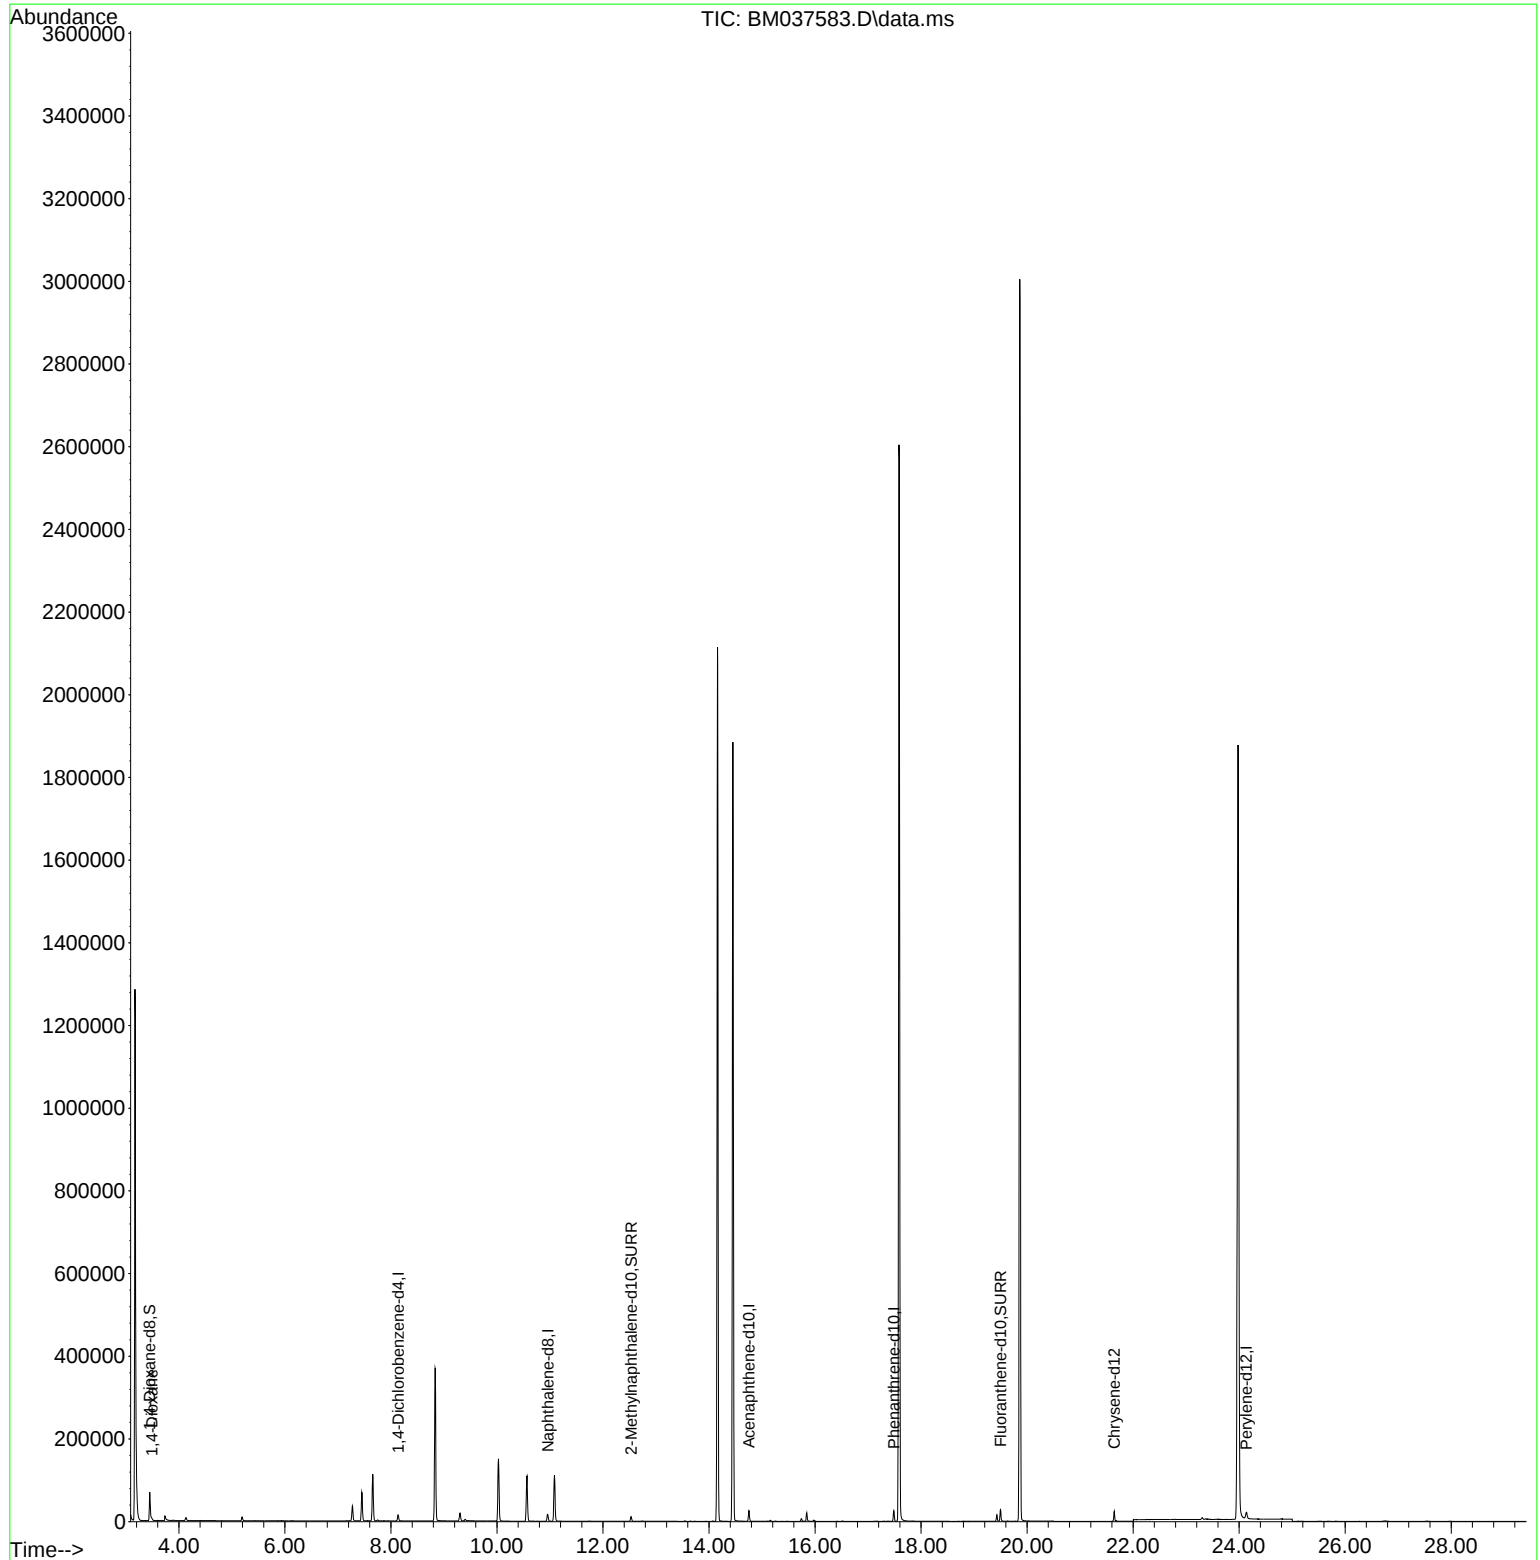

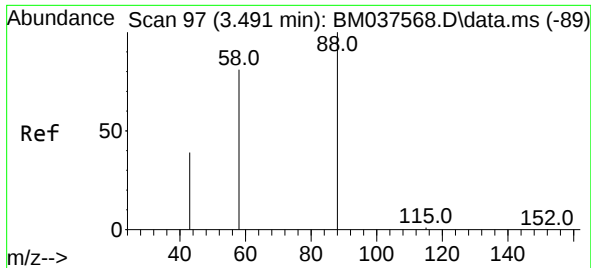

#2
 1,4-Dioxane
 Concen: 0.248 ng/ul
 RT: 3.487 min Scan# 96
 Delta R.T. -0.004 min
 Lab File: BM037583.D
 Acq: 19 Nov 2022 03:04

Instrument :
 BNA_M
 ClientSampleId :
 BGCF6

Tgt Ion: 88 Resp: 2189
 Ion Ratio Lower Upper
 88 100
 43 61.7 102.8 154.2#
 58 68.0 67.3 100.9

