

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
 Data File : BM037584.D
 Acq On : 19 Nov 2022 03:41
 Operator : CG/JU
 Sample : N5689-09
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGCD2

Quant Time: Nov 19 04:36:02 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 18 06:51:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.136	152	7188	0.400	ng/ul	0.00
4) Naphthalene-d8	10.952	136	21129	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.751	164	13311	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.486	188	27571	0.400	ng/ul	0.00
17) Chrysene-d12	21.643	240	19776	0.400	ng/ul	# 0.00
23) Perylene-d12	24.136	264	22431	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.449	96	39547	4.732	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.530	152	12688	0.362	ng/ul	0.00
18) Fluoranthene-d10	19.498	212	27262	0.417	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.491	88	2074	0.238	ng/ul#	54


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
Data File : BM037584.D
Acq On : 19 Nov 2022 03:41
Operator : CG/JU
Sample : N5689-09
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGCD2

Quant Time: Nov 19 04:36:02 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 18 06:51:41 2022
Response via : Initial Calibration

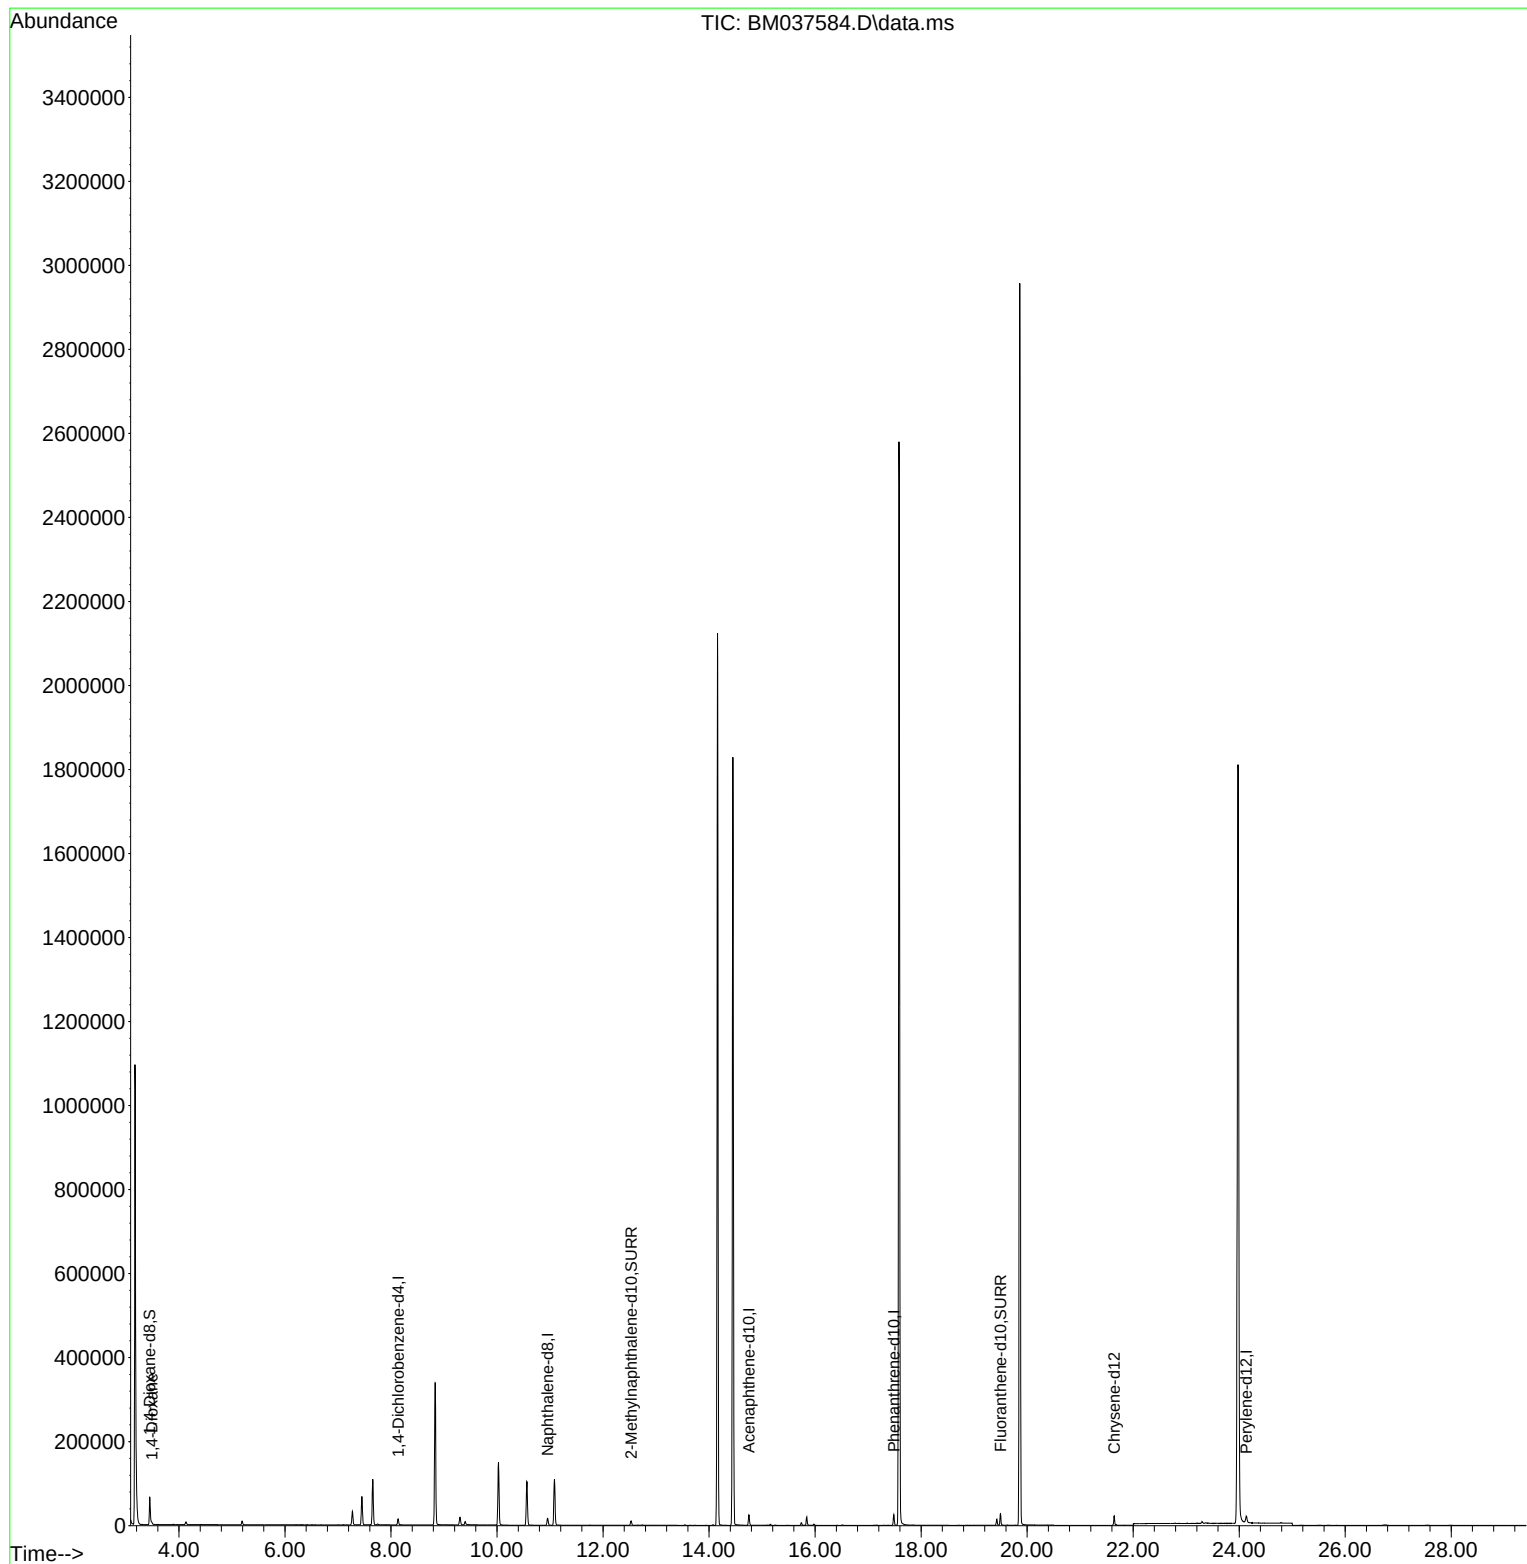

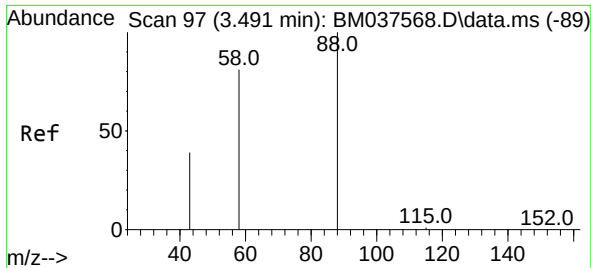

#2
 1,4-Dioxane
 Concen: 0.238 ng/ul
 RT: 3.491 min Scan# 91
 Delta R.T. -0.000 min
 Lab File: BM037584.D
 Acq: 19 Nov 2022 03:41

Instrument :
 BNA_M
 ClientSampleId :
 BGCD2

Tgt Ion: 88 Resp: 2074

Ion	Ratio	Lower	Upper
88	100		
43	56.6	102.8	154.2#
58	65.9	67.3	100.9#

