

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
 Data File : BM037591.D
 Acq On : 19 Nov 2022 08:30
 Operator : CG/JU
 Sample : N5689-13
 Misc :
 ALS Vial : 78 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGCD6

Quant Time: Nov 20 23:47:28 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 18 06:51:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.132	152	8613	0.400	ng/ul	0.00
4) Naphthalene-d8	10.952	136	25481	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.752	164	15829	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.483	188	33067	0.400	ng/ul	0.00
17) Chrysene-d12	21.642	240	24025	0.400	ng/ul	# 0.00
23) Perylene-d12	24.133	264	26397	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.449	96	35060	3.501	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.525	152	13985	0.331	ng/ul	0.00
18) Fluoranthene-d10	19.494	212	31545	0.397	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.487	88	1790	0.172	ng/ul#	57


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
Data File : BM037591.D
Acq On : 19 Nov 2022 08:30
Operator : CG/JU
Sample : N5689-13
Misc :
ALS Vial : 78 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGCD6

Quant Time: Nov 20 23:47:28 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 18 06:51:41 2022
Response via : Initial Calibration

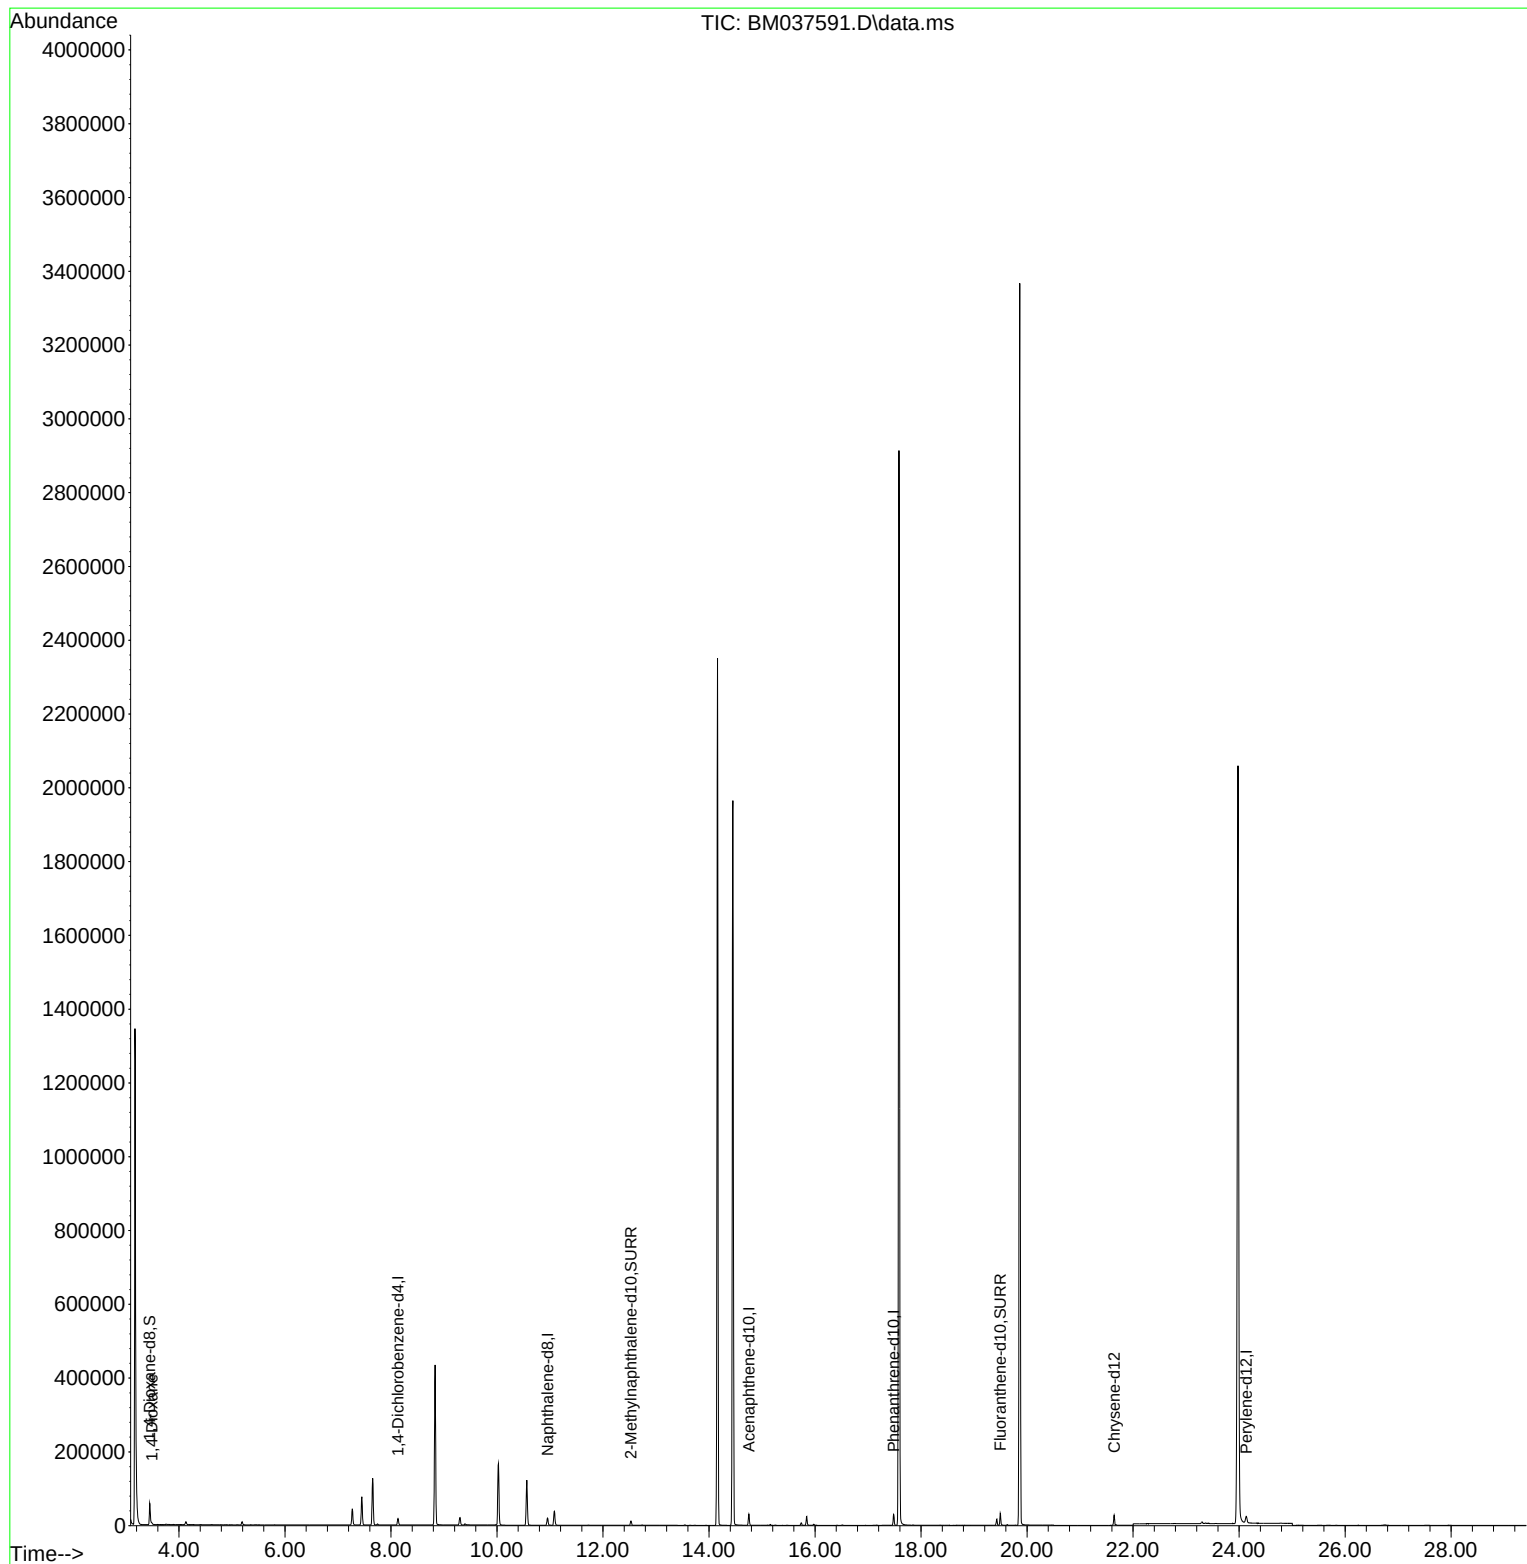

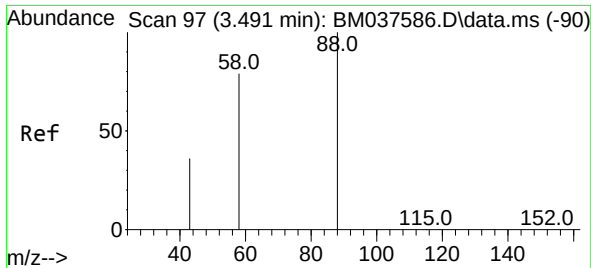

#2
 1,4-Dioxane
 Concen: 0.172 ng/ul
 RT: 3.487 min Scan# 90
 Delta R.T. -0.004 min
 Lab File: BM037591.D
 Acq: 19 Nov 2022 08:30

Instrument :
 BNA_M
 ClientSampleId :
 BGCD6

Tgt Ion: 88 Resp: 1790
 Ion Ratio Lower Upper
 88 100
 43 63.8 102.8 154.2#
 58 63.6 67.3 100.9#

