

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
 Data File : BM037592.D
 Acq On : 19 Nov 2022 09:06
 Operator : CG/JU
 Sample : N5689-14
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGCD7

Quant Time: Nov 20 23:47:34 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 18 06:51:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.132	152	7931	0.400	ng/ul	0.00
4) Naphthalene-d8	10.952	136	23615	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.751	164	14803	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.482	188	31099	0.400	ng/ul	0.00
17) Chrysene-d12	21.643	240	25550	0.400	ng/ul	# 0.00
23) Perylene-d12	24.133	264	28154	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.449	96	45821	4.969	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.530	152	12368	0.316	ng/ul	0.00
18) Fluoranthene-d10	19.494	212	32129	0.381	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.487	88	2860	0.298	ng/ul#	56


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
Data File : BM037592.D
Acq On : 19 Nov 2022 09:06
Operator : CG/JU
Sample : N5689-14
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGCD7

Quant Time: Nov 20 23:47:34 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 18 06:51:41 2022
Response via : Initial Calibration

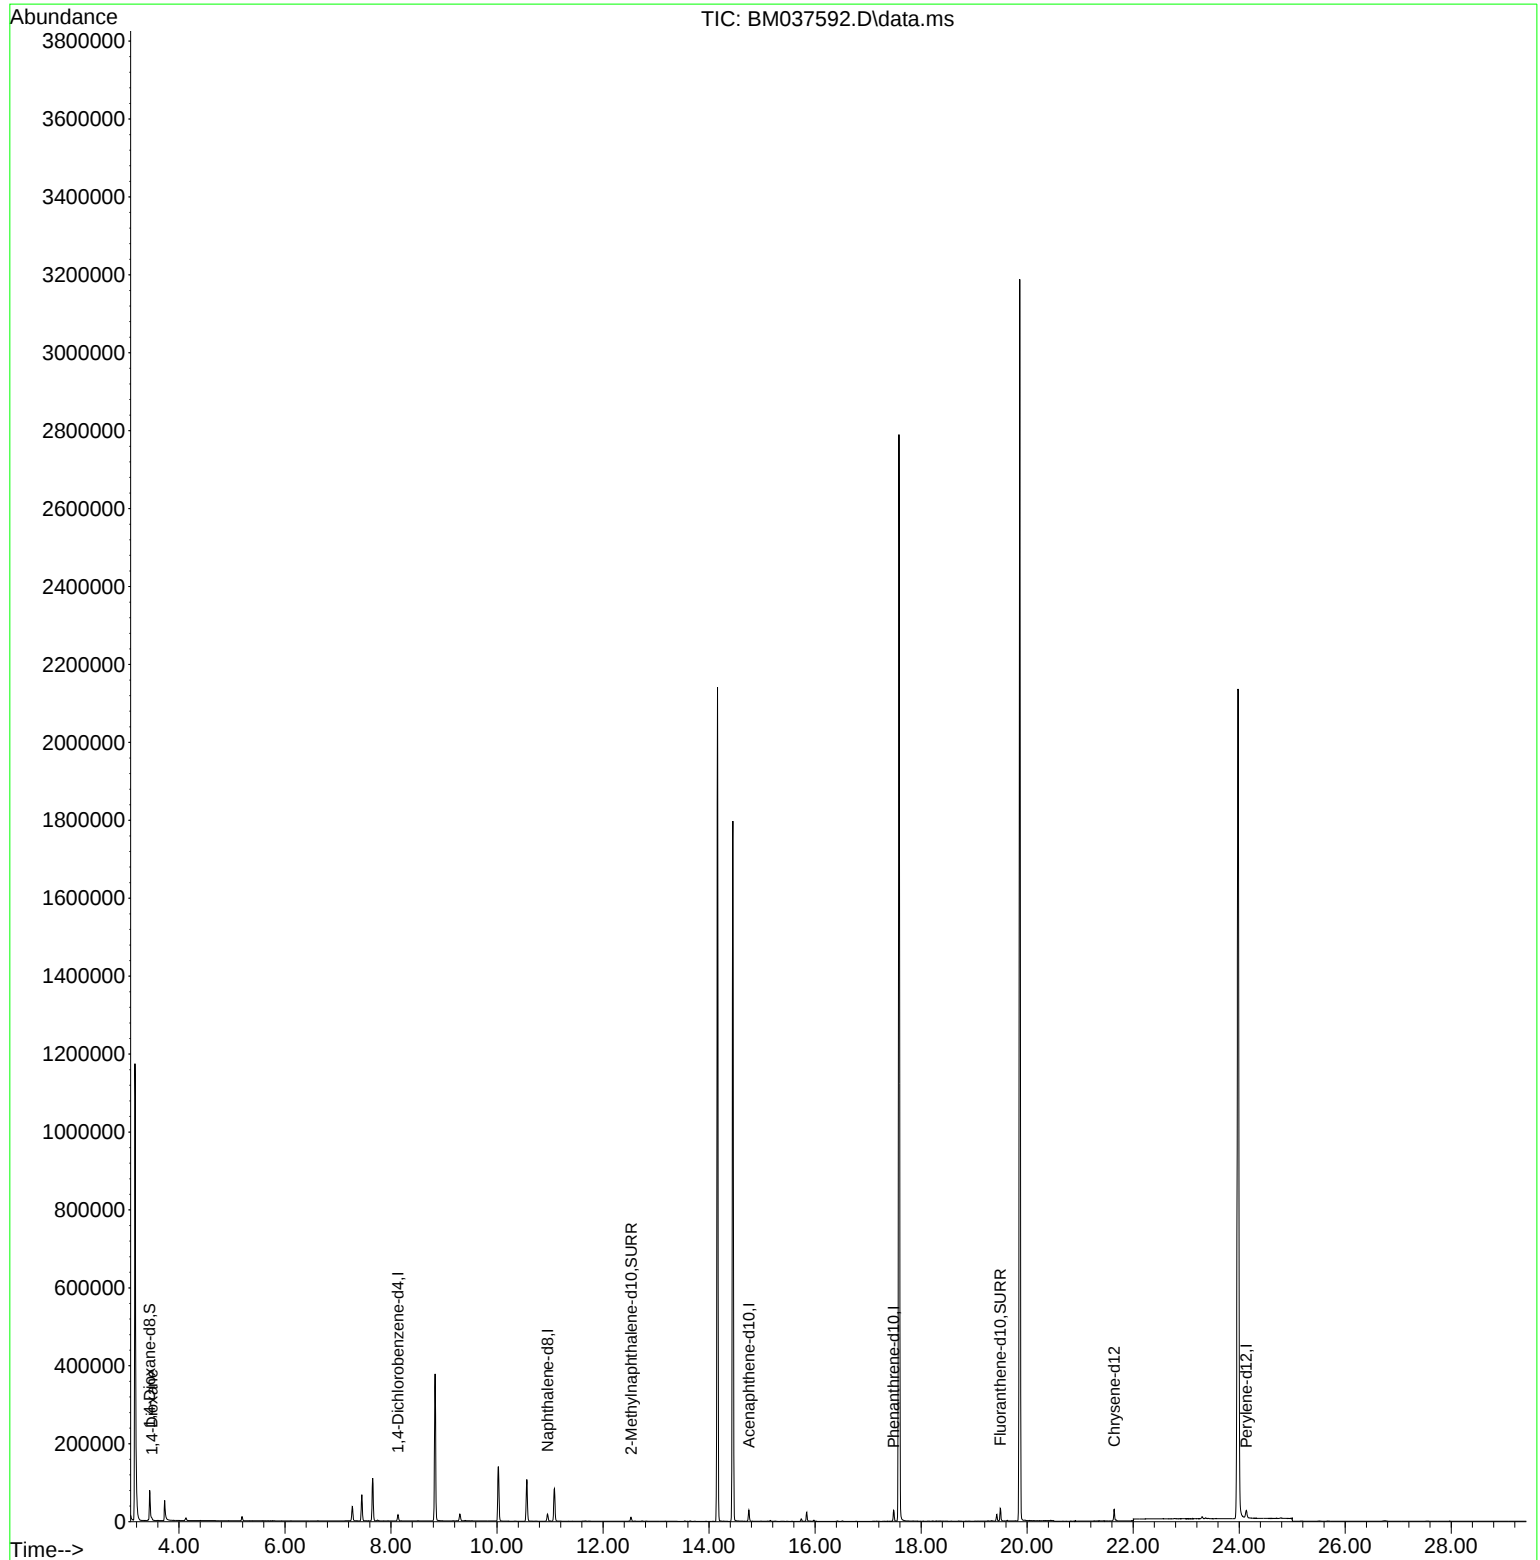

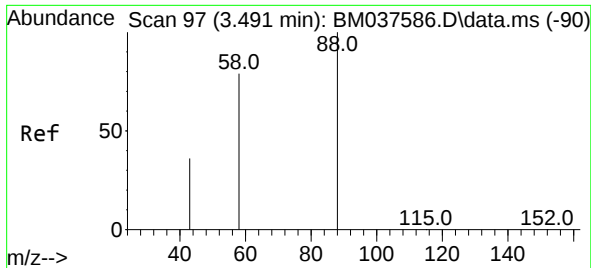

#2
 1,4-Dioxane
 Concen: 0.298 ng/ul
 RT: 3.487 min Scan# 90
 Delta R.T. -0.004 min
 Lab File: BM037592.D
 Acq: 19 Nov 2022 09:06

Instrument :
 BNA_M
 ClientSampleId :
 BGCD7

Tgt Ion:	88	Resp:	2860
Ion	Ratio	Lower	Upper
88	100		
43	57.2	102.8	154.2#
58	69.6	67.3	100.9

