

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
 Data File : BM037595.D
 Acq On : 19 Nov 2022 10:55
 Operator : CG/JU
 Sample : N5689-17
 Misc :
 ALS Vial : 82 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGCF9

Quant Time: Nov 20 23:47:52 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 18 06:51:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.132	152	10163	0.400	ng/ul	0.00
4) Naphthalene-d8	10.952	136	30749	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.751	164	19549	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.482	188	43102	0.400	ng/ul	0.00
17) Chrysene-d12	21.643	240	33227	0.400	ng/ul	0.00
23) Perylene-d12	24.133	264	32794	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.453	96	56731	4.801	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.525	152	16683	0.327	ng/ul	0.00
18) Fluoranthene-d10	19.498	212	46060	0.419	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.491	88	3299	0.268	ng/ul#	47


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
Data File : BM037595.D
Acq On : 19 Nov 2022 10:55
Operator : CG/JU
Sample : N5689-17
Misc :
ALS Vial : 82 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGCF9

Quant Time: Nov 20 23:47:52 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 18 06:51:41 2022
Response via : Initial Calibration

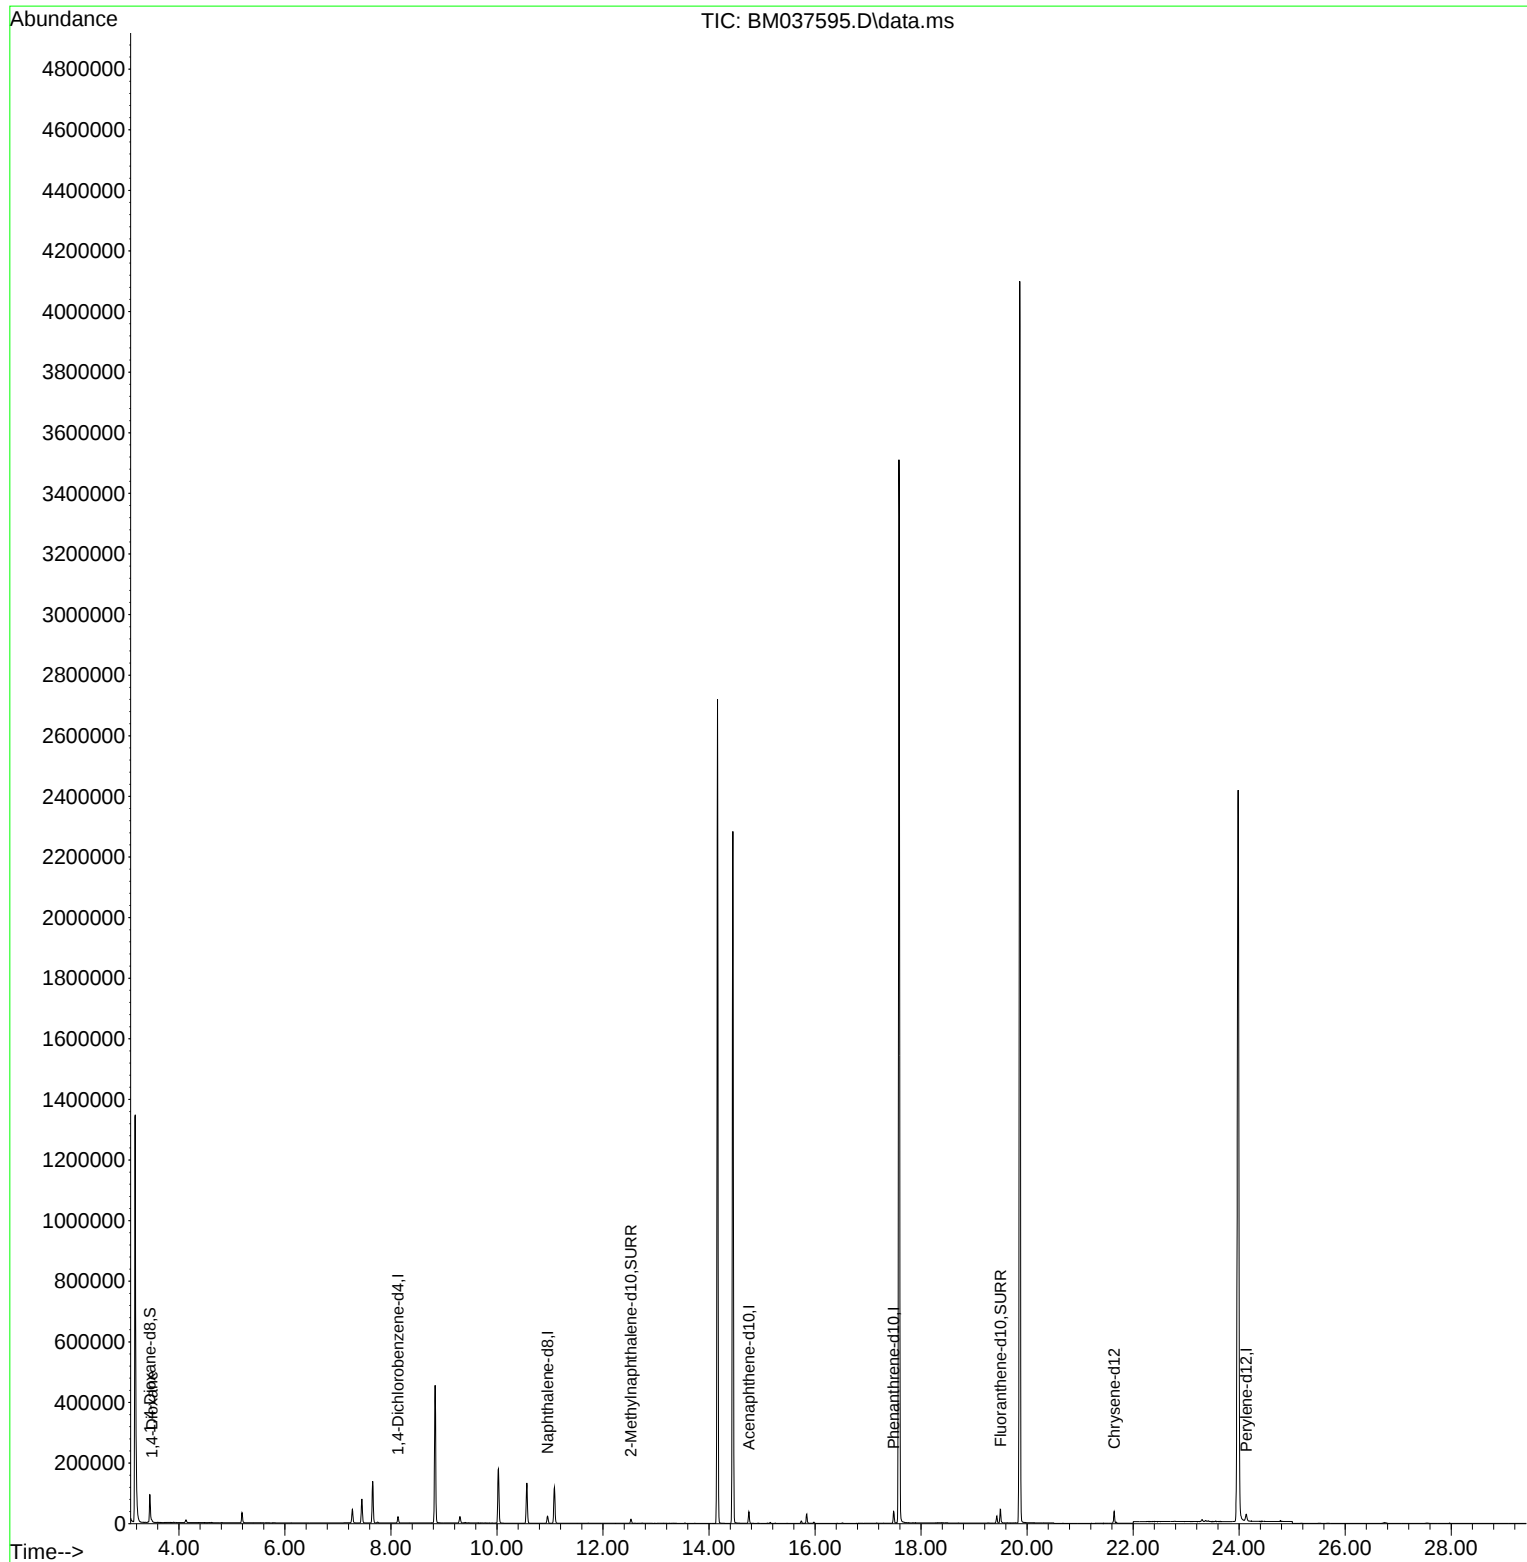

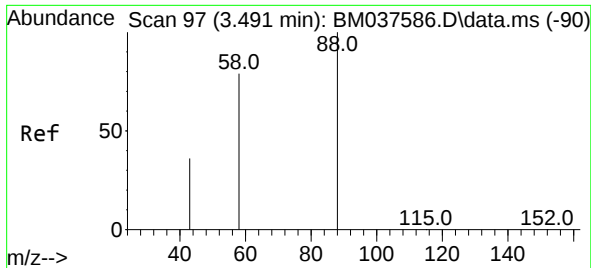

#2
 1,4-Dioxane
 Concen: 0.268 ng/ul
 RT: 3.491 min Scan# 91
 Delta R.T. 0.000 min
 Lab File: BM037595.D
 Acq: 19 Nov 2022 10:55

Instrument :
 BNA_M
 ClientSampleId :
 BGCF9

Tgt Ion: 88 Resp: 3299
 Ion Ratio Lower Upper
 88 100
 43 50.1 102.8 154.2#
 58 55.8 67.3 100.9#

