

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
 Data File : BM037597.D
 Acq On : 19 Nov 2022 12:07
 Operator : CG/JU
 Sample : N5689-19
 Misc :
 ALS Vial : 84 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGCG1

Quant Time: Nov 20 23:48:04 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 18 06:51:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.132	152	6932	0.400	ng/ul	0.00
4) Naphthalene-d8	10.952	136	20211	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.751	164	12111	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.482	188	26237	0.400	ng/ul	0.00
17) Chrysene-d12	21.643	240	19721	0.400	ng/ul	# 0.00
23) Perylene-d12	24.137	264	21247	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.449	96	29977	3.719	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.525	152	8815	0.263	ng/ul	0.00
18) Fluoranthene-d10	19.494	212	21553	0.331	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.487	88	1618	0.193	ng/ul#	57


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111722\
Data File : BM037597.D
Acq On : 19 Nov 2022 12:07
Operator : CG/JU
Sample : N5689-19
Misc :
ALS Vial : 84 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGCG1

Quant Time: Nov 20 23:48:04 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 18 06:51:41 2022
Response via : Initial Calibration

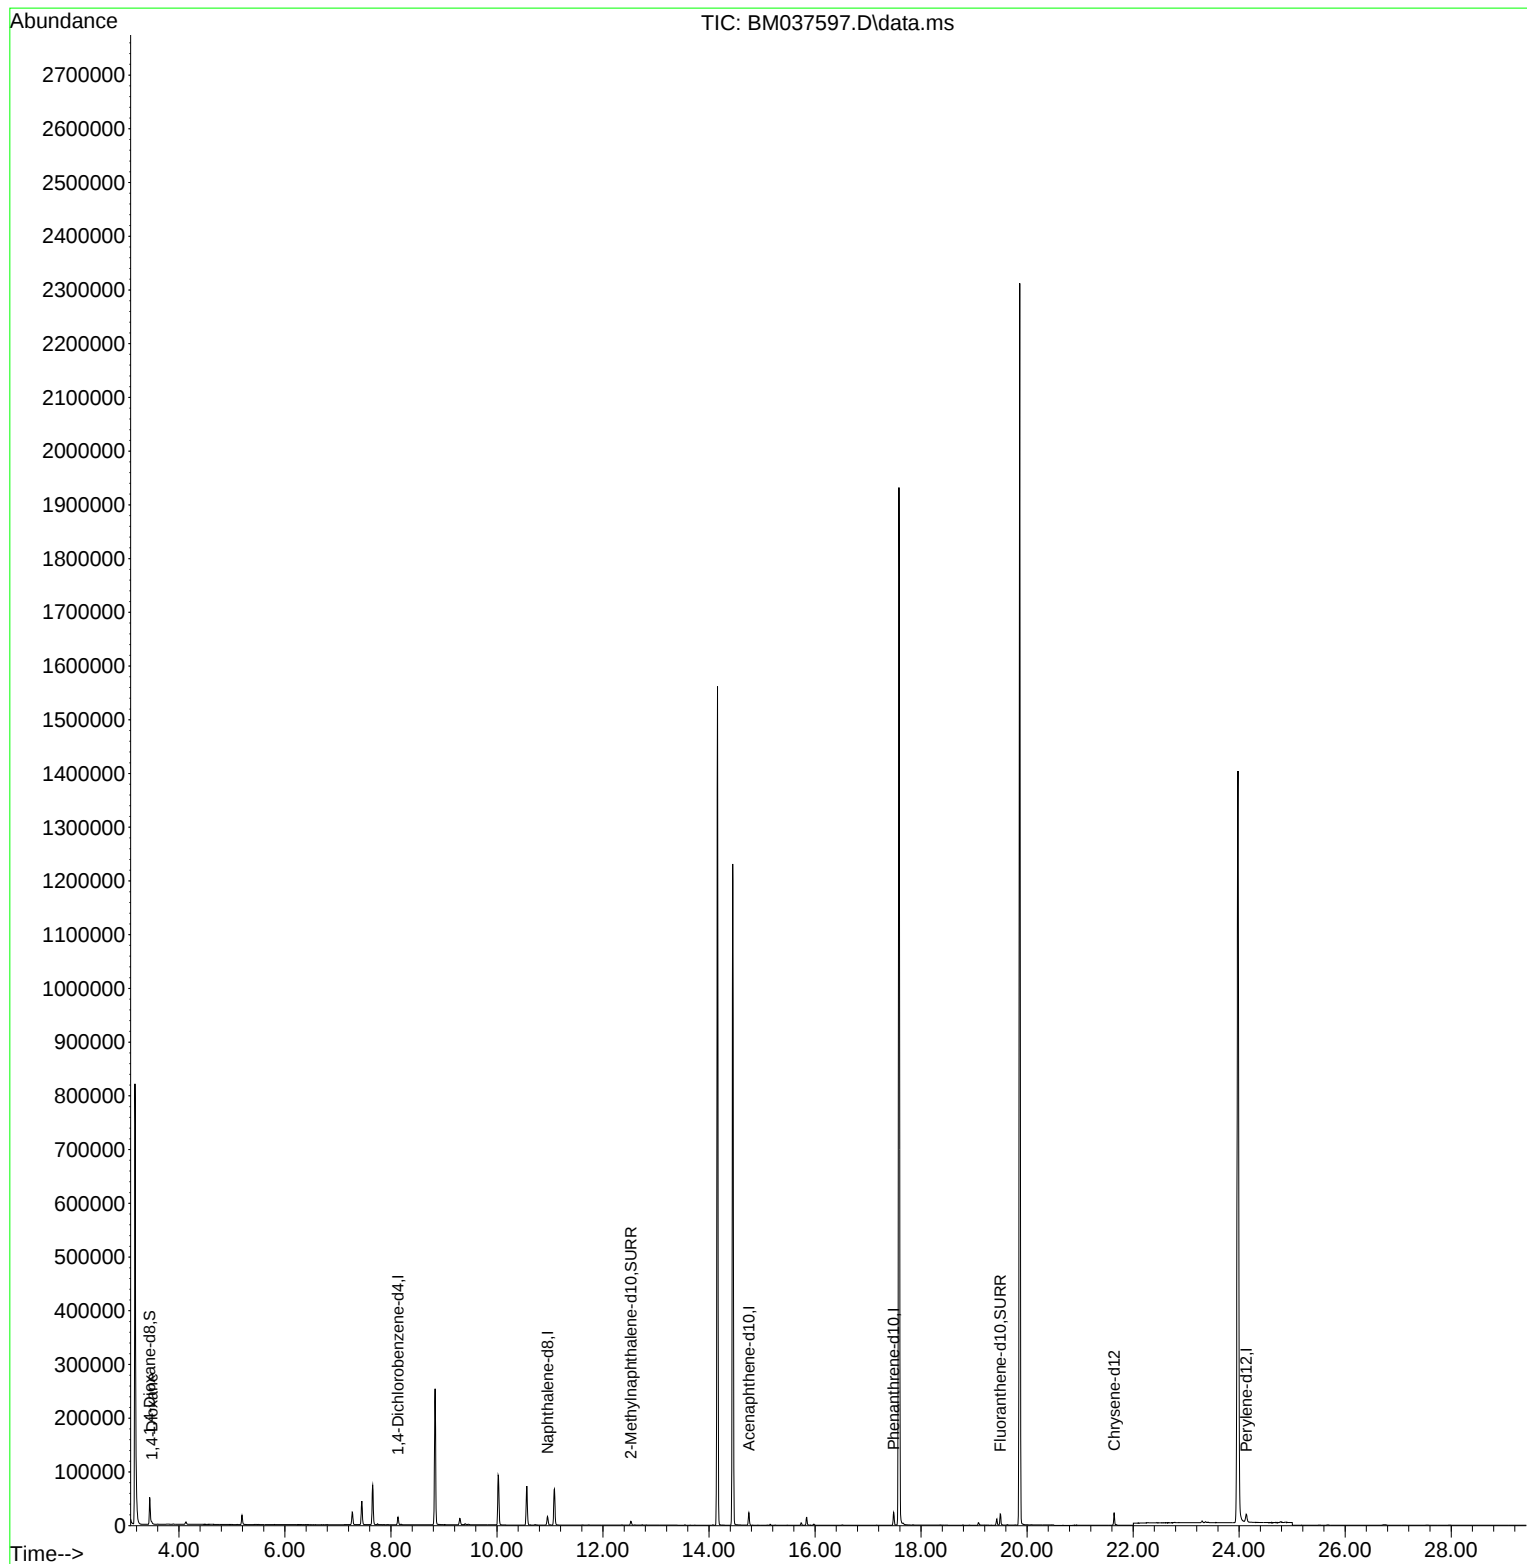

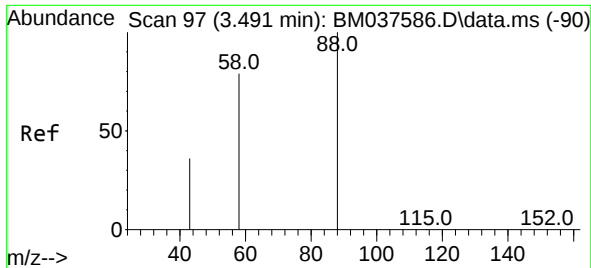

#2
 1,4-Dioxane
 Concen: 0.193 ng/ul
 RT: 3.487 min Scan# 90
 Delta R.T. -0.004 min
 Lab File: BM037597.D
 Acq: 19 Nov 2022 12:07

Instrument :
 BNA_M
 ClientSampleId :
 BGCG1

Tgt Ion: 88 Resp: 1618

Ion	Ratio	Lower	Upper
88	100		
43	63.1	102.8	154.2#
58	64.7	67.3	100.9#

