

Data Path : Z:\HPCHEM1\BNA M\DATA\BM111815\
 Data File : BM003176.D
 Acq On : 19 Nov 2015 00:48
 Operator : UM/IZ
 Sample : G4323-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4HT4

Manual Integrations
 APPROVED

Mmdadoda
 11/19/2015 6:42:51 PM

Quant Time: Nov 19 03:56:40 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-SIM-BM111815.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 19 03:20:59 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	28827	0.40	ng/ul	0.00
4) Naphthalene-d8	10.53	136	115494	0.40	ng/ul	0.00
8) Acenaphthene-d10	14.38	164	69050	0.40	ng/ul	0.00
12) Phenanthrene-d10	17.12	188	155964m	0.40	ng/ul	0.00
18) Chrysene-d12	21.32	240	217520	0.40	ng/ul	0.00
22) Perylene-d12	23.58	264	212445	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	3.20	96	119598	3.88	ng/uL	0.00
6) 2-Methylnaphthalene-d10	12.12	152	34854	0.22	ng/ul	0.00
16) Fluoranthene-d10	19.17	212	67514	0.18	ng/ul	0.00
Target Compounds						
5) Naphthalene	10.58	128	6160	0.02	ng/ul#	91
13) Pentachlorophenol	16.78	266	2807	0.08	ng/ul#	16
14) Phenanthrene	17.17	178	14695m	0.03	ng/ul	
17) Fluoranthene	19.19	202	3329	0.01	ng/ul	61

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM111815\
Data File : BM003176.D
Acq On : 19 Nov 2015 00:48
Operator : UM/IZ
Sample : G4323-03
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
A4HT4

Quant Time: Nov 19 03:56:40 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-SIM-BM111815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 19 03:20:59 2015
Response via : Initial Calibration

Manual Integrations
APPROVED

Mmdadoda
11/19/2015 6:42:51 PM

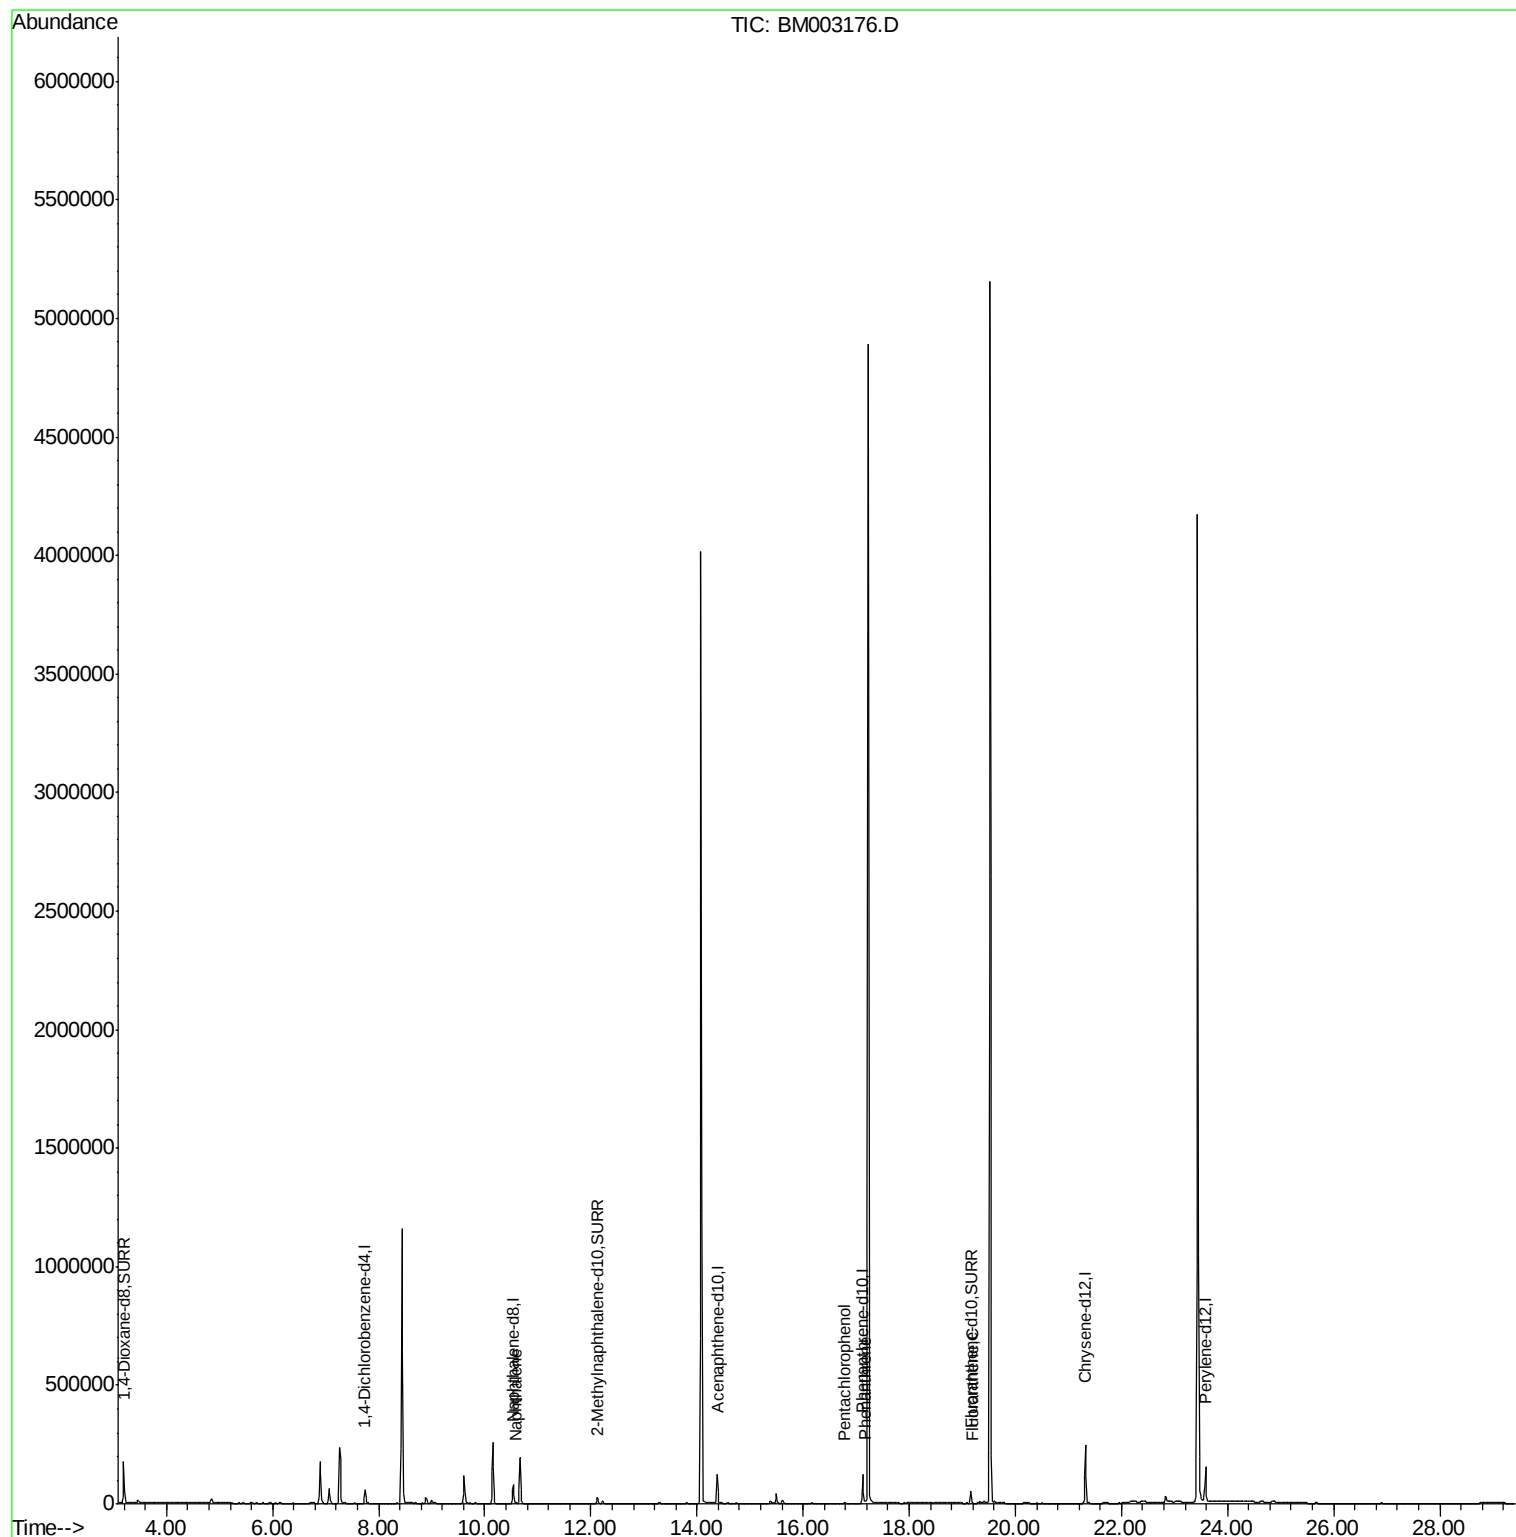

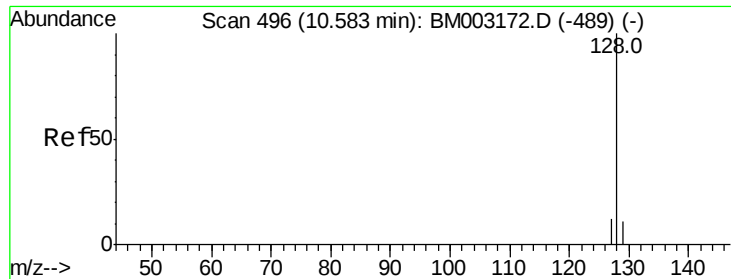

#5

Naphthalene

Concen: 0.02 ng/ul

RT: 10.58 min Scan# 496

Delta R.T. 0.00 min

Lab File: BM003176.D

Acq: 19 Nov 2015 00:48

Instrument :

BNA_M

ClientSampleId :


A4HT4

Tot Ion:128 Resp: 6160

Ion	Ratio	Lower	Upper
128	100		
129	16.1	9.0	13.6#
127	14.3	9.6	14.4

Manual Integrations
APPROVED




Mmdadoda
11/19/2015 6:42:51 PM

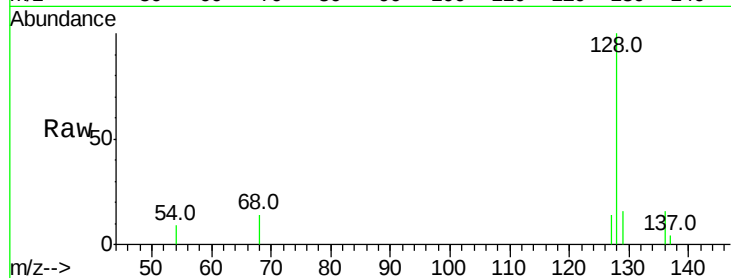

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

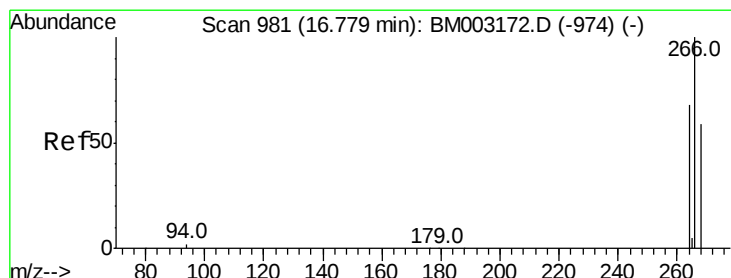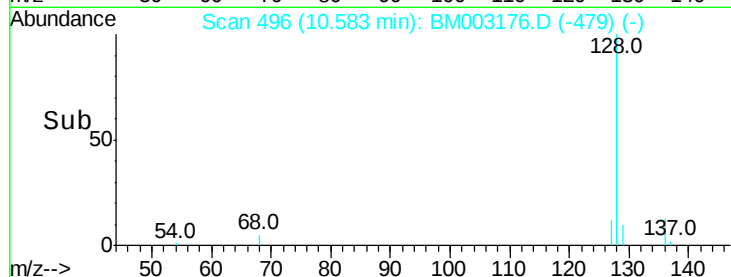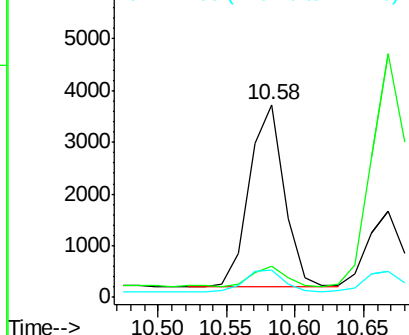

#13

Pentachlorophenol

Concen: 0.08 ng/ul

RT: 16.78 min Scan# 981

Delta R.T. 0.00 min

Lab File: BM003176.D

Acq: 19 Nov 2015 00:48




Tgt Ion:266 Resp: 2807


Ion	Ratio	Lower	Upper
266	100		
264	63.7	0.3	0.5#
268	67.0	0.0	0.0#

Abundance Ion 266.00 (265.70 to 266.70): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

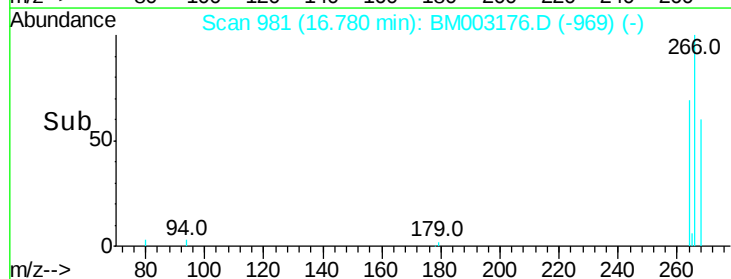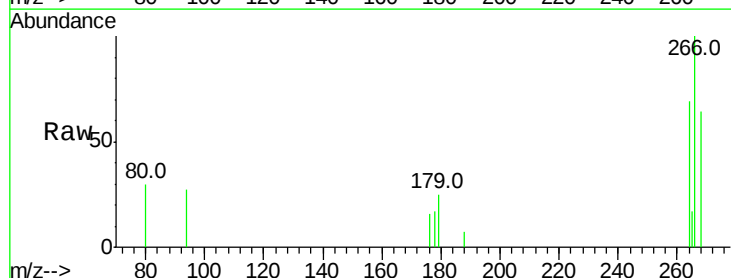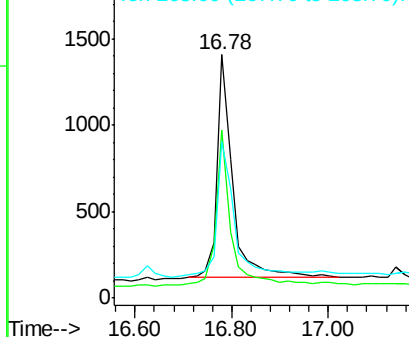

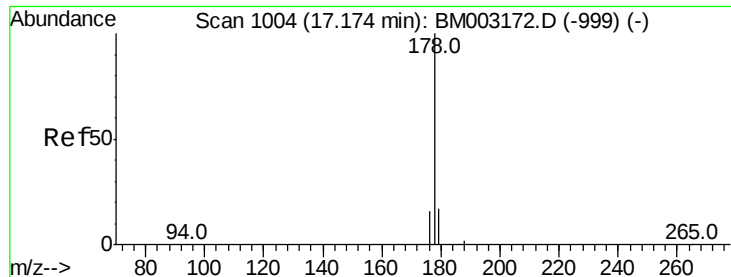

#14

Phenanthrene

Concen: 0.03 ng/ul m

RT: 17.17 min Scan# 1004

Delta R.T. 0.00 min

Lab File: BM003176.D

Acq: 19 Nov 2015 00:48

Instrument :

BNA_M

ClientSampleId :





A4HT4

Tot Ion:178 Resp: 14695

Ion	Ratio	Lower	Upper
178	100		
176	18.5	13.0	19.4
179	21.4	14.2	21.2#

Manual Integrations
APPROVED

Mmdadoda
11/19/2015 6:42:51 PM

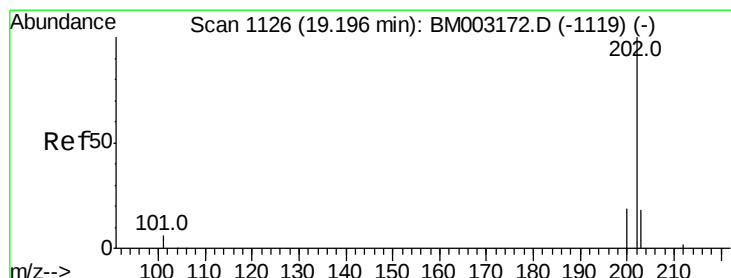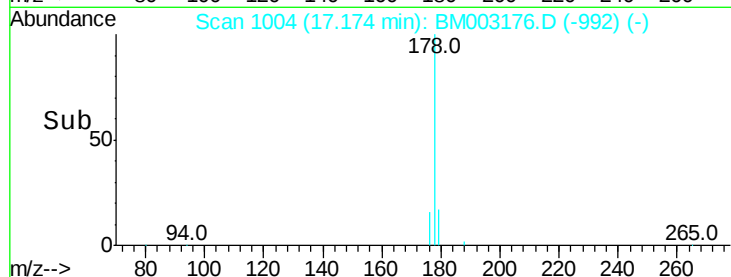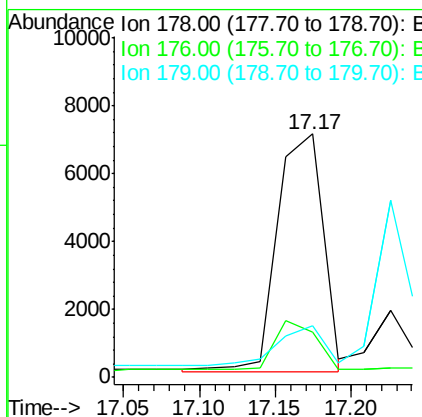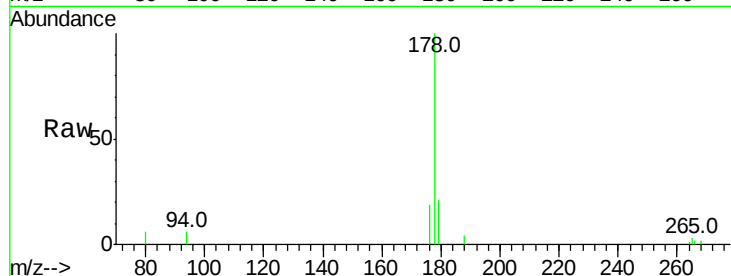

#17

Fluoranthene

Concen: 0.01 ng/ul

RT: 19.19 min Scan# 1126

Delta R.T. -0.00 min

Lab File: BM003176.D

Acq: 19 Nov 2015 00:48

Tgt Ion:202 Resp: 3329

Ion	Ratio	Lower	Upper
202	100		
101	24.4	0.0	29.6
203	32.9	0.0	36.3

