


Data Path : Z:\HPCHEM1\BNA M\Data\BM111815\
 Data File : BM003165.D
 Acq On : 18 Nov 2015 18:10
 Operator : UM/IZ
 Sample : DFTPP45
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP45

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_F\METHODS\SOM01.2-BF062612.M
 Title : SVOA CALIBRATION
 Last Update : Fri Jun 29 16:06:57 2012

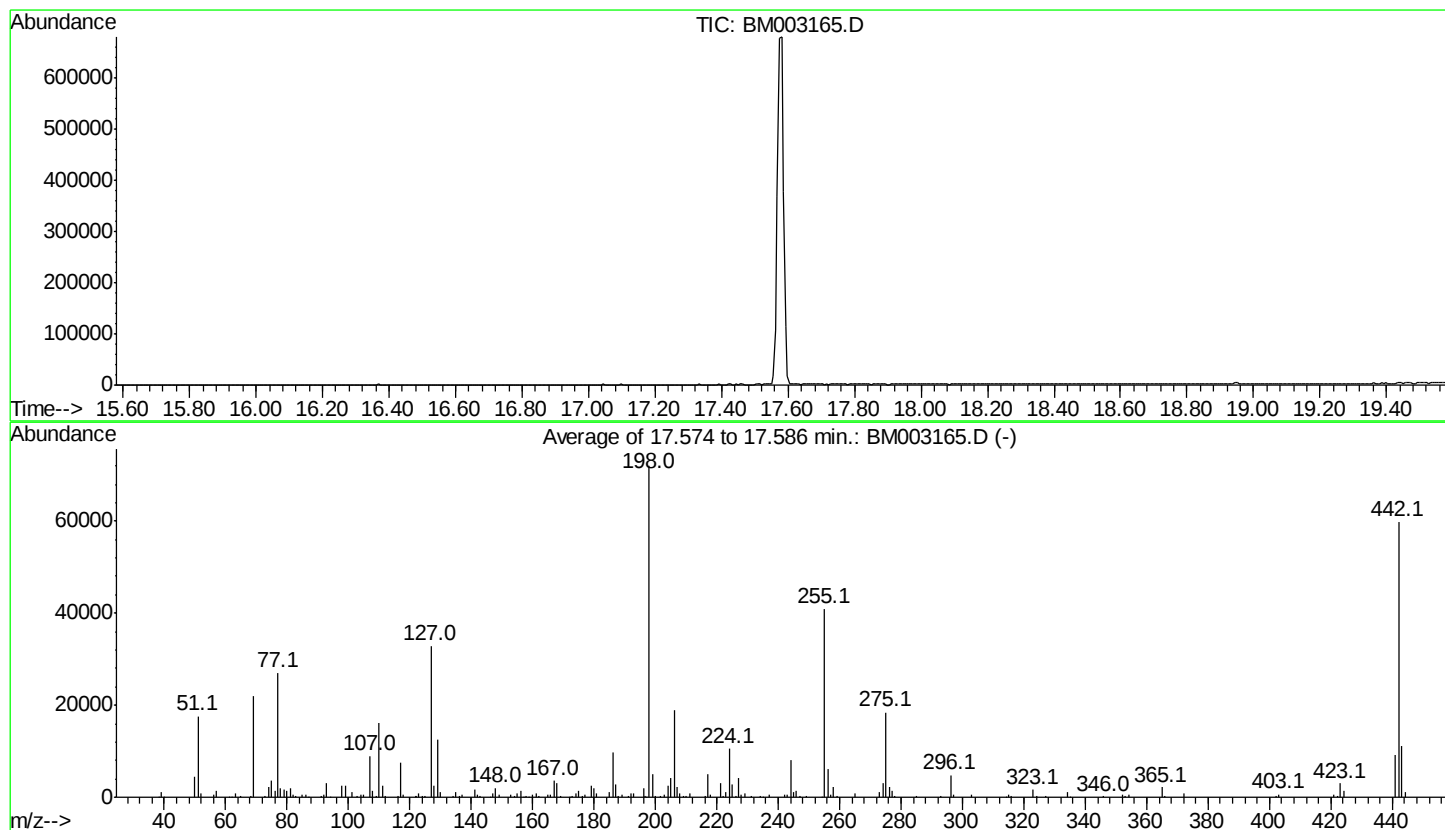

AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2457

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.5	17622	PASS
68	69	0.00	2	1.5	337	PASS
69	198	0.00	100	30.4	21917	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.7	32962	PASS
197	198	0.00	1	0.3	233	PASS
198	198	100	100	100.0	72064	PASS
199	198	5	9	6.8	4919	PASS
275	198	10	60	25.6	18484	PASS
365	198	1	100	3.0	2175	PASS
441	443	0.01	100	82.6	9231	PASS
442	198	50	100	83.1	59896	PASS
443	442	15	24	18.7	11175	PASS

Scan 2457 (17.539 min): BM003165.D
DFTPP45

m/z	Abundance
44.00	520.0
207.00	916.0

Instrument :
BNA_M
ClientSampleId :
DFTPP45

m/z	Abundance
38.00	342.0
39.10	1630.0
40.00	313.0
44.00	555.0
50.00	6138.0
51.10	23400.0
52.00	1096.0
56.00	713.0
57.00	1740.0
61.00	411.0
62.00	421.0
63.00	1076.0
65.00	529.0
68.00	588.0
69.00	28624.0
73.00	376.0
74.00	2952.0
75.00	4535.0
76.00	1617.0
77.10	35720.0
78.00	2847.0
79.00	2375.0
80.00	1646.0
81.00	2534.0
82.00	616.0
83.00	604.0
84.90	703.0
86.00	779.0
87.10	364.0
91.00	469.0
92.00	696.0
93.00	4017.0
94.00	313.0
98.00	3272.0
99.00	3379.0
101.00	1289.0
103.00	542.0
104.00	869.0
105.00	895.0
107.00	11459.0
108.00	1813.0
109.00	358.0
110.00	20352.0
111.00	3283.0
112.00	418.0
116.00	599.0
117.00	9322.0
118.00	780.0
121.90	857.0
123.00	1052.0
123.90	571.0
124.90	466.0
127.00	41024.0
128.00	3176.0
129.00	15799.0
130.00	1368.0
134.00	485.0
135.00	1319.0
136.00	573.0
137.00	949.0
141.00	1916.0
142.10	517.0
142.90	482.0
147.00	1121.0
148.00	2567.0
148.90	674.0
153.00	608.0
154.00	416.0
155.00	1169.0
156.00	1749.0
158.00	303.0
158.80	310.0
160.00	614.0
161.00	1047.0
161.90	324.0
165.00	747.0
165.90	628.0
167.00	4378.0
168.00	3703.0
169.00	492.0
171.90	353.0
173.00	412.0
174.00	739.0
175.00	1711.0
176.10	490.0
177.00	847.0
179.00	2937.0
180.00	2597.0
181.00	1059.0
185.00	1624.0
186.00	11457.0
187.10	3157.0

Instrument :
BNA_M
ClientSampleId :
DFTPP45

188.00	407.0
189.00	659.0
191.10	479.0
192.00	1051.0
193.10	1239.0
196.10	2207.0
196.80	335.0
197.10	349.0
198.00	84416.0
199.00	5970.0
200.00	357.0
201.60	446.0
203.00	580.0
204.10	2898.0
205.00	5281.0
206.10	22576.0
207.10	3497.0
208.00	870.0
209.00	300.0
210.10	341.0
211.00	904.0
216.00	384.0
217.00	5664.0
218.00	733.0
221.10	3225.0
223.10	1304.0
224.10	12076.0
225.00	3064.0
226.00	407.0
227.00	4742.0
228.00	717.0
229.00	1074.0
231.00	469.0
234.00	307.0
237.00	694.0
242.10	580.0
243.00	600.0
244.10	9413.0
245.10	1279.0
246.00	1736.0
246.90	367.0
249.00	367.0
255.10	45688.0
256.10	7164.0
257.00	706.0
258.00	2406.0
259.00	375.0
265.10	937.0
273.10	1306.0
274.10	3341.0
275.10	20168.0
276.10	2790.0
277.10	1748.0
278.00	492.0
285.00	303.0
293.00	361.0
296.10	4994.0
297.00	742.0
303.10	583.0
315.00	532.0
316.00	352.0
323.10	1658.0
324.20	370.0
327.00	314.0
334.00	1125.0
346.00	359.0
352.10	520.0
353.00	324.0
354.10	536.0
365.00	2169.0
366.00	350.0
372.10	781.0
402.10	320.0
403.00	575.0
421.10	412.0
422.00	392.0
423.10	2915.0
424.10	1379.0
441.10	8539.0
442.10	55584.0
443.10	10577.0
444.10	972.0

Instrument :
BNA_M
ClientSampleId :
DFTPP45

m/z	Abundance
39.00	1407.0
43.90	442.0
50.10	4925.0
51.10	19592.0
52.00	944.0
56.00	613.0
57.00	1571.0
63.00	965.0
65.00	506.0
68.10	423.0
69.00	24952.0
73.00	342.0
74.10	2484.0
75.00	4323.0
76.10	1524.0
77.10	30304.0
78.00	2229.0
79.00	1963.0
80.00	1576.0
81.00	2187.0
82.00	523.0
83.00	440.0
85.00	655.0
86.00	501.0
90.90	518.0
91.90	752.0
93.00	3563.0
98.00	2803.0
99.00	2922.0
101.00	1248.0
103.00	431.0
104.00	748.0
105.10	691.0
107.00	10230.0
108.00	1594.0
109.10	363.0
110.00	18816.0
111.00	2779.0
112.00	370.0
115.90	559.0
117.00	8509.0
118.00	649.0
122.10	614.0
123.00	1061.0
123.90	488.0
125.00	546.0
127.00	38144.0
128.00	2717.0
129.00	14498.0
130.00	1137.0
134.00	383.0
135.00	1288.0
136.00	510.0
137.00	676.0
141.00	1833.0
141.90	663.0
143.00	498.0
146.00	354.0
147.00	966.0
148.00	2114.0
149.00	537.0
153.00	614.0
154.00	474.0
155.00	1066.0
156.00	1661.0
157.00	326.0
157.90	368.0
159.90	621.0
161.00	979.0
161.90	334.0
165.00	806.0
166.00	551.0
167.00	4005.0
168.00	3509.0
168.90	490.0
173.00	457.0
174.00	896.0
175.00	1685.0
176.00	583.0
177.00	858.0
179.00	2816.0
180.00	2268.0
180.90	995.0
185.00	1348.0
186.00	11337.0
187.00	3190.0
187.90	405.0
189.00	775.0
190.90	422.0
192.00	1034.0
193.00	953.0
196.00	2454.0

Instrument :
BNA_M
ClientSampleId :
DFTPP45

196.80	364.0
198.00	84888.0
199.00	5754.0
199.90	436.0
201.40	385.0
202.90	427.0
204.10	2851.0
205.00	4796.0
206.10	21792.0
207.00	3581.0
208.00	989.0
208.90	365.0
210.00	319.0
211.00	892.0
216.10	504.0
217.00	5860.0
218.00	824.0
221.10	3711.0
221.90	819.0
223.00	1291.0
224.10	12244.0
225.10	3251.0
226.10	483.0
227.00	5110.0
227.90	644.0
228.90	1087.0
231.10	393.0
234.00	300.0
235.00	424.0
237.00	686.0
242.00	666.0
243.00	691.0
244.10	9304.0
245.10	1420.0
246.00	1842.0
247.00	334.0
249.00	355.0
254.10	353.0
255.10	48576.0
256.10	7024.0
257.00	666.0
258.00	2931.0
259.00	442.0
265.00	1153.0
273.00	1492.0
274.00	3800.0
275.10	22032.0
276.10	2595.0
277.00	1652.0
278.00	366.0
285.10	385.0
293.00	477.0
296.00	5835.0
297.10	931.0
303.00	613.0
314.10	391.0
315.00	730.0
316.00	345.0
323.10	1813.0
324.00	334.0
327.00	415.0
334.10	1185.0
335.00	317.0
346.00	358.0
352.10	601.0
353.00	512.0
354.10	454.0
365.10	2540.0
366.00	374.0
372.10	1047.0
402.00	417.0
403.10	735.0
421.00	626.0
422.10	612.0
423.10	3720.0
424.10	1558.0
441.10	11040.0
442.10	72736.0
443.10	13595.0
444.10	1411.0

Instrument :
BNA_M
ClientSampleId :
DFTPP45

m/z	Abundance
39.00	742.0
44.00	537.0
50.00	2561.0
51.10	9874.0
52.00	565.0
55.90	306.0
57.00	632.0
63.00	496.0
69.00	12177.0
74.00	1306.0
75.00	2225.0
76.00	832.0
77.10	15248.0
78.10	1127.0
79.00	982.0
79.90	806.0
81.00	1039.0
81.90	309.0
85.00	350.0
86.00	392.0
93.00	1748.0
98.00	1383.0
99.00	1457.0
101.00	640.0
104.00	376.0
104.90	387.0
107.00	5067.0
108.10	750.0
110.00	9559.0
111.00	1326.0
117.00	4542.0
118.00	373.0
122.90	603.0
127.00	19720.0
128.00	1365.0
129.00	7551.0
130.00	642.0
134.90	594.0
137.00	493.0
141.00	1041.0
141.90	321.0
146.90	605.0
148.00	1326.0
149.00	337.0
152.90	318.0
155.00	609.0
156.00	893.0
160.00	392.0
161.00	458.0
165.00	385.0
166.00	315.0
167.00	2167.0
168.00	1940.0
174.00	543.0
175.10	892.0
177.00	375.0
179.00	1658.0
180.00	1238.0
181.00	543.0
185.00	769.0
186.00	6382.0
187.00	1806.0
189.00	391.0
192.00	601.0
193.00	632.0
196.00	1340.0
198.00	46888.0
199.00	3034.0
203.00	301.0
204.00	1556.0
205.00	2788.0
206.10	12031.0
207.00	2392.0
208.00	627.0
209.00	326.0
210.90	516.0
217.00	3406.0
218.00	484.0
221.10	1935.0
221.90	455.0
223.00	748.0
224.10	7023.0
225.00	1769.0
227.00	3009.0
227.90	411.0
229.00	590.0
231.00	305.0
237.00	328.0
242.00	369.0
243.00	331.0
244.10	5804.0
245.10	661.0

Instrument :
BNA_M
ClientSampleId :
DFTPP45

246.00	954.0
255.10	28728.0
256.00	3885.0
256.90	414.0
258.00	1579.0
265.00	609.0
273.00	910.0
274.10	2409.0
275.10	13253.0
276.00	1627.0
277.00	1135.0
296.00	3607.0
297.00	406.0
303.10	507.0
315.00	453.0
323.10	1195.0
334.00	707.0
352.00	379.0
354.10	403.0
365.10	1818.0
372.10	632.0
403.10	477.0
421.10	339.0
423.10	2485.0
424.10	929.0
441.10	8114.0
442.10	51368.0
443.10	9354.0
444.10	952.0

Instrument :
BNA_M
ClientSampleId :
DFTPP45