

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111824\
 Data File : BM048791.D
 Acq On : 19 Nov 2024 00:29
 Operator : RC/JU
 Sample : P4829-16
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E29S6

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/19/2024
 Supervised By :mohammad ahmed 11/20/2024

Quant Time: Nov 19 00:59:12 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 18 23:00:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.629	152	2938m	0.400	ng/ul	-0.12
4) Naphthalene-d8	10.404	136	8720	0.400	ng/ul	-0.08
9) Acenaphthene-d10	14.277	164	4506	0.400	ng/ul	-0.02
13) Phenanthrene-d10	17.024	188	9427m	0.400	ng/ul	-0.05
17) Chrysene-d12	21.240	240	8088	0.400	ng/ul	0.00
23) Perylene-d12	23.426	264	5997m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.085	96	16163	4.560	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.032	152	3005	0.267	ng/ul	-0.06
18) Fluoranthene-d10	19.059	212	8444	0.372	ng/ul	-0.03
Target Compounds						Qvalue
5) Naphthalene	10.454	128	764	0.035	ng/ul#	65

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM111824\
Data File : BM048791.D
Acq On : 19 Nov 2024 00:29
Operator : RC/JU
Sample : P4829-16
Misc :
ALS Vial : 25 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
E29S6

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/19/2024
Supervised By :mohammad ahmed 11/20/2024


Quant Time: Nov 19 00:59:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 18 23:00:29 2024
Response via : Initial Calibration

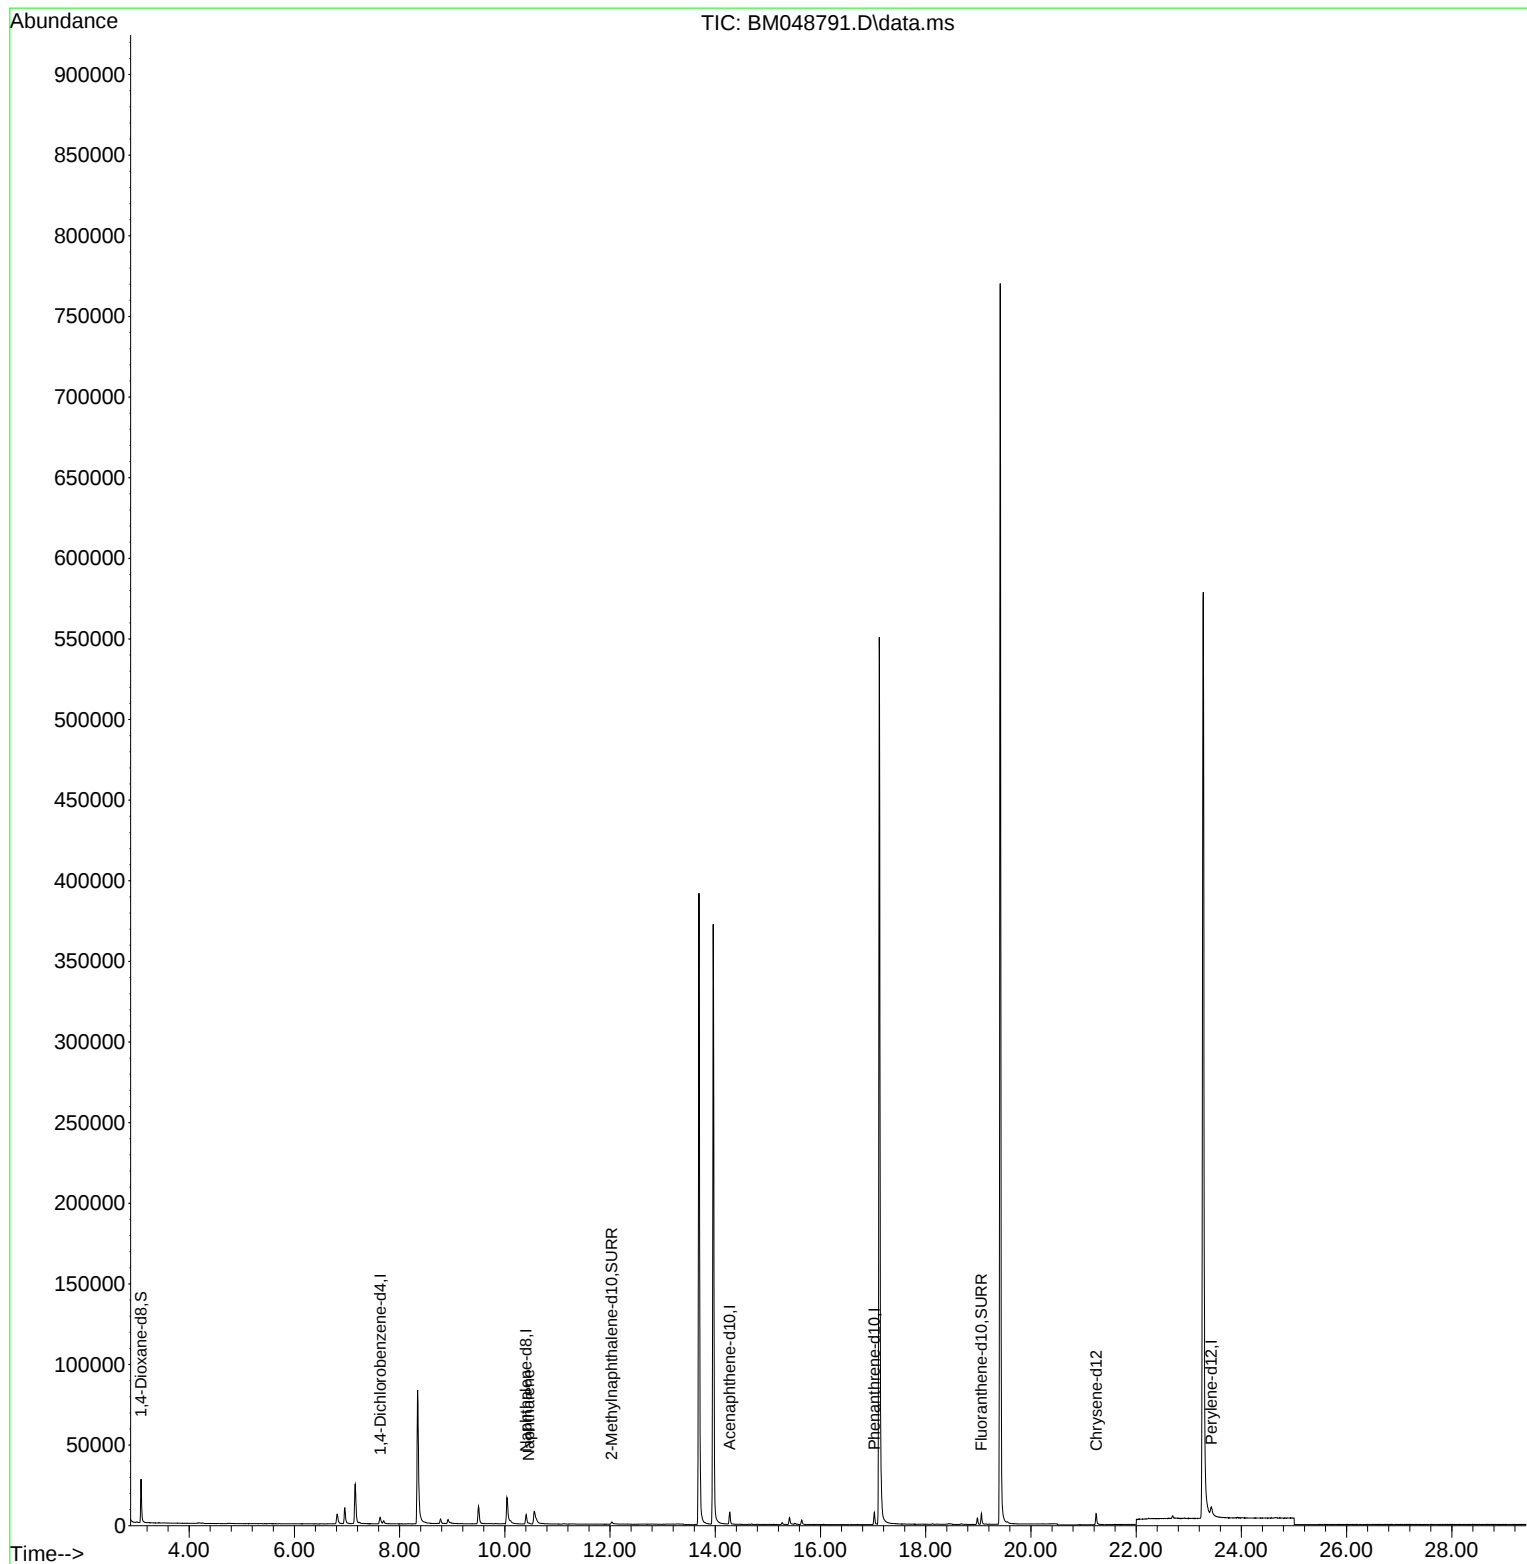

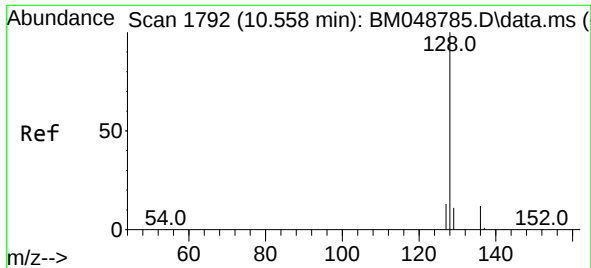

#5
Naphthalene
Concen: 0.035 ng/ul
RT: 10.454 min Scan# 11
Delta R.T. -0.083 min
Lab File: BM048791.D
Acq: 19 Nov 2024 00:29

Instrument :
BNA_M
ClientSampleId :
E29S6

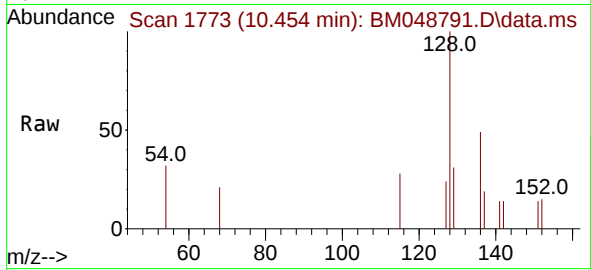

Tgt Ion:128 Resp: 764
Ion Ratio Lower Upper
128 100
129 30.6 10.0 15.0
127 23.9 10.9 16.3

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/19/2024
Supervised By :mohammad ahmed 11/20/2024

