

Data Path : Z:\HPCHEM1\BNA M\DATA\BM111915\
 Data File : BM003204.D
 Acq On : 19 Nov 2015 23:45
 Operator : UM/IZ
 Sample : G4323-24
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4J43

Quant Time: Nov 20 03:41:41 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-SIM-BM111815.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 20 03:16:26 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	242	0.40	ng/ul	0.00
4) Naphthalene-d8	10.53	136	1722	0.40	ng/ul	0.00
8) Acenaphthene-d10	14.38	164	3196	0.40	ng/ul	0.00
12) Phenanthrene-d10	17.23	188	3865129	0.40	ng/ul	0.10
18) Chrysene-d12	21.32	240	2493	0.40	ng/ul	-0.01
22) Perylene-d12	23.44	264	4140826	0.40	ng/ul	-0.15

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
2) 1,4-Dioxane-d8	3.20	96	86282	333.72	ng/uL	0.00
6) 2-Methylnaphthalene-d10	12.12	152	22224	9.49	ng/ul	0.00
16) Fluoranthene-d10	19.17	212	43595	0.00	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
5) Naphthalene	10.58	128	1752	0.40	ng/ul#	75
7) 2-Methylnaphthalene	12.19	142	250	0.09	ng/ul#	100
9) Acenaphthylene	14.07	152	426	0.03	ng/ul#	1
10) Acenaphthene	14.45	153	254	0.02	ng/ul#	79
11) Fluorene	15.49	166	400	0.03	ng/ul#	1
13) Pentachlorophenol	16.78	266	770	0.00	ng/ul#	22
14) Phenanthrene	17.23	178	1927	0.00	ng/ul#	1
15) Anthracene	17.23	178	2176	0.00	ng/ul#	1
17) Fluoranthene	19.35	202	244	0.00	ng/ul#	1
19) Pyrene	19.53	202	7425	0.87	ng/ul#	1
20) Benzo(a)anthracene	21.31	228	258	0.04	ng/ul#	1
21) Chrysene	21.36	228	412	0.05	ng/ul#	35
23) Benzo(b)fluoranthene	22.71	252	19	0.00	ng/ul#	1
24) Benzo(k)fluoranthene	22.83	252	80	0.00	ng/ul#	1
25) Benzo(a)pyrene	23.44	252	15412	0.00	ng/ul#	66
26) Indeno(1,2,3-cd)pyrene	25.66	276	10	0.00	ng/ul#	100
27) Dibenzo(a,h)anthracene	25.67	278	73	0.00	ng/ul#	1
28) Benzo(a,h,i)perylene	26.41	276	46	0.00	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM111915\
Data File : BM003204.D
Acq On : 19 Nov 2015 23:45
Operator : UM/IZ
Sample : G4323-24
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4J43

Quant Time: Nov 20 03:41:41 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-SIM-BM111815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 20 03:16:26 2015
Response via : Initial Calibration

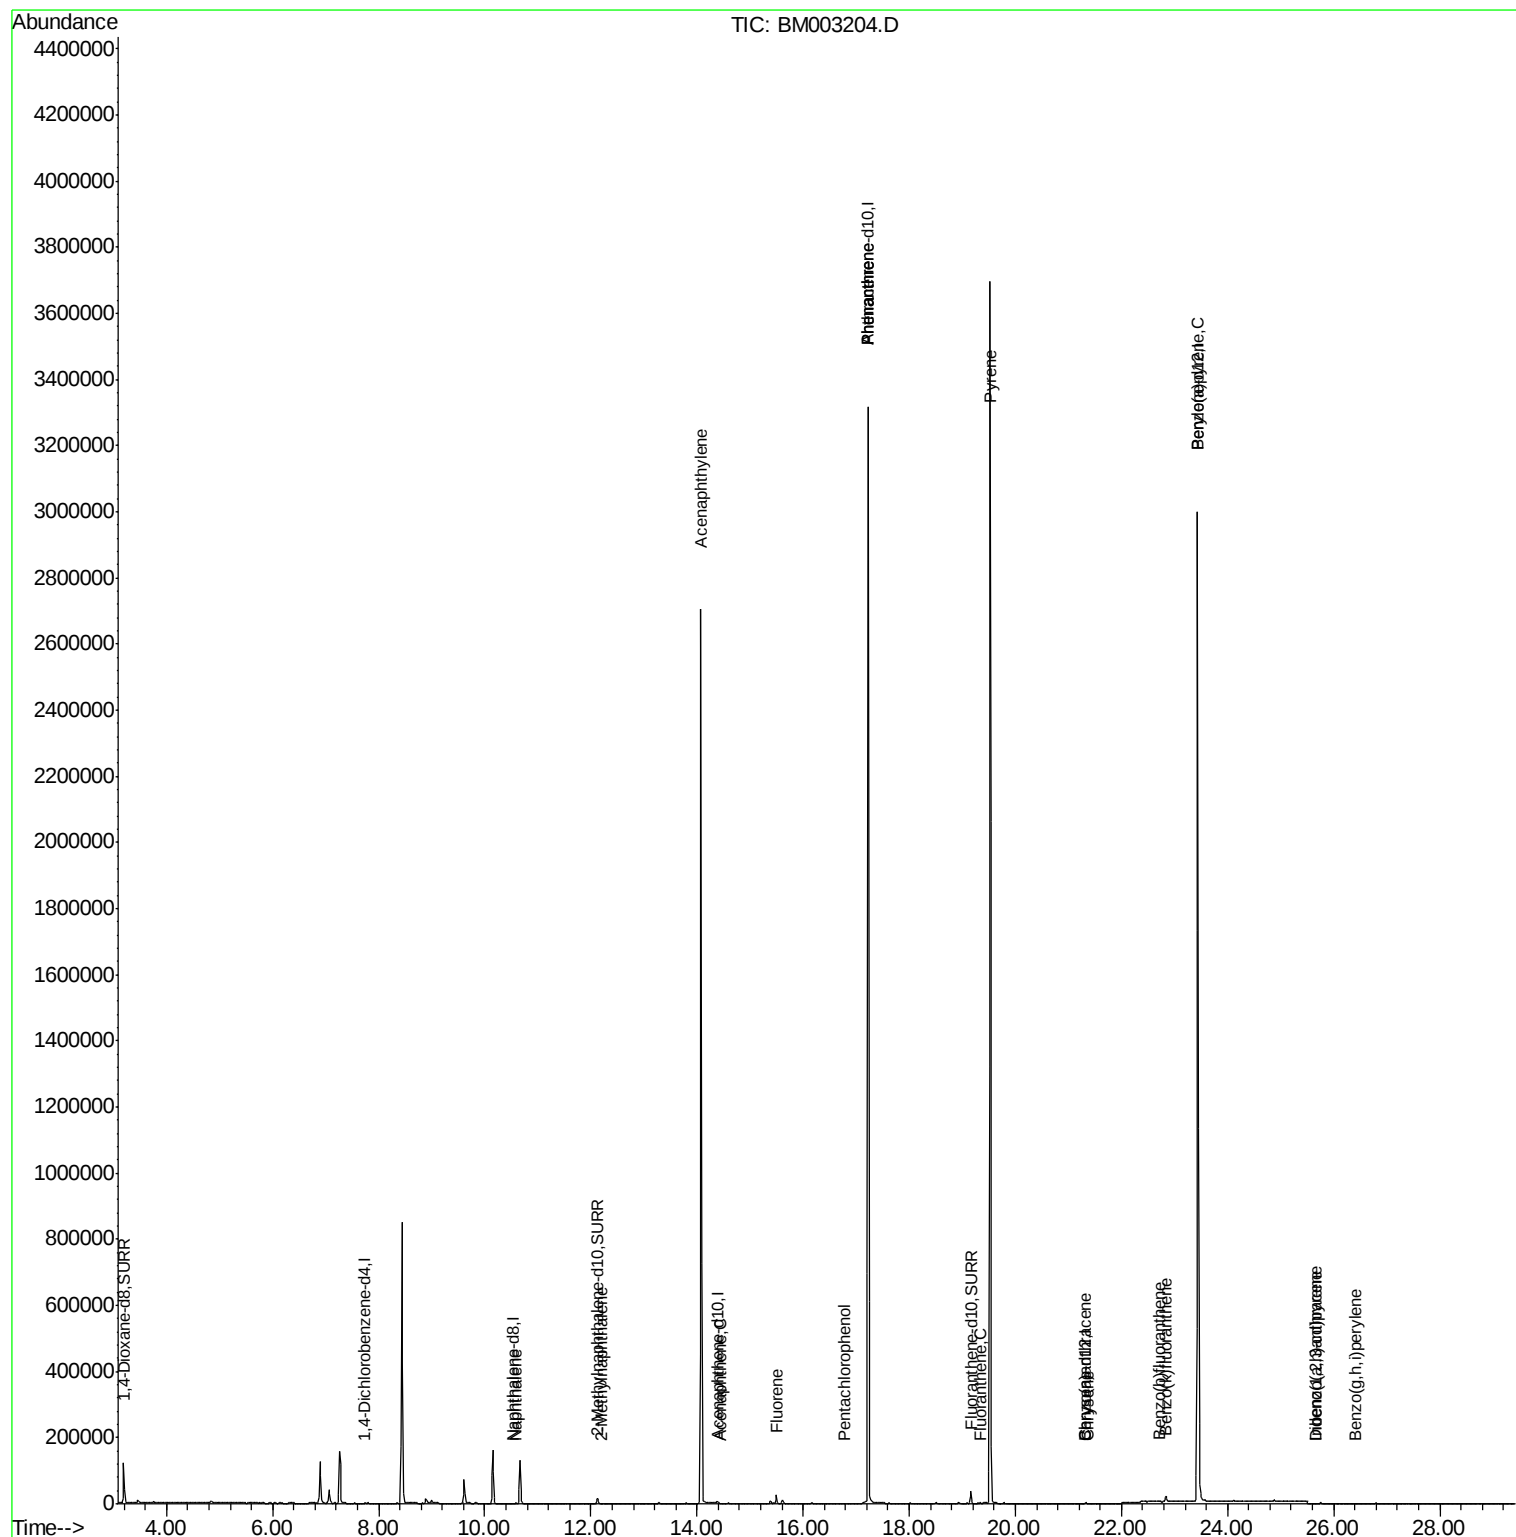

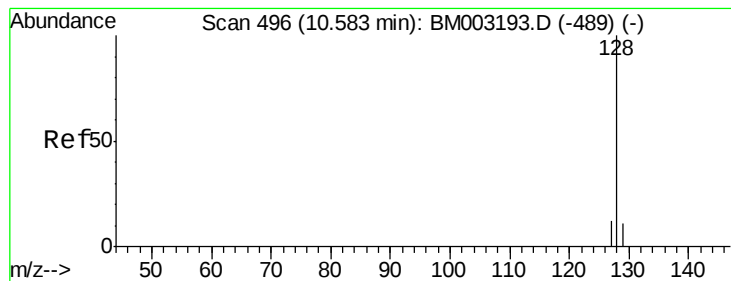

#5

Naphthalene

Concen: 0.40 ng/ul

RT: 10.58 min Scan# 496

Delta R.T. 0.00 min

Lab File: BM003204.D

Acq: 19 Nov 2015 23:45

Instrument :

BNA_M

ClientSampleId :

A4J43


Tot Ion:128 Resp: 1752

Ion Ratio Lower Upper

128 100

129 24.5 9.0 13.6#




127 18.6 9.6 14.4#



Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

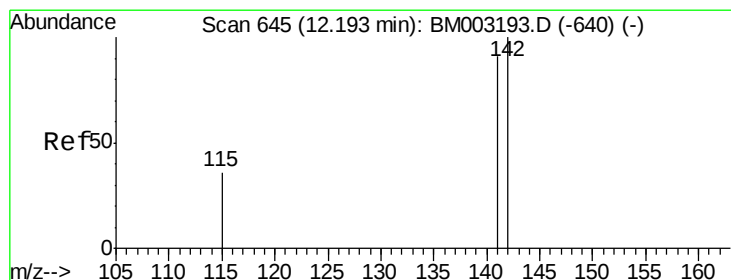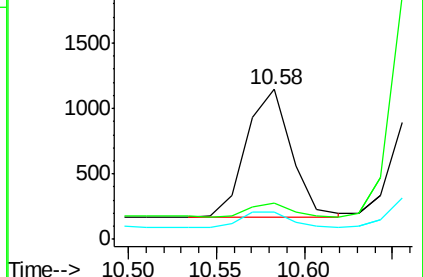

#7

2-Methylnaphthalene

Concen: 0.09 ng/ul

RT: 12.19 min Scan# 645

Delta R.T. 0.00 min

Lab File: BM003204.D


Acq: 19 Nov 2015 23:45

Tgt Ion:142 Resp: 250

Ion Ratio Lower Upper



142 100


141 90.8 0.0 0.0#



Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

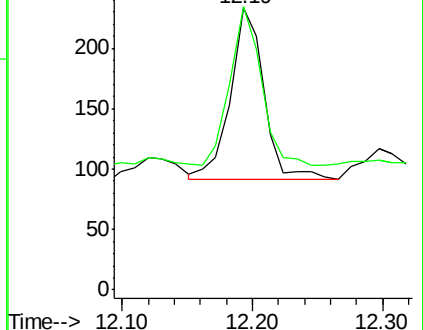



#9

Acenaphthylene

Concen: 0.03 ng/ul

RT: 14.07 min Scan# 823

Delta R.T. -0.02 min

Lab File: BM003204.D

Acq: 19 Nov 2015 23:45

Instrument :

BNA_M

ClientSampleId :

A4J43




Tot Ion:152 Resp: 426

Ion Ratio Lower Upper

152 100

151 53.8 17.6 26.4#

153 218.1 9.7 14.5#

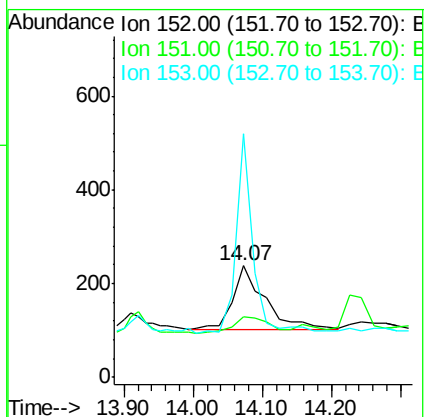

#10

Acenaphthene

Concen: 0.02 ng/ul

RT: 14.45 min Scan# 845

Delta R.T. 0.00 min

Lab File: BM003204.D

Acq: 19 Nov 2015 23:45




Tgt Ion:153 Resp: 254


Ion Ratio Lower Upper

153 100

152 83.4 33.9 50.9#

154 97.9 80.6 121.0



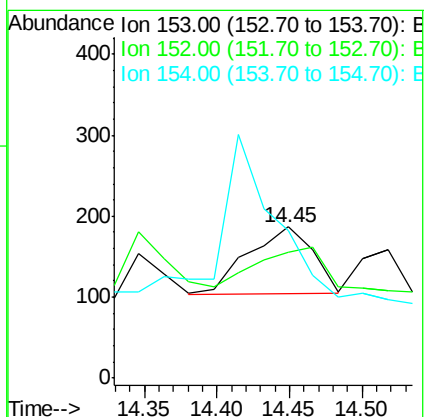





#11
 Fluorene
 Concen: 0.03 ng/ul
 RT: 15.49 min Scan# 906
 Delta R.T. 0.05 min
 Lab File: BM003204.D
 Acq: 19 Nov 2015 23:45




Instrument :
 BNA_M
 ClientSampleId :
 A4J43


Tot Ion:166 Resp: 400
 Ion Ratio Lower Upper
 166 100
 165 137.7 69.6 104.4#
 167 862.7 11.9 17.9#

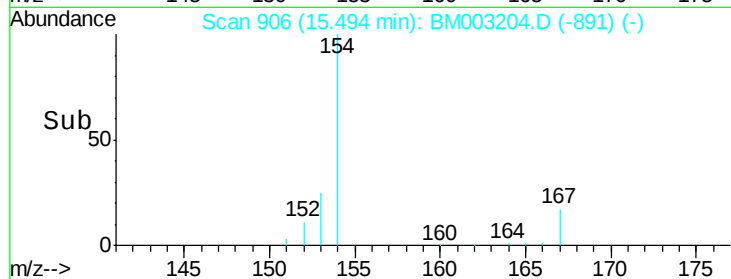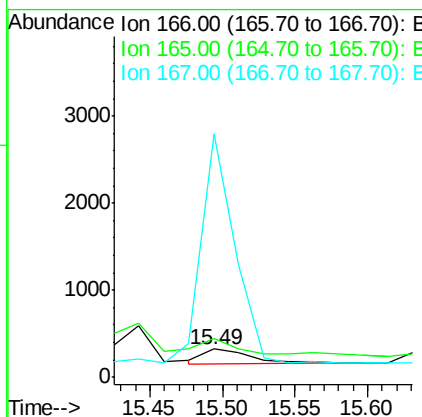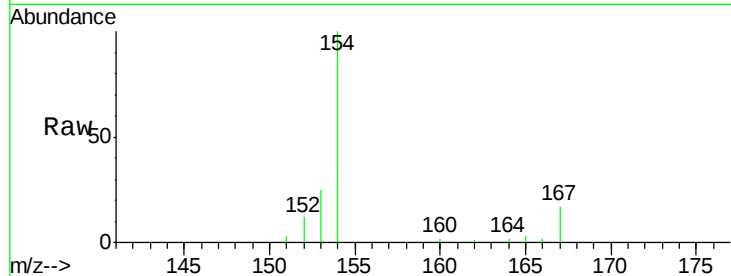

#13
 Pentachlorophenol
 Concen: 0.00 ng/ul
 RT: 16.78 min Scan# 981
 Delta R.T. 0.00 min
 Lab File: BM003204.D
 Acq: 19 Nov 2015 23:45

Tgt Ion:266 Resp: 770
 Ion Ratio Lower Upper
 266 100
 264 58.8 0.3 0.5#
 268 61.2 0.0 0.0#

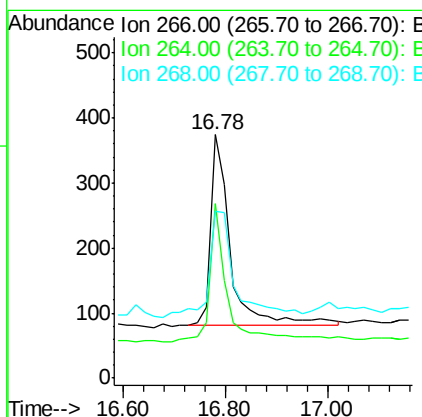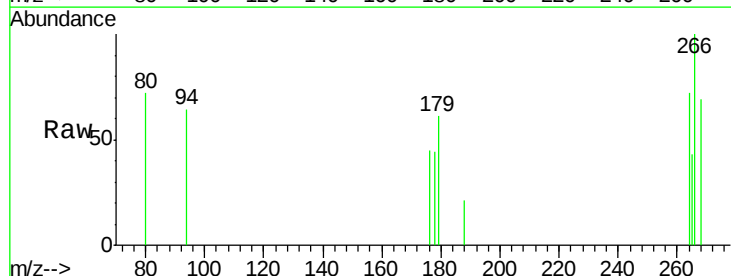

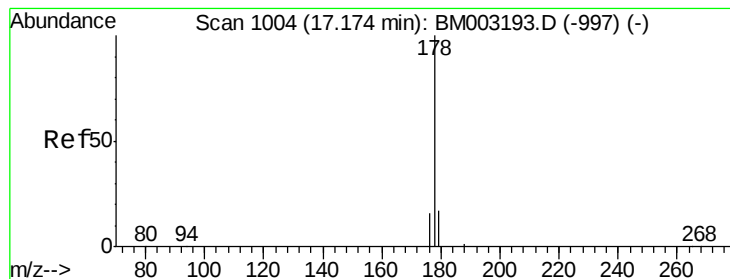

#14

Phenanthrene

Concen: 0.00 ng/ul

RT: 17.23 min Scan# 1007

Delta R.T. 0.05 min

Lab File: BM003204.D

Acq: 19 Nov 2015 23:45

Instrument :

BNA_M

ClientSampleId :

A4J43


Tot Ion:178 Resp: 1927

Ion Ratio Lower Upper

178 100

176 14.2 13.0 19.4




179 257.0 14.2 21.2#

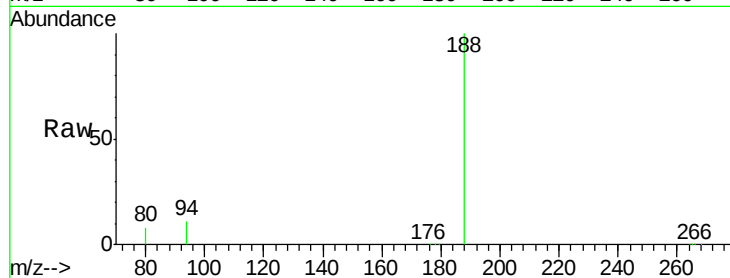

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

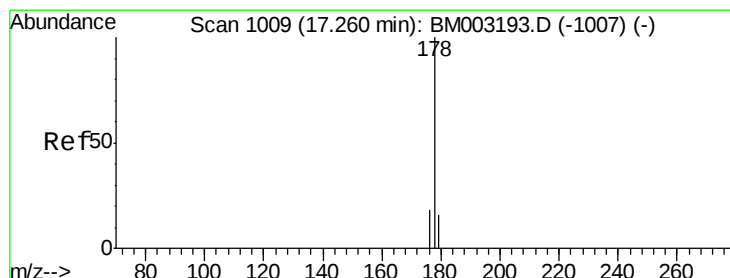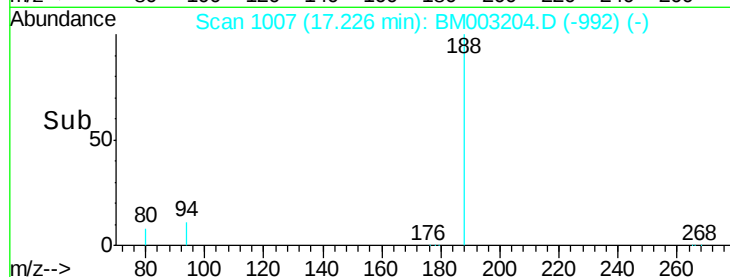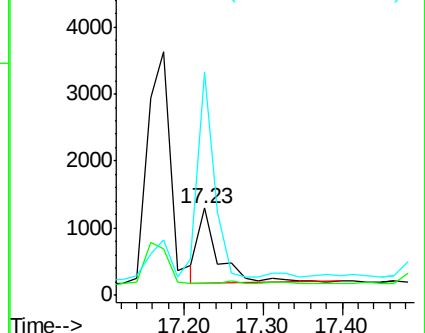

#15

Anthracene

Concen: 0.00 ng/ul

RT: 17.23 min Scan# 1007

Delta R.T. -0.03 min

Lab File: BM003204.D

Acq: 19 Nov 2015 23:45


Tgt Ion:178 Resp: 2176

Ion Ratio Lower Upper

178 100

176 14.2 14.0 21.0



179 257.0 12.9 19.3#

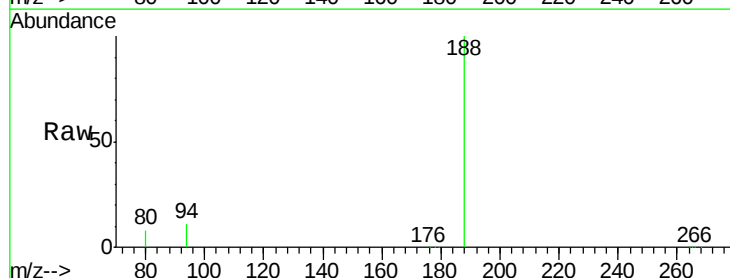


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

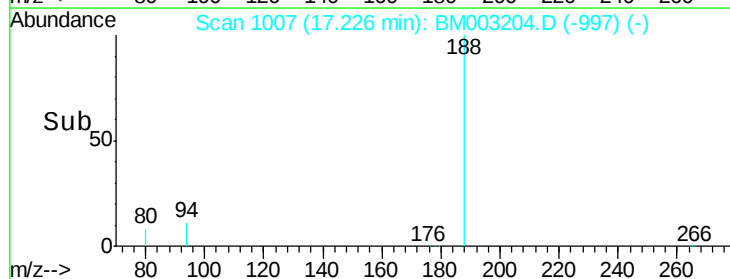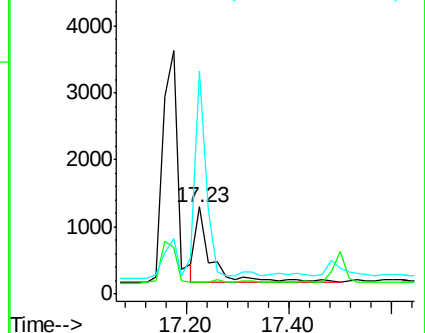



#17

Fluoranthene

Concen: 0.00 ng/ul

RT: 19.35 min Scan# 1139

Delta R.T. 0.16 min

Lab File: BM003204.D

Acq: 19 Nov 2015 23:45

Instrument :

BNA_M

ClientSampleId :

A4J43


Tot Ion:202 Resp: 244

Ion Ratio Lower Upper

202 100

101 128.4 0.0 29.6#




203 206.7 0.0 36.3#

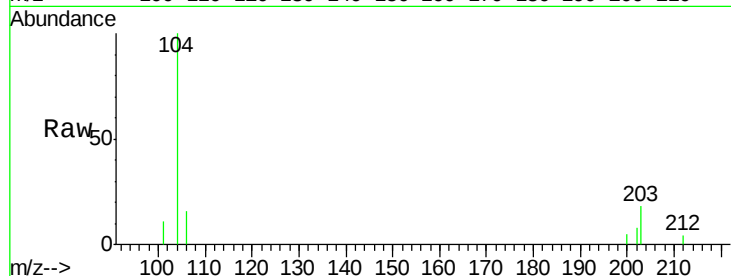

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

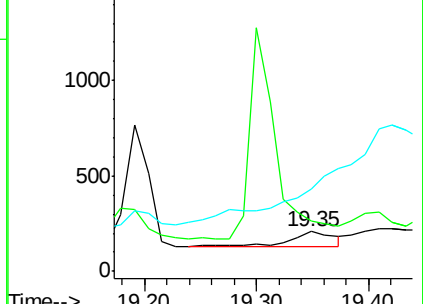

#19

Pyrene

Concen: 0.87 ng/ul

RT: 19.53 min Scan# 1154

Delta R.T. -0.02 min

Lab File: BM003204.D

Acq: 19 Nov 2015 23:45


Tgt Ion:202 Resp: 7425

Ion Ratio Lower Upper

202 100

200 5.1 17.8 26.8#



203 173.0 12.8 19.2#




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

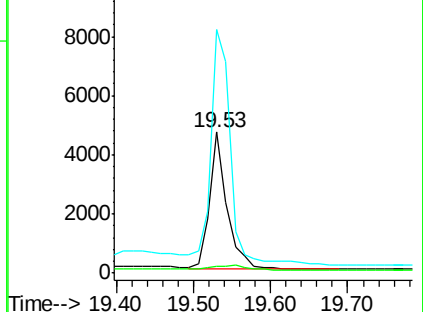

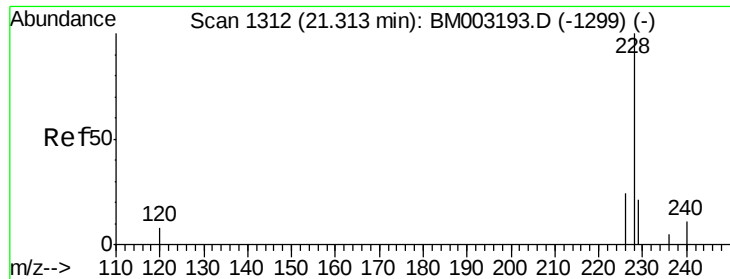

#20

Benzo(a)anthracene

Concen: 0.04 ng/ul

RT: 21.31 min Scan# 1312

Delta R.T. 0.00 min

Lab File: BM003204.D

Acq: 19 Nov 2015 23:45

Instrument :

BNA_M

ClientSampleId :

A4J43


Tot Ion:228 Resp: 258

Ion Ratio Lower Upper

228 100

226 65.3 18.8 28.2#




229 75.3 17.1 25.7#

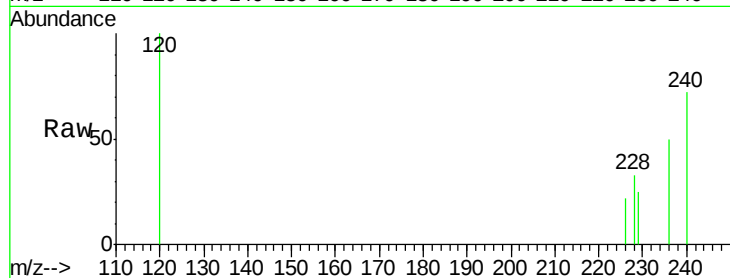

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

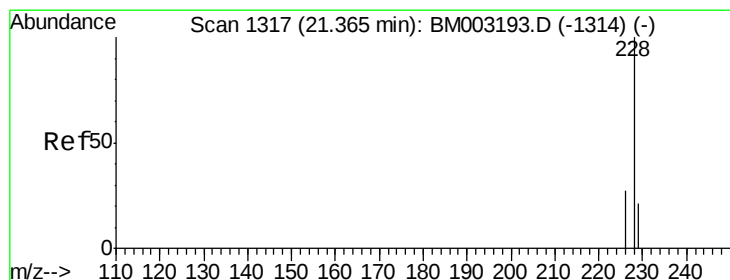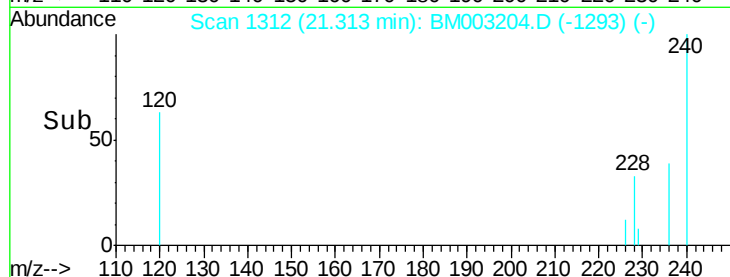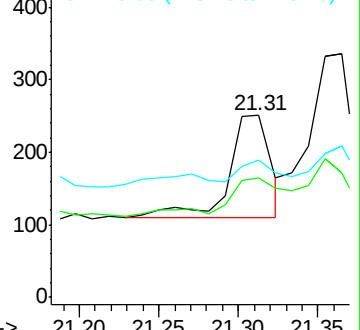

#21

Chrysene

Concen: 0.05 ng/ul

RT: 21.36 min Scan# 1317

Delta R.T. 0.00 min

Lab File: BM003204.D

Acq: 19 Nov 2015 23:45


Tgt Ion:228 Resp: 412

Ion Ratio Lower Upper

228 100

226 50.9 21.2 31.8#



229 61.9 17.0 25.6#

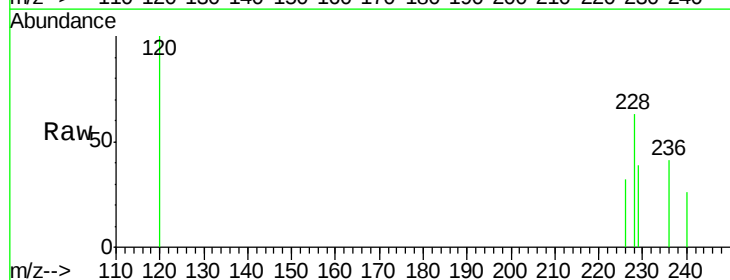


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

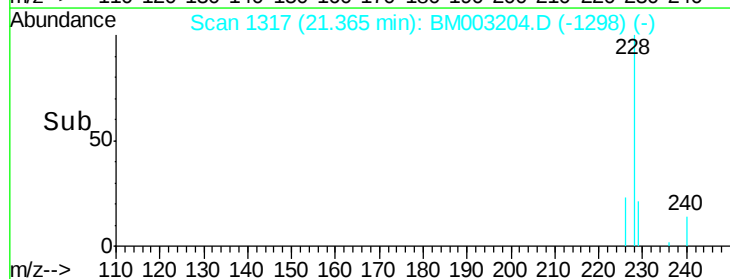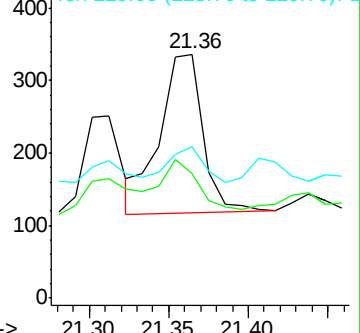

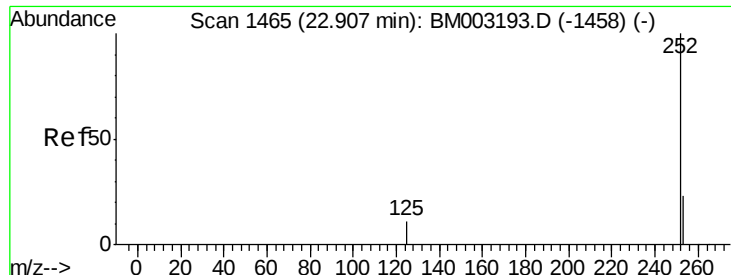

#23

Benzo(b)fluoranthene

Concen: 0.00 ng/u1

RT: 22.71 min Scan# 1446

Delta R.T. -0.20 min

Lab File: BM003204.D

Acq: 19 Nov 2015 23:45

Instrument :

BNA_M

ClientSampleId :

A4J43


Tot Ion:252 Resp: 19

Ion Ratio Lower Upper

252 100

253 184.4 0.0 45.4#




125 198.5 0.0 28.8#

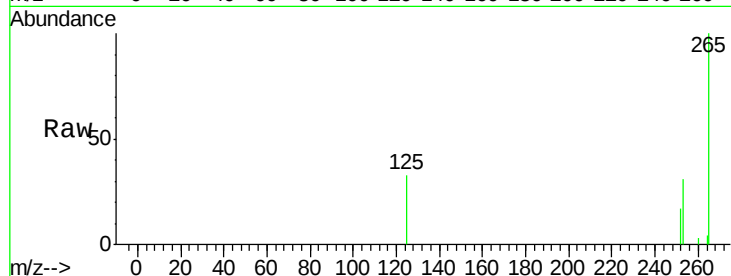

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

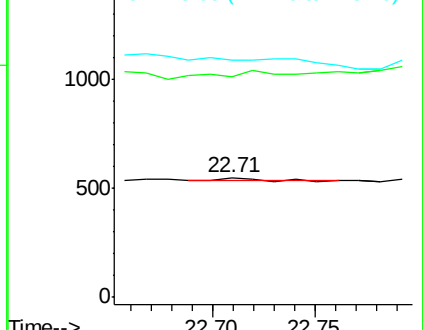

#24

Benzo(k)fluoranthene

Concen: 0.00 ng/u1

RT: 22.83 min Scan# 1458

Delta R.T. -0.11 min

Lab File: BM003204.D

Acq: 19 Nov 2015 23:45


Tgt Ion:252 Resp: 80

Ion Ratio Lower Upper

252 100

253 180.5 19.8 29.8#



125 491.7 10.4 15.6#




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

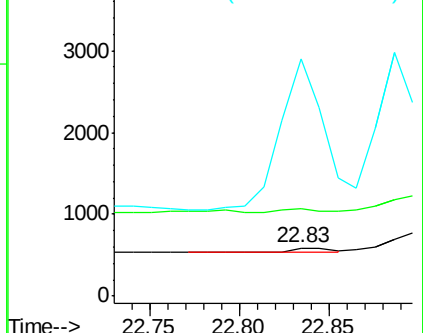

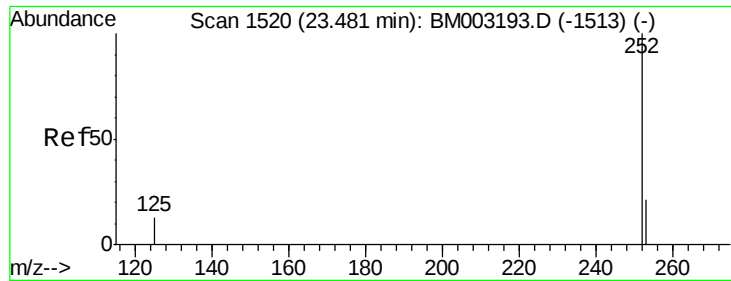

#25

Benzo(a)pyrene

Concen: 0.00 ng/u1

RT: 23.44 min Scan# 1516

Delta R.T. -0.04 min

Lab File: BM003204.D

Acq: 19 Nov 2015 23:45

Instrument :

BNA_M

ClientSampled :

A4J43


Tot Ion:252 Resp: 15412

Ion Ratio Lower Upper

252 100

253 37.2 19.4 29.2#




125 35.8 12.7 19.1#

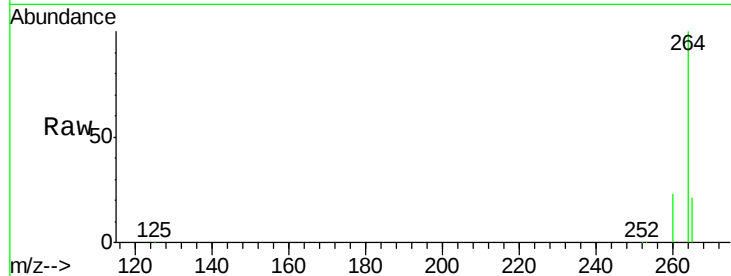

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

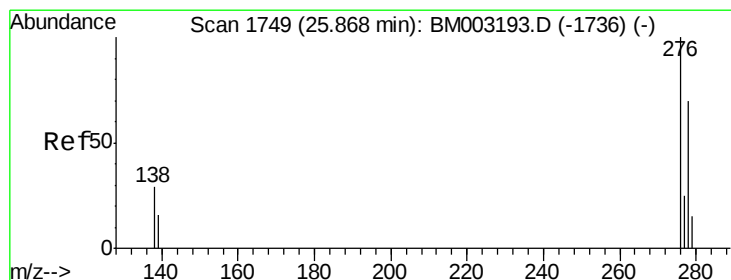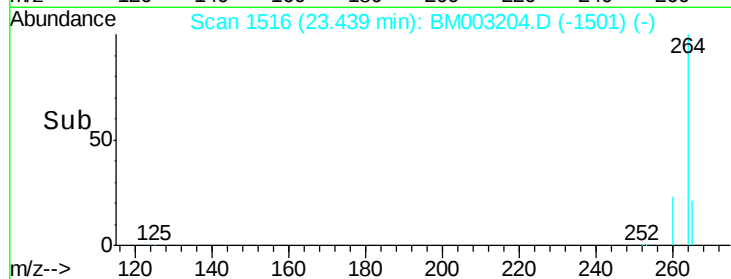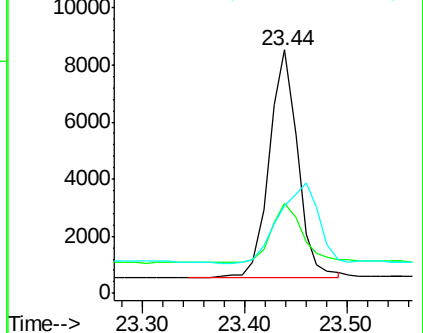

#26

Indeno(1,2,3-cd)pyrene

Concen: 0.00 ng/u1

RT: 25.66 min Scan# 1729

Delta R.T. -0.21 min

Lab File: BM003204.D

Acq: 19 Nov 2015 23:45


Tgt Ion:276 Resp: 10

Ion Ratio Lower Upper

276 100

138 0.0 0.0 0.0



277 0.0 0.0 0.0




Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E




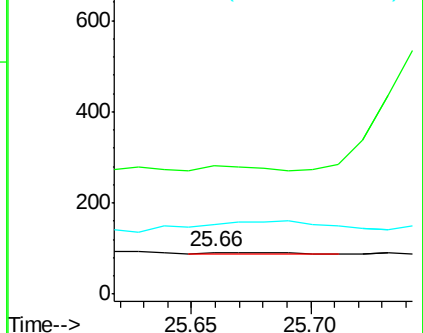




#27
Dibenzo(a,h)anthracene
Concen: 0.00 ng/ul
RT: 25.67 min Scan# 1730
Delta R.T. -0.21 min
Lab File: BM003204.D
Acq: 19 Nov 2015 23:45

Instrument :
BNA_M
ClientSampleId :
A4J43

Tot Ion:278 Resp: 73
Ion Ratio Lower Upper
278 100
139 293.6 16.4 24.6#
279 920.2 20.2 30.2#

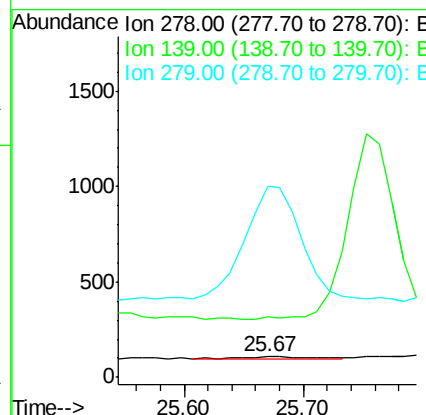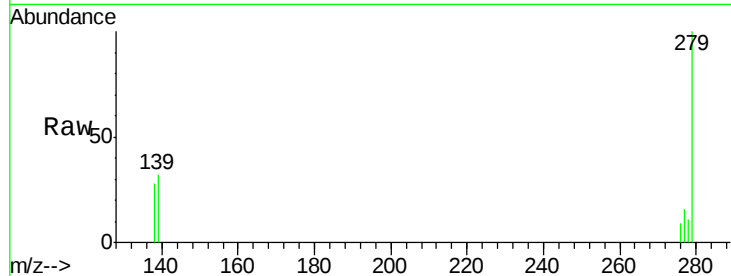

#28
Benzo(g,h,i)perylene
Concen: 0.00 ng/ul
RT: 26.41 min Scan# 1801
Delta R.T. -0.16 min
Lab File: BM003204.D
Acq: 19 Nov 2015 23:45

Tgt Ion:276 Resp: 46
Ion Ratio Lower Upper
276 100
277 141.5 18.9 28.3#
138 273.4 22.5 33.7#

