


Data Path : Z:\HPCHEM1\BNA M\Data\BM111915\
 Data File : BM003187.D
 Acq On : 19 Nov 2015 10:36
 Operator : UM/IZ
 Sample : DFTPP46
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP46

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM111815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 20 13:20:12 2015

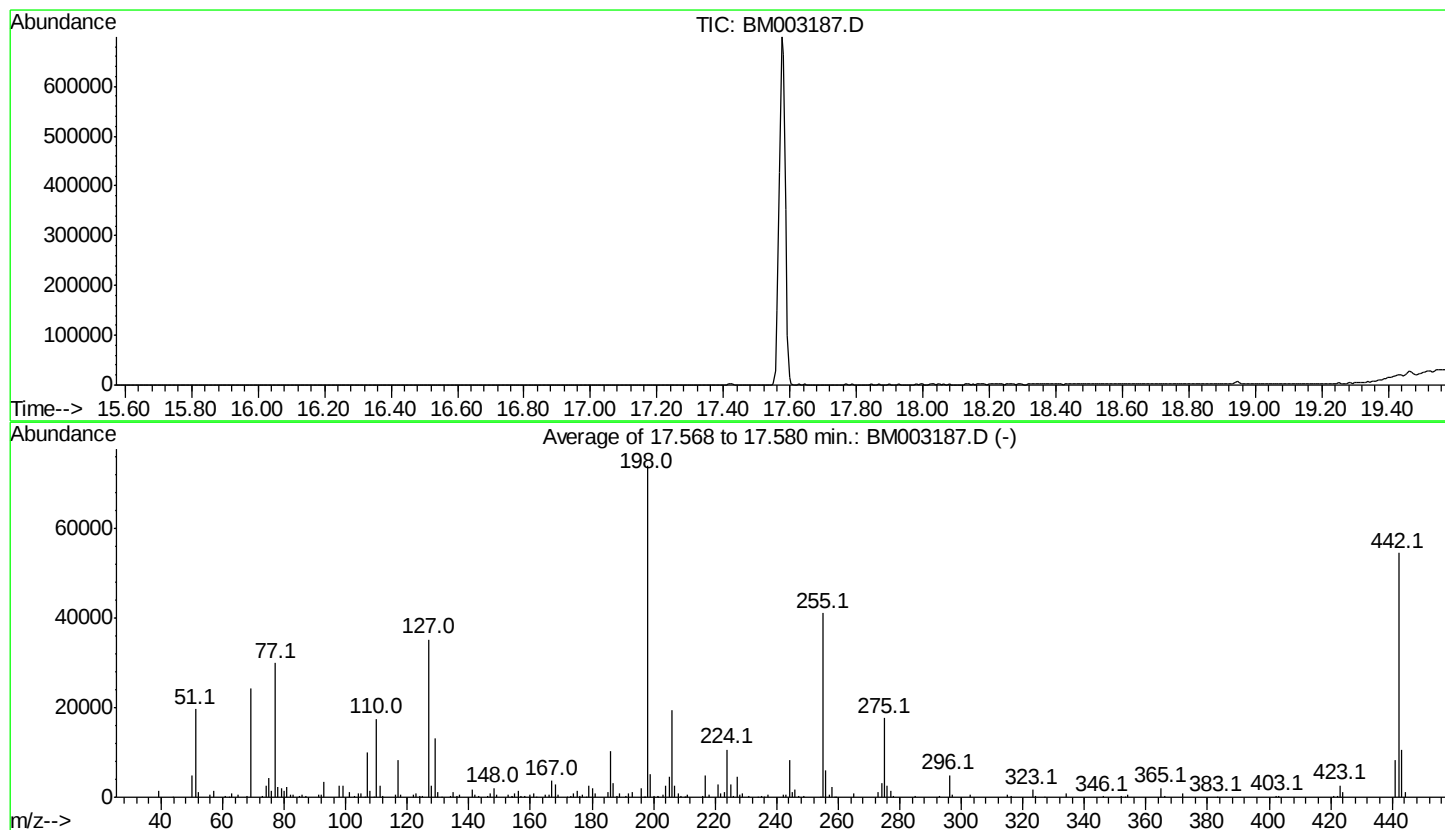

AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.6	19688	PASS
68	69	0.00	2	1.7	427	PASS
69	198	0.00	100	33.0	24434	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.6	35304	PASS
197	198	0.00	1	0.2	132	PASS
198	198	100	100	100.0	74144	PASS
199	198	5	9	6.8	5074	PASS
275	198	10	60	23.8	17625	PASS
365	198	1	100	2.8	2103	PASS
441	443	0.01	100	77.0	8231	PASS
442	198	50	100	73.7	54634	PASS
443	442	15	24	19.6	10690	PASS

Scan 2456 (17.533 min): BM003187.D
DFTPP46

m/z	Abundance
44.00	396.0
207.00	781.0

Instrument :
BNA_M
ClientSampleId :
DFTPP46

m/z	Abundance
39.00	1361.0
43.90	353.0
50.10	4263.0
51.10	16600.0
52.00	898.0
56.00	531.0
57.00	1265.0
63.00	728.0
65.00	395.0
68.00	343.0
69.00	20728.0
73.00	347.0
74.00	2151.0
75.00	3557.0
76.00	1062.0
77.10	25504.0
78.00	1883.0
79.00	1754.0
80.00	1195.0
81.00	1890.0
82.00	463.0
83.00	474.0
86.00	483.0
87.00	304.0
91.00	489.0
92.10	381.0
93.00	3086.0
98.00	2142.0
99.00	2399.0
101.00	1016.0
103.00	344.0
104.00	782.0
105.00	645.0
107.00	8115.0
108.00	1278.0
110.00	13861.0
111.00	2152.0
116.00	432.0
117.00	6365.0
117.90	559.0
122.00	412.0
123.00	844.0
125.00	317.0
127.00	27144.0
128.00	1904.0
129.00	10397.0
130.00	1020.0
135.00	919.0
137.00	570.0
141.00	1334.0
142.00	336.0
147.00	808.0
148.00	1667.0
149.00	565.0
153.00	475.0
153.90	319.0
155.00	789.0
156.00	1026.0
160.00	347.0
160.90	704.0
165.00	478.0
166.00	375.0
167.00	2719.0
168.00	2718.0
169.00	340.0
174.00	531.0
175.00	1062.0
176.10	323.0
177.00	480.0
179.00	1827.0
180.00	1792.0
181.00	688.0
185.00	933.0
186.10	7574.0
187.00	2459.0
188.00	334.0
189.00	526.0
191.00	347.0
192.00	629.0
193.00	699.0
196.00	1528.0
198.00	53600.0
199.00	3832.0
201.50	380.0
203.00	374.0
204.00	1913.0
205.00	3477.0
206.10	14102.0
207.00	2661.0
208.00	695.0
210.90	493.0
217.00	3510.0

Instrument :
BNA_M
ClientSampleId :
DFTPP46

218.00	510.0
221.00	1802.0
222.00	534.0
223.00	803.0
224.00	7530.0
225.00	1915.0
227.00	3201.0
228.00	508.0
229.00	733.0
237.00	441.0
242.00	367.0
243.10	408.0
244.10	5725.0
245.00	723.0
246.00	1140.0
255.10	28080.0
256.00	4167.0
257.00	383.0
258.00	1642.0
265.00	714.0
273.00	1063.0
274.10	2071.0
275.10	11628.0
276.00	1578.0
277.00	1031.0
296.10	3235.0
297.10	408.0
303.10	345.0
315.10	355.0
323.10	989.0
334.00	648.0
354.10	374.0
365.00	1213.0
372.10	402.0
423.10	1593.0
424.10	607.0
441.10	4434.0
442.10	29976.0
443.10	6003.0
444.10	607.0

Instrument :
BNA_M
ClientSampleId :
DFTPP46

m/z	Abundance
39.00	1887.0
44.00	482.0
50.10	5682.0
51.10	23312.0
52.00	1281.0
55.90	662.0
57.00	1760.0
61.00	331.0
61.90	399.0
63.00	1074.0
65.00	574.0
68.00	567.0
69.00	28432.0
73.00	363.0
74.00	3049.0
75.00	5035.0
76.00	1706.0
77.10	34784.0
78.00	2665.0
79.00	2246.0
80.00	1649.0
81.00	2503.0
82.00	637.0
83.00	628.0
85.00	462.0
86.00	751.0
87.00	414.0
91.00	668.0
92.00	623.0
93.00	4136.0
98.00	3006.0
99.00	3030.0
101.00	1510.0
103.00	483.0
104.00	863.0
105.00	946.0
107.00	11243.0
108.00	1775.0
109.00	344.0
110.00	20912.0
111.00	3233.0
112.00	442.0
116.00	655.0
117.00	9738.0
118.00	705.0
122.00	716.0
123.00	1106.0
123.90	541.0
124.90	515.0
127.00	41816.0
128.00	3165.0
129.00	15292.0
130.00	1429.0
131.00	323.0
134.00	533.0
135.00	1425.0
136.00	542.0
137.00	736.0
141.00	2058.0
142.00	734.0
143.00	457.0
146.00	394.0
147.00	1192.0
148.00	2594.0
149.00	689.0
152.90	747.0
154.10	422.0
155.00	1123.0
156.00	1823.0
157.00	330.0
158.00	430.0
160.00	744.0
161.00	1008.0
162.00	364.0
165.00	781.0
166.00	642.0
167.00	4168.0
168.00	3327.0
169.00	616.0
171.90	411.0
172.90	457.0
174.00	949.0
175.00	1831.0
176.10	561.0
177.00	787.0
178.00	309.0
179.00	3313.0
180.00	2539.0
181.00	1043.0
185.00	1462.0
186.00	12162.0
187.00	3374.0

Instrument :
BNA_M
ClientSampleId :
DFTPP46

188.00	500.0
189.00	916.0
191.00	346.0
192.00	1066.0
193.00	1115.0
196.10	2513.0
197.10	397.0
198.00	86536.0
199.00	6060.0
199.90	472.0
201.20	316.0
203.00	552.0
204.00	3163.0
205.10	5178.0
206.10	23400.0
207.10	3956.0
208.00	947.0
209.10	385.0
210.10	322.0
211.10	805.0
216.00	481.0
217.00	5665.0
218.00	822.0
221.00	3252.0
221.80	949.0
223.00	1165.0
224.10	12331.0
225.10	3262.0
226.10	378.0
227.00	5195.0
228.00	788.0
229.00	1194.0
231.00	439.0
234.90	379.0
236.00	307.0
237.00	578.0
242.10	658.0
243.10	652.0
244.10	9995.0
245.10	1207.0
246.00	1670.0
247.00	340.0
248.90	375.0
254.10	319.0
255.10	48080.0
256.10	6862.0
257.00	691.0
258.10	2727.0
258.90	354.0
265.00	1165.0
273.10	1231.0
274.00	3808.0
275.10	20120.0
276.00	2940.0
277.00	1790.0
277.90	402.0
285.10	366.0
293.10	467.0
296.10	5853.0
297.00	799.0
303.00	666.0
315.00	690.0
316.10	401.0
323.10	1813.0
324.10	384.0
334.10	1112.0
346.10	451.0
352.10	501.0
354.10	528.0
365.10	2444.0
366.00	400.0
372.10	871.0
402.10	362.0
403.10	515.0
421.10	421.0
422.00	532.0
423.10	3019.0
424.10	1344.0
441.10	9452.0
442.10	61080.0
443.10	12356.0
444.10	1198.0

Instrument :
BNA_M
ClientSampleId :
DFTPP46

m/z	Abundance
39.10	1395.0
44.00	387.0
50.10	4932.0
51.10	19152.0
52.00	957.0
56.00	685.0
57.00	1328.0
61.00	361.0
63.00	887.0
65.00	523.0
67.90	373.0
69.00	24144.0
73.10	324.0
74.00	2563.0
75.00	3987.0
76.00	1439.0
77.10	29752.0
78.10	2112.0
79.00	1861.0
80.00	1469.0
81.00	2110.0
82.10	540.0
83.00	431.0
85.00	495.0
85.90	688.0
91.00	545.0
92.00	583.0
93.00	3501.0
98.00	2717.0
99.00	2337.0
101.00	1321.0
102.90	423.0
104.00	803.0
105.00	774.0
106.00	307.0
107.00	10439.0
108.00	1382.0
110.00	18032.0
111.00	2678.0
112.00	431.0
116.00	510.0
117.00	8479.0
118.00	668.0
122.00	606.0
123.00	885.0
123.90	581.0
125.00	478.0
127.00	36952.0
128.00	2735.0
129.00	13739.0
130.00	1125.0
134.00	431.0
135.00	1092.0
136.00	586.0
137.00	779.0
140.90	1921.0
142.10	714.0
143.00	468.0
146.00	339.0
146.90	912.0
148.00	2076.0
149.10	534.0
153.00	509.0
153.90	492.0
155.00	1015.0
156.00	1609.0
156.90	305.0
157.90	356.0
160.00	499.0
161.00	979.0
165.00	824.0
165.90	523.0
167.00	4003.0
168.00	2915.0
169.00	484.0
173.00	632.0
174.00	931.0
175.10	1433.0
176.00	396.0
177.00	851.0
179.00	2894.0
180.00	2086.0
181.00	997.0
185.00	1440.0
186.00	11068.0
187.00	3528.0
188.00	378.0
189.00	834.0
191.00	417.0
192.00	942.0
193.00	1255.0
196.00	2270.0

Instrument :
BNA_M
ClientSampleId :
DFTPP46

196.80	398.0
198.00	82296.0
199.00	5331.0
200.00	405.0
201.30	341.0
202.90	627.0
204.00	3027.0
205.10	5067.0
206.10	21048.0
207.10	3449.0
208.00	945.0
209.00	376.0
210.30	375.0
211.00	858.0
216.00	456.0
217.00	5230.0
218.00	656.0
221.10	3557.0
221.90	731.0
223.00	1083.0
224.10	12233.0
225.00	3074.0
226.10	468.0
227.00	5130.0
228.00	623.0
229.00	1023.0
231.00	346.0
234.00	414.0
234.90	397.0
237.00	552.0
242.10	707.0
243.00	663.0
244.10	9213.0
245.00	1252.0
246.00	2076.0
247.00	316.0
249.00	338.0
255.10	47464.0
256.10	6631.0
257.00	584.0
258.00	2512.0
259.10	458.0
265.00	1131.0
273.00	1349.0
274.00	3953.0
275.10	21128.0
276.10	2973.0
277.00	1757.0
278.00	345.0
285.10	387.0
293.00	374.0
296.00	5913.0
297.00	835.0
303.00	681.0
315.00	619.0
316.10	437.0
323.10	2044.0
324.00	304.0
327.00	403.0
334.10	1259.0
346.00	388.0
352.10	567.0
353.00	366.0
354.10	704.0
365.10	2652.0
366.00	327.0
372.10	936.0
383.10	300.0
402.10	332.0
403.00	557.0
421.10	509.0
422.10	539.0
423.10	3531.0
424.10	1312.0
441.10	10809.0
442.10	72848.0
443.10	13712.0
444.10	1324.0

Instrument :
BNA_M
ClientSampleId :
DFTPP46