

Data Path : Z:\HPCHEM1\BNA M\DATA\BM112017\
 Data File : BM013047.D
 Acq On : 20 Nov 2017 15:14
 Operator : SJ/JU
 Sample : PB104370BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK70

Quant Time: Nov 21 00:44:26 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM111617.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 20 17:14:21 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	217584	20.00	ng/ul	0.00
18) Naphthalene-d8	10.50	136	949112	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.36	164	579338	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.10	188	1235928	20.00	ng/ul	0.00
75) Chrysene-d12	21.29	240	1018828	20.00	ng/ul	0.00
83) Perylene-d12	23.52	264	874651	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.25	96	22346	4.76	ng/uL	0.00
5) Phenol-d5	6.89	99	515500	27.35	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.06	67	316232	29.57	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	424312	28.17	ng/ul	0.00
13) 4-Methylphenol-d8	8.42	113	441939	28.63	ng/ul	0.00
19) Nitrobenzene-d5	8.87	128	222086	32.83	ng/ul	0.00
22) 2-Nitrophenol-d4	9.59	143	243275	37.81	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.12	165	438667	26.86	ng/ul	0.00
29) 4-Chloroaniline-d4	10.64	131	614256	35.97	ng/ul	0.00
43) Dimethylphthalate-d6	13.77	166	1627134	32.02	ng/ul	0.00
46) Acenaphthylene-d8	14.05	160	1861651	28.75	ng/ul	0.00
51) 4-Nitrophenol-d4	14.56	143	241123	31.28	ng/ul	0.00
57) Fluorene-d10	15.35	176	1295803	30.01	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.47	200	202771	37.84	ng/ul	0.00
70) Anthracene-d10	17.20	188	2093072	33.08	ng/ul	0.00
76) Pyrene-d10	19.50	212	2089322	40.14	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.38	264	1595879	35.98	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) 2,6-Dinitrotoluene	13.77	165	10003	1.35	ng/ul#	27




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM112017\
Data File : BM013047.D
Acq On : 20 Nov 2017 15:14
Operator : SJ/JU
Sample : PB104370BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK70

Quant Time: Nov 21 00:44:26 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM111617.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Nov 20 17:14:21 2017
Response via : Initial Calibration

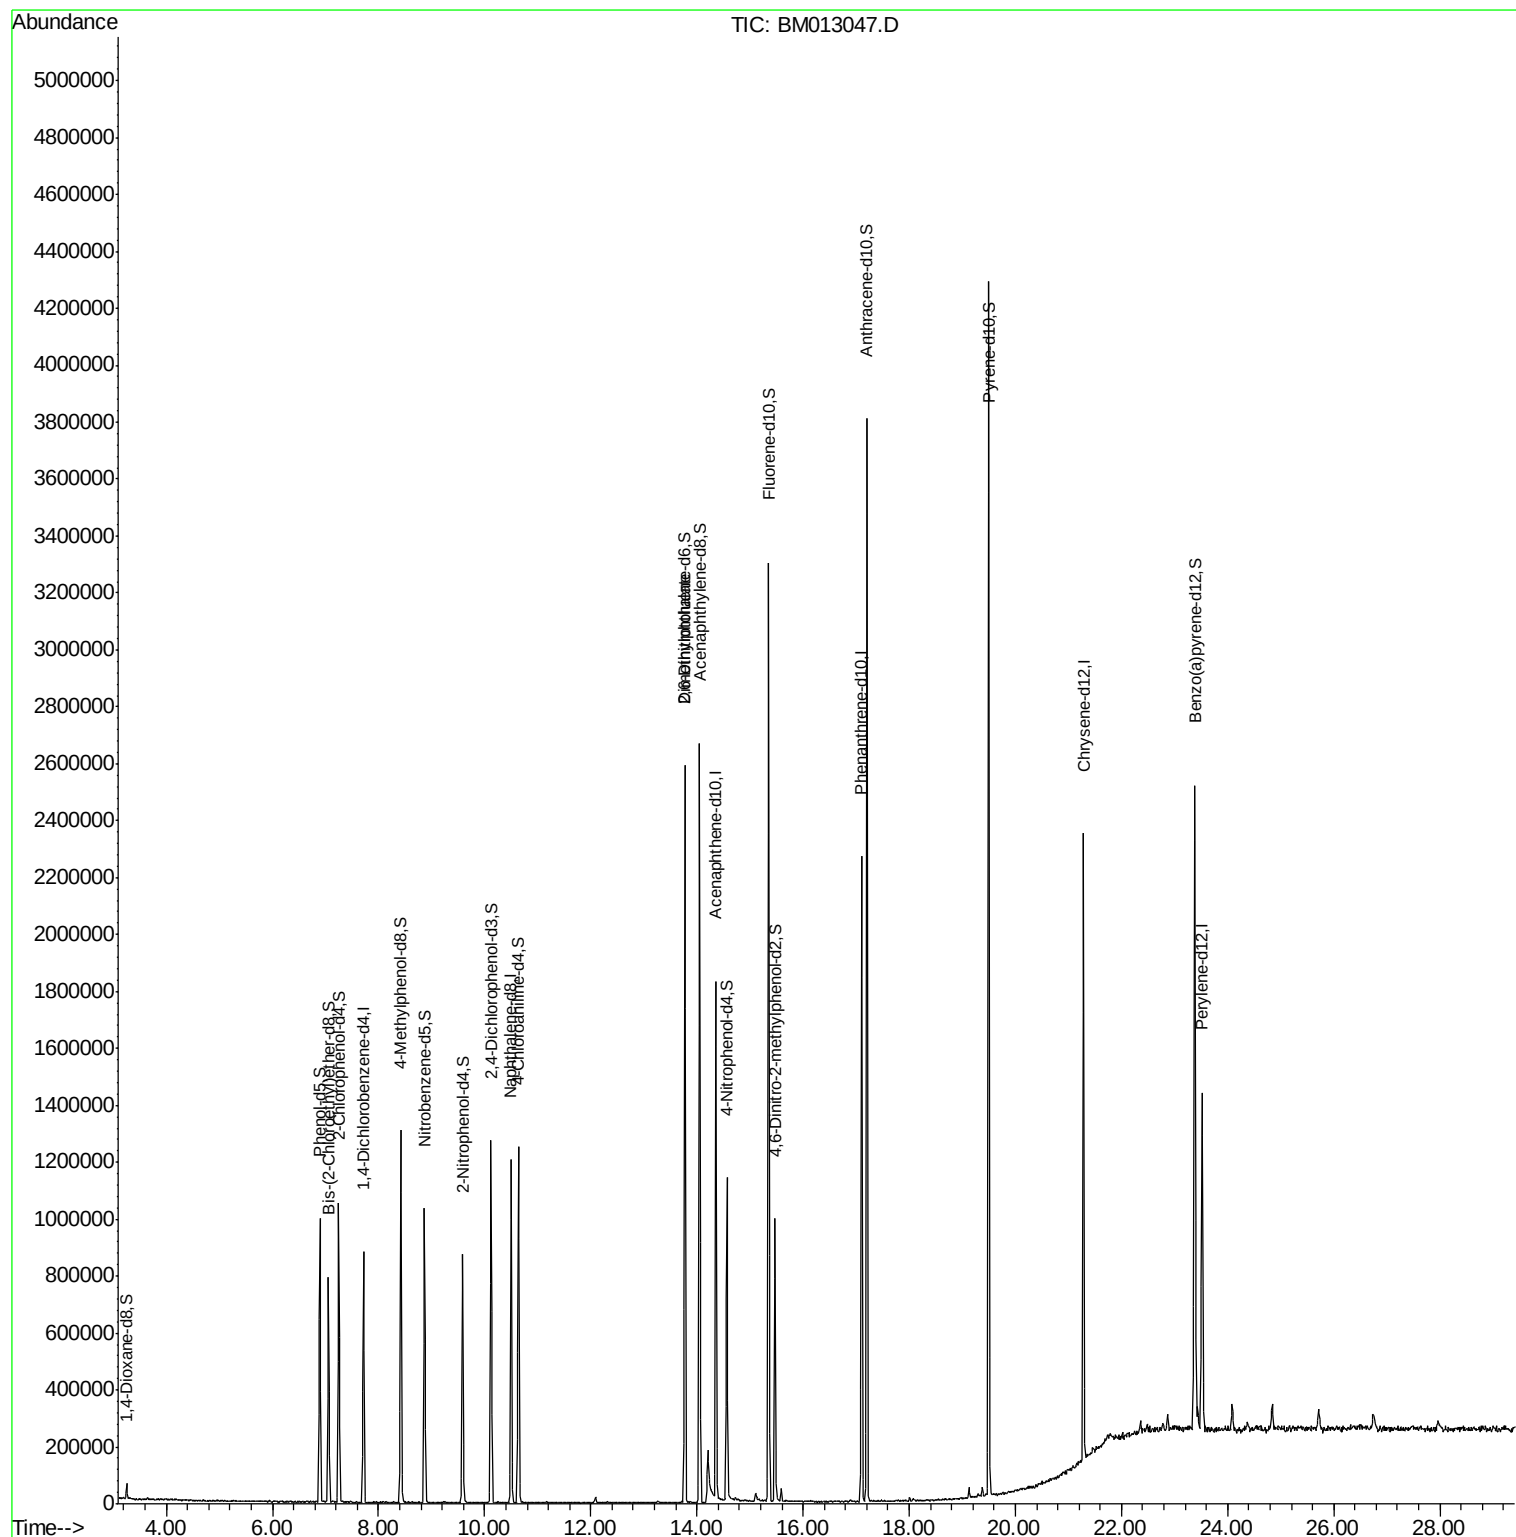

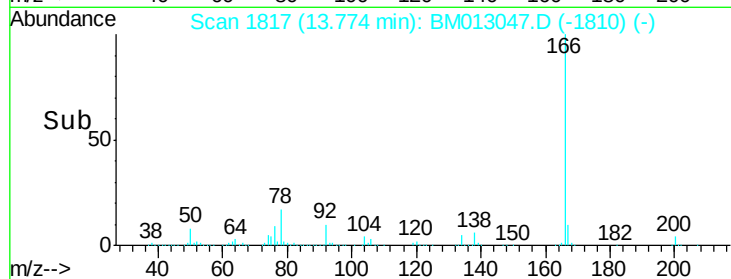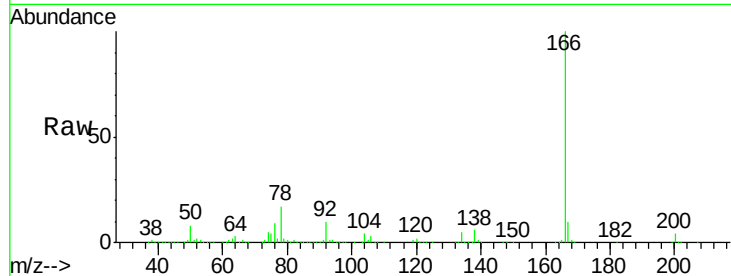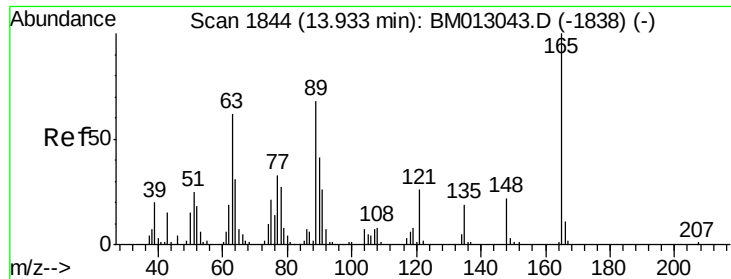

#45

2,6-Dinitrotoluene

Concen: 1.35 ng/ul

RT: 13.77 min Scan# 1817

Delta R.T. -0.16 min

Lab File: BM013047.D

Acq: 20 Nov 2017 15:14

Instrument :

BNA_M

ClientSampleId :

SBLK70

Tot Ion:165 Resp: 10003

Ion Ratio Lower Upper

165 100

89 4.4 52.6 79.0#

121 43.2 14.6 22.0#

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 89.00 (88.70 to 89.70): BM0

Ion 121.00 (120.70 to 121.70): E

