

Data Path : Z:\HPCHEM1\BNA M\DATA\BM112017\
 Data File : BM013050.D
 Acq On : 20 Nov 2017 17:01
 Operator : SJ/JU
 Sample : I6496-12
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0B95

Quant Time: Nov 21 00:45:01 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM111617.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 20 17:14:21 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	205817	20.00	ng/ul	0.00
18) Naphthalene-d8	10.50	136	878889	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.36	164	539277	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.10	188	1157307	20.00	ng/ul	0.00
75) Chrysene-d12	21.29	240	953770	20.00	ng/ul	0.00
83) Perylene-d12	23.52	264	813662	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.25	96	26321	5.92	ng/uL	0.00
5) Phenol-d5	6.89	99	135873	7.62	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.06	67	342534	33.86	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	378698	26.58	ng/ul	0.00
13) 4-Methylphenol-d8	8.42	113	253771	17.38	ng/ul	0.00
19) Nitrobenzene-d5	8.87	128	245637	39.22	ng/ul	0.00
22) 2-Nitrophenol-d4	9.59	143	261769	43.93	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.12	165	460770	30.46	ng/ul	0.00
29) 4-Chloroaniline-d4	10.63	131	1919	0.12	ng/ul	0.00
43) Dimethylphthalate-d6	13.77	166	1719335	36.35	ng/ul	0.00
46) Acenaphthylene-d8	14.05	160	2082113	34.54	ng/ul	0.00
51) 4-Nitrophenol-d4	14.56	143	48980	6.83	ng/ul	0.00
57) Fluorene-d10	15.35	176	1397455	34.76	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.47	200	209561	41.76	ng/ul	0.00
70) Anthracene-d10	17.20	188	2123672	35.84	ng/ul	0.00
76) Pyrene-d10	19.50	212	2040912	41.89	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.38	264	1542136	37.38	ng/ul	0.00


Target Compounds					Ovalue
45) 2,6-Dinitrotoluene	13.78	165	10748	1.56 ng/ul#	33




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM112017\
Data File : BM013050.D
Acq On : 20 Nov 2017 17:01
Operator : SJ/JU
Sample : I6496-12
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B95

Quant Time: Nov 21 00:45:01 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM111617.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Nov 20 17:14:21 2017
Response via : Initial Calibration

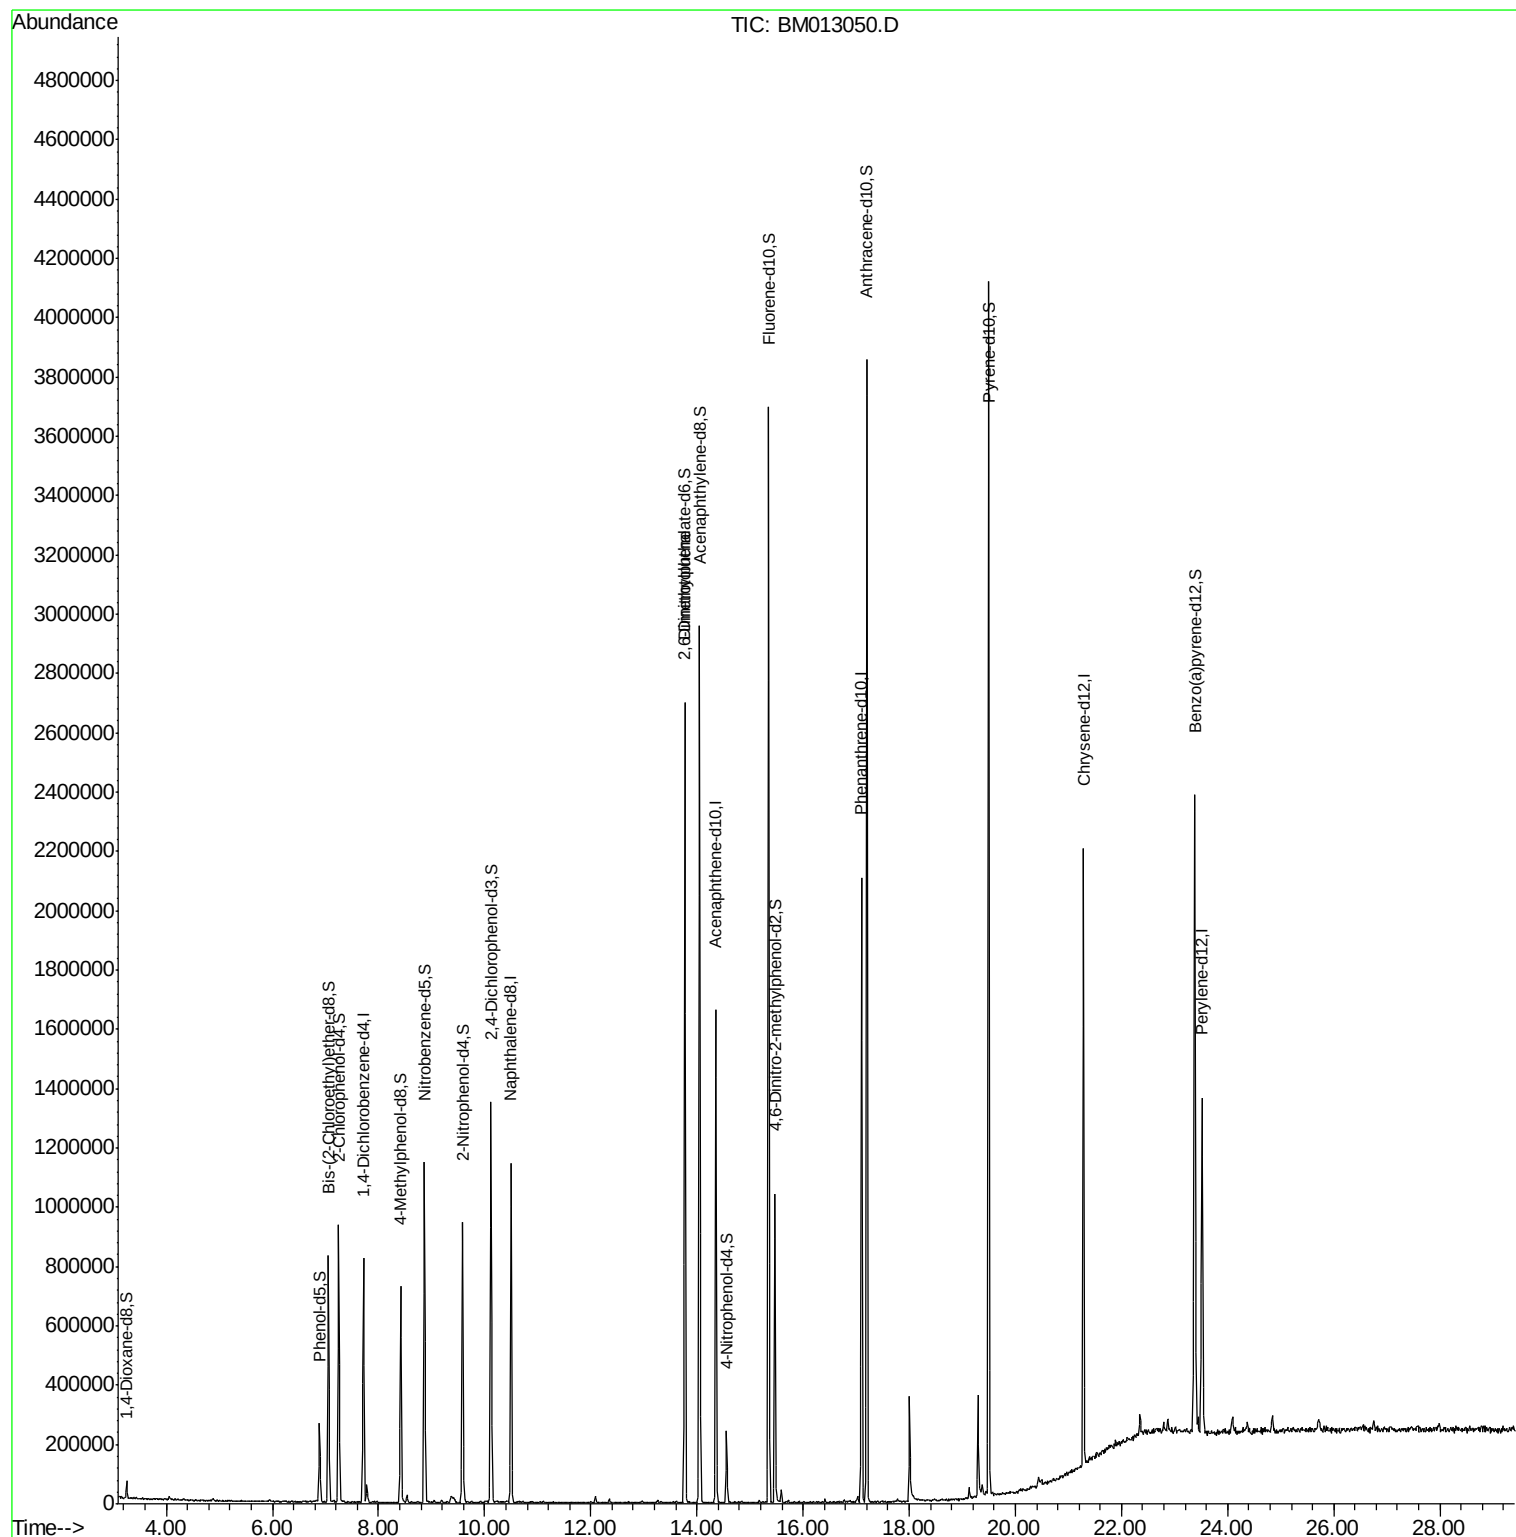

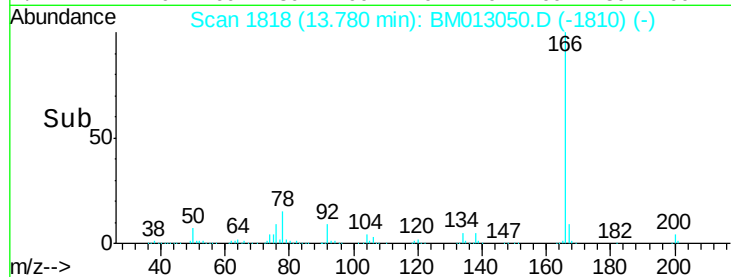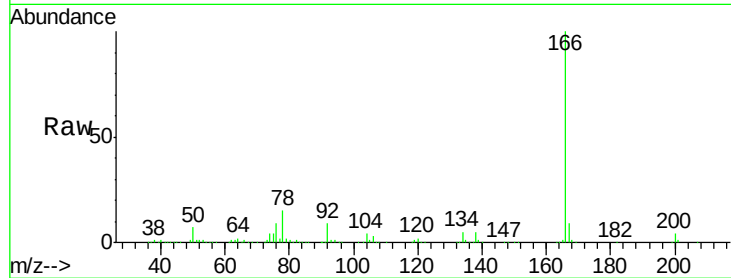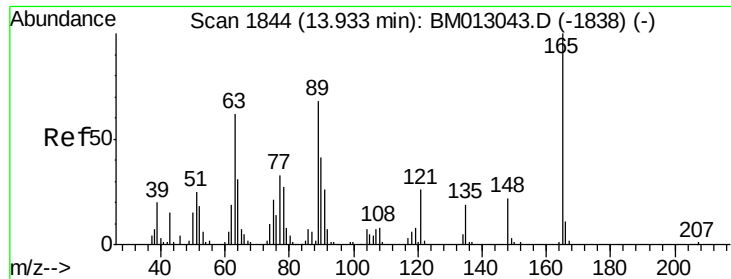

#45
 2,6-Dinitrotoluene
 Concen: 1.56 ng/ul
 RT: 13.78 min Scan# 1818
 Delta R.T. -0.15 min
 Lab File: BM013050.D
 Acq: 20 Nov 2017 17:01

Instrument :
 BNA_M
 ClientSampleId :
 C0B95

Tot Ion	Ratio	Lower	Upper
165	100		
89	0.0	52.6	79.0#
121	23.0	14.6	22.0#

