

Data Path : Z:\HPCHEM1\BNA M\DATA\BM112017\
 Data File : BM013064.D
 Acq On : 21 Nov 2017 03:23
 Operator : SJ/JU
 Sample : I6514-10
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0B93

Manual Integrations
 APPROVED

Sohil
 11/21/2017 2:29:24 PM

Quant Time: Nov 21 04:12:57 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM111617.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 21 01:43:17 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	233845	20.00	ng/ul	0.00
18) Naphthalene-d8	10.49	136	1044232	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.35	164	661078	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.10	188	1503391	20.00	ng/ul	0.00
75) Chrysene-d12	21.28	240	1386626	20.00	ng/ul	0.00
83) Perylene-d12	23.51	264	1104798	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.25	96	28328m	5.61	ng/uL	0.00
5) Phenol-d5	6.88	99	121654	6.01	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.05	67	189862	16.52	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	242378	14.97	ng/ul	0.00
13) 4-Methylphenol-d8	8.42	113	195136	11.76	ng/ul	0.00
19) Nitrobenzene-d5	8.86	128	135101	18.15	ng/ul	0.00
22) 2-Nitrophenol-d4	9.58	143	152568	21.55	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.12	165	284346	15.82	ng/ul	0.00
29) 4-Chloroaniline-d4	10.63	131	1101	0.06	ng/ul	0.00
43) Dimethylphthalate-d6	13.77	166	967805	16.69	ng/ul	0.00
46) Acenaphthylene-d8	14.05	160	1146892	15.52	ng/ul	0.00
51) 4-Nitrophenol-d4	14.56	143	53389	6.07	ng/ul	0.00
57) Fluorene-d10	15.35	176	813278	16.50	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.46	200	135221	20.74	ng/ul	0.00
70) Anthracene-d10	17.20	188	1228319	15.96	ng/ul	0.00
76) Pyrene-d10	19.49	212	1299199	18.34	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.37	264	945982	16.89	ng/ul	0.00

Target Compounds				Ovalue	
6) Phenol	6.91	94	50372	2.520	ng/ul# 86

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM112017\
Data File : BM013064.D
Acq On : 21 Nov 2017 03:23
Operator : SJ/JU
Sample : I6514-10
Misc :
ALS Vial : 22 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
C0B93

Manual Integrations
APPROVED

Sohil
11/21/2017 2:29:24 PM

Quant Time: Nov 21 04:12:57 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM111617.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 21 01:43:17 2017
Response via : Initial Calibration

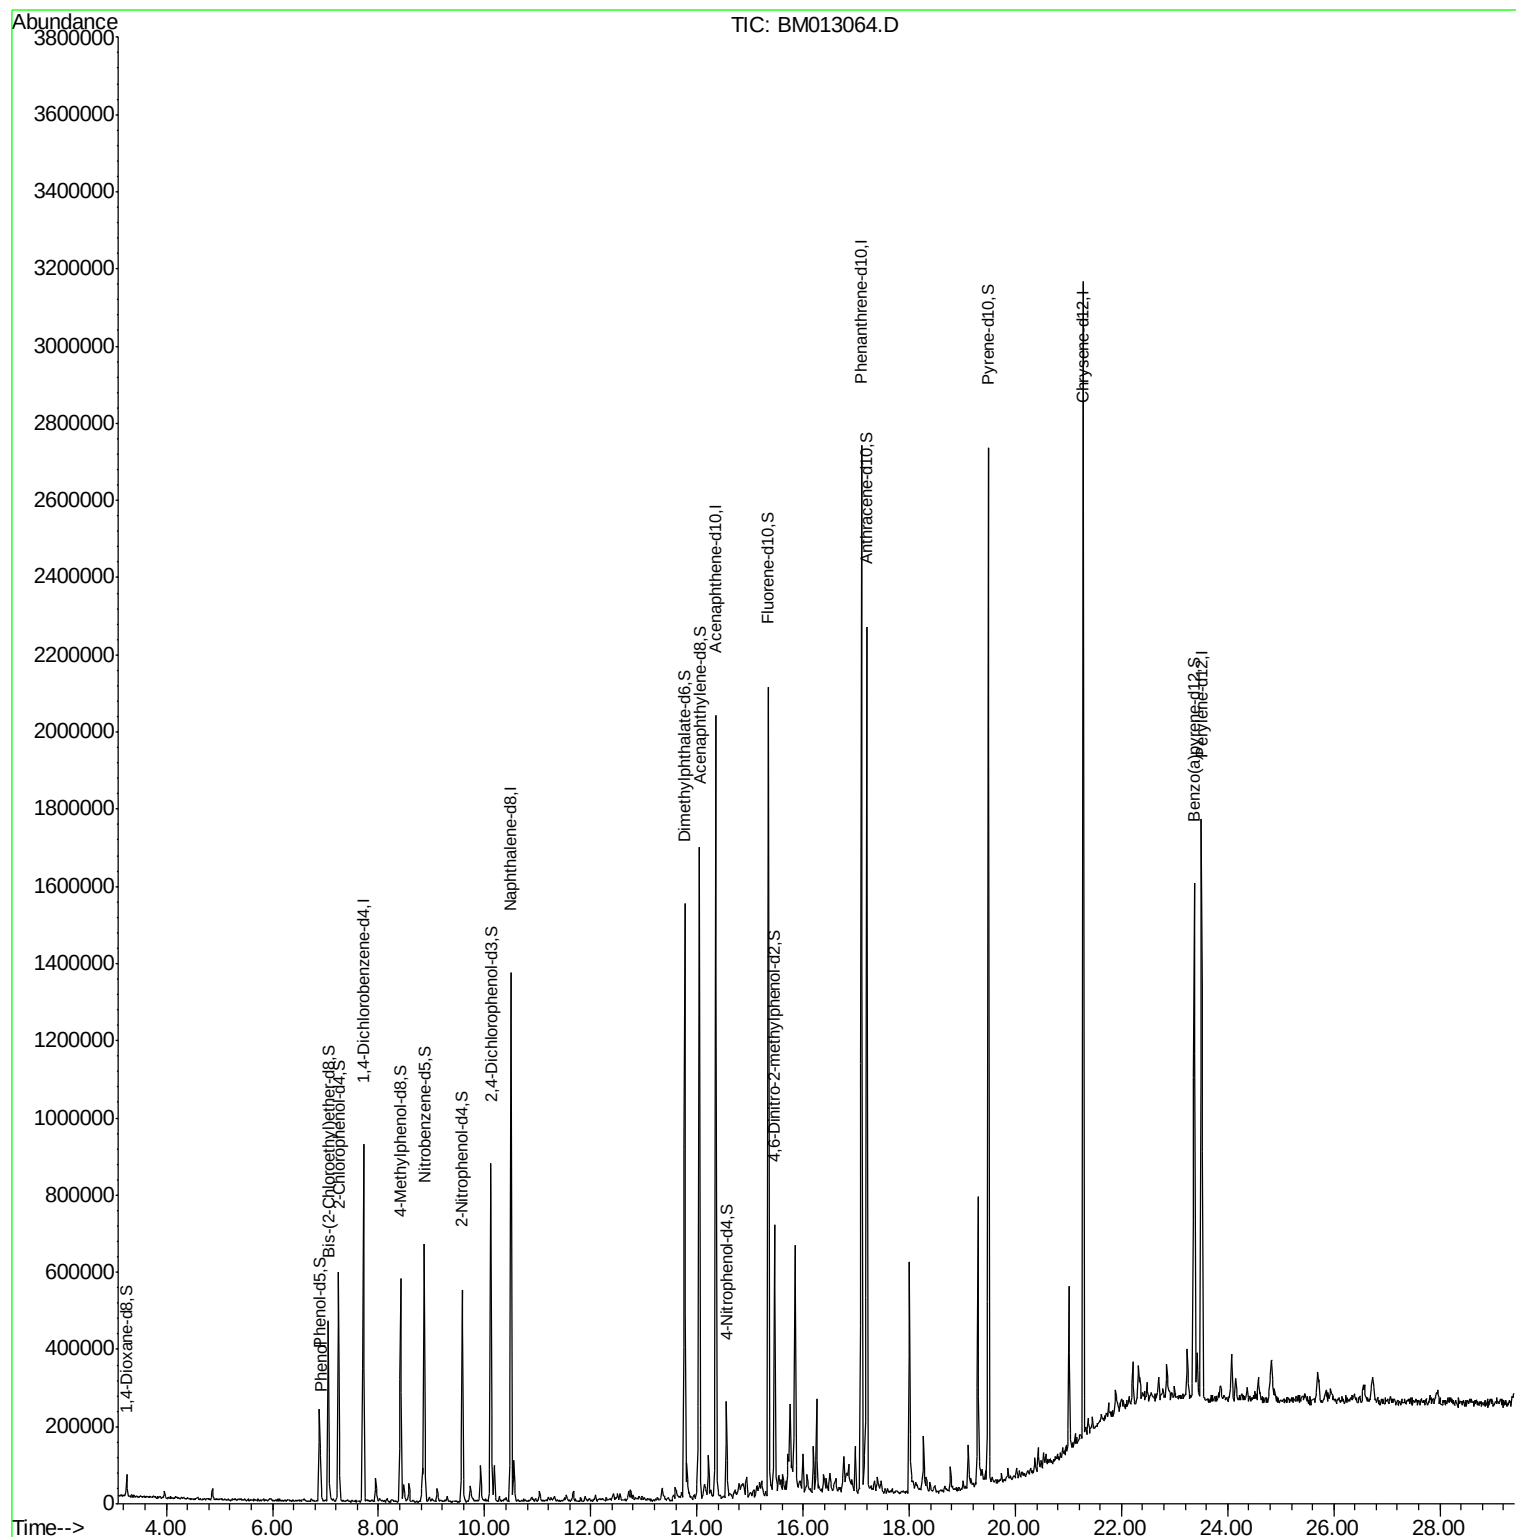

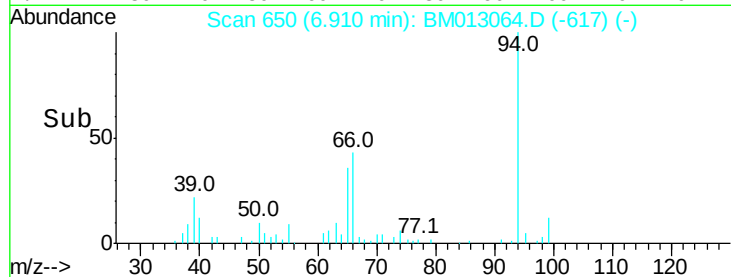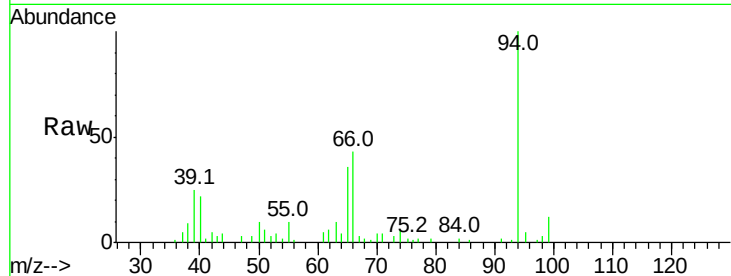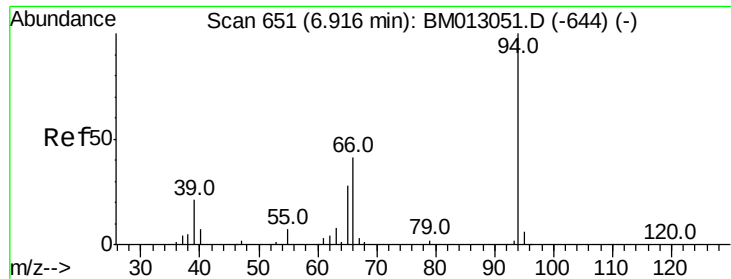

#6

Phenol

Concen: 2.520 ng/ul

RT: 6.91 min Scan# 650

Delta R.T. -0.01 min

Lab File: BM013064.D

Acq: 21 Nov 2017 03:23

Tot Ion:	94	Resp:	50372
Ion Ratio	Lower	Upper	
94	100		
65	36.4	28.2	42.4
66	43.2	47.2	70.8#

Instrument :

BNA_M

ClientSampleId :

C0B93

Manual Integrations
APPROVED

Sohil
11/21/2017 2:29:24 PM

