


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM112020\
Data File : BM027870.D
Acq On : 21 Nov 2020 01:51
Operator : JU/CG
Sample : SP5357
Misc : SURROGATE SOLUTION
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SP5357

Manual Integrations
APPROVED

mohammad
11/24/2020 8:58:06 AM

Quant Time: Nov 21 03:26:25 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM112020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 21 02:40:49 2020
Response via : Initial Calibration

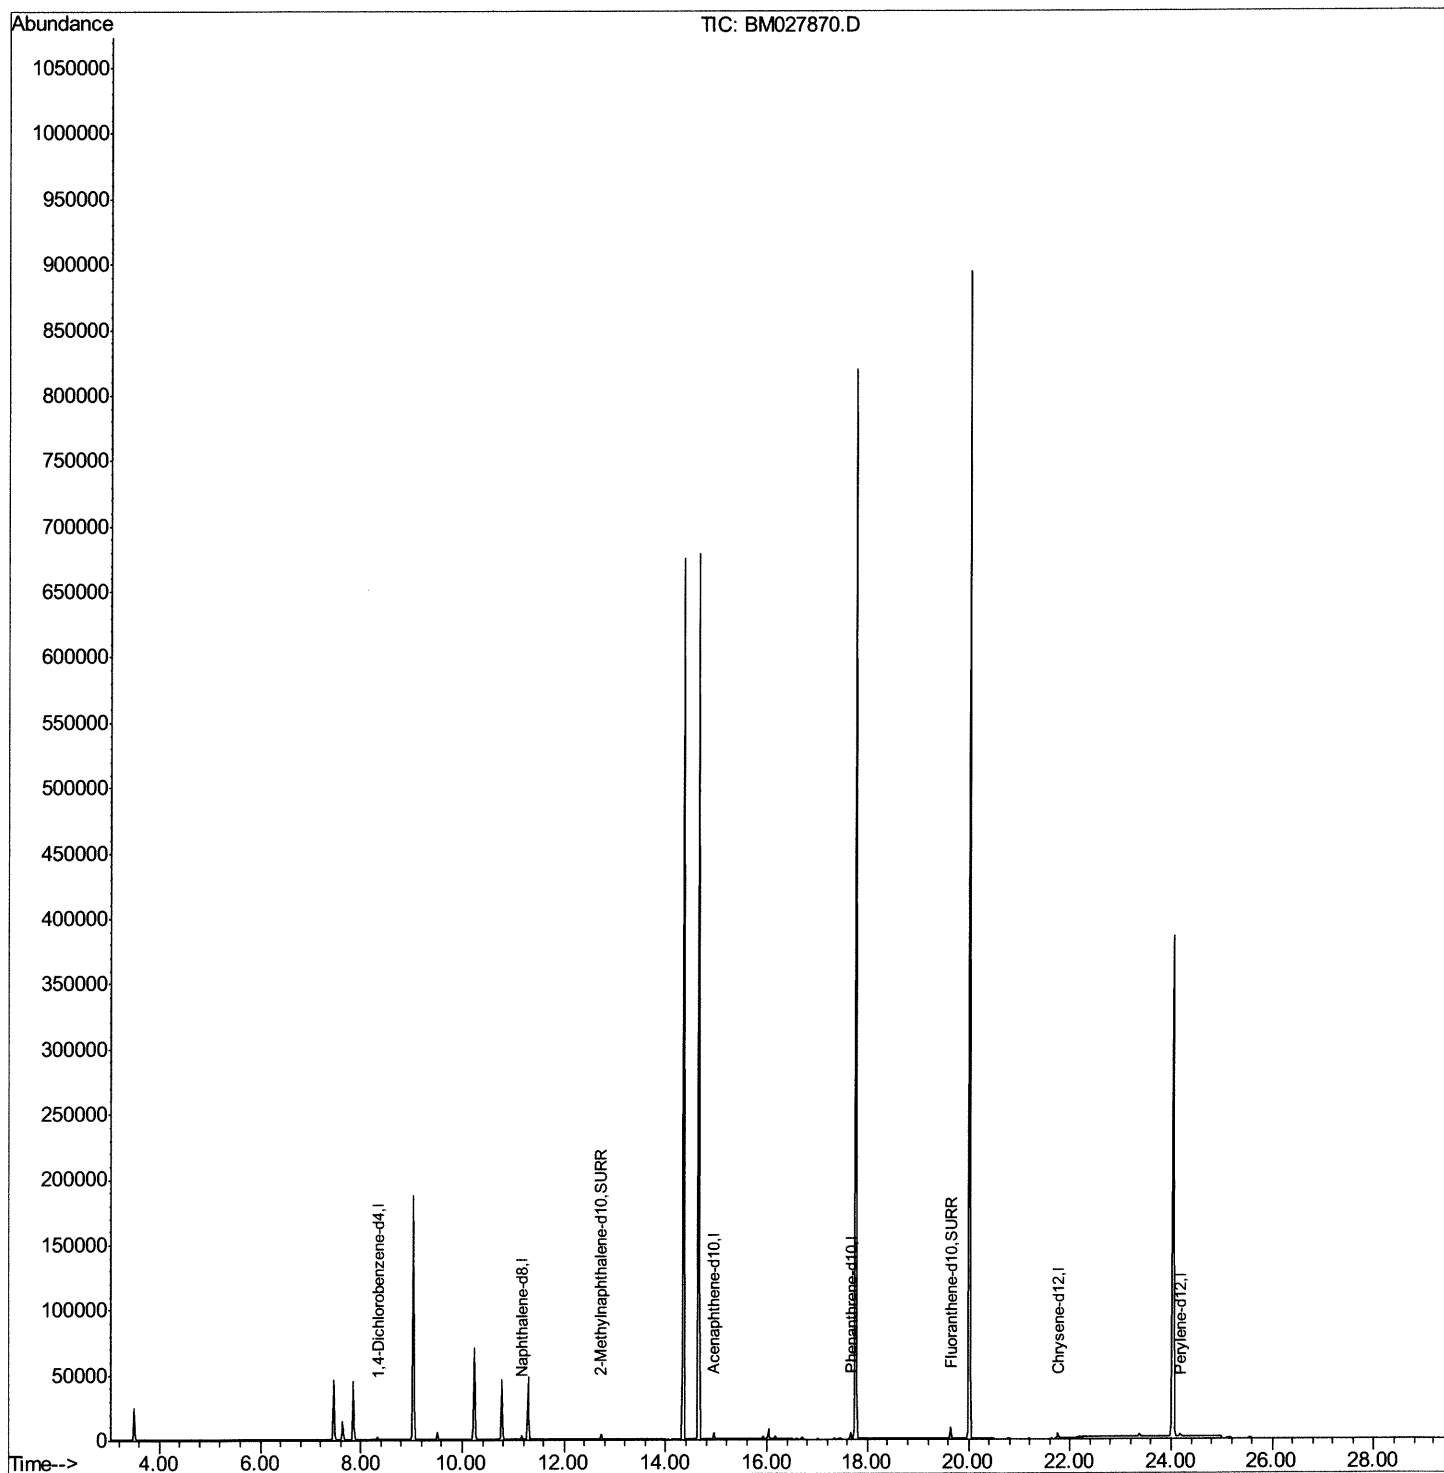

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM112020\
 Data File : BM027870.D
 Acq On : 21 Nov 2020 01:51
 Operator : JU/CG
 Sample : SP5357
 Misc : SURROGATE SOLUTION
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 SP5357

Manual Integrations
APPROVED

mohammad
 11/24/2020 8:58:06 AM

Quant Time: Nov 21 03:23:52 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM112020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 21 02:40:49 2020
 Response via : Initial Calibration

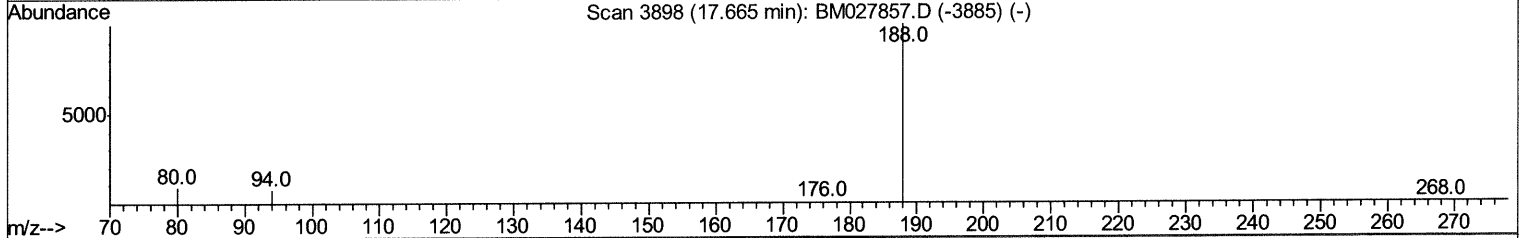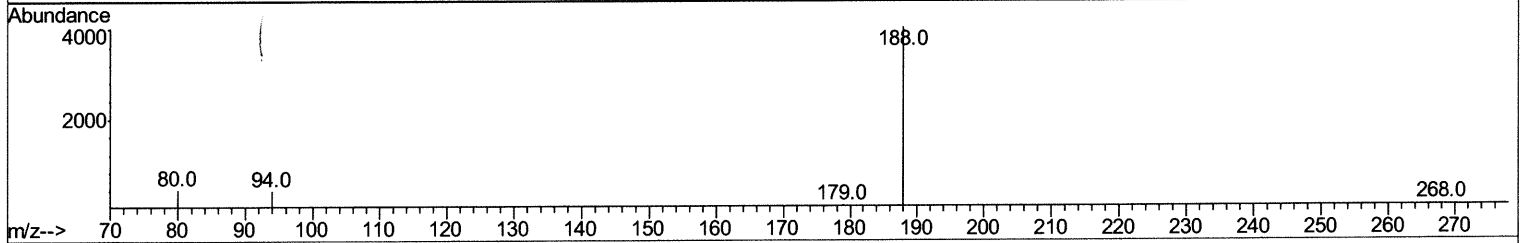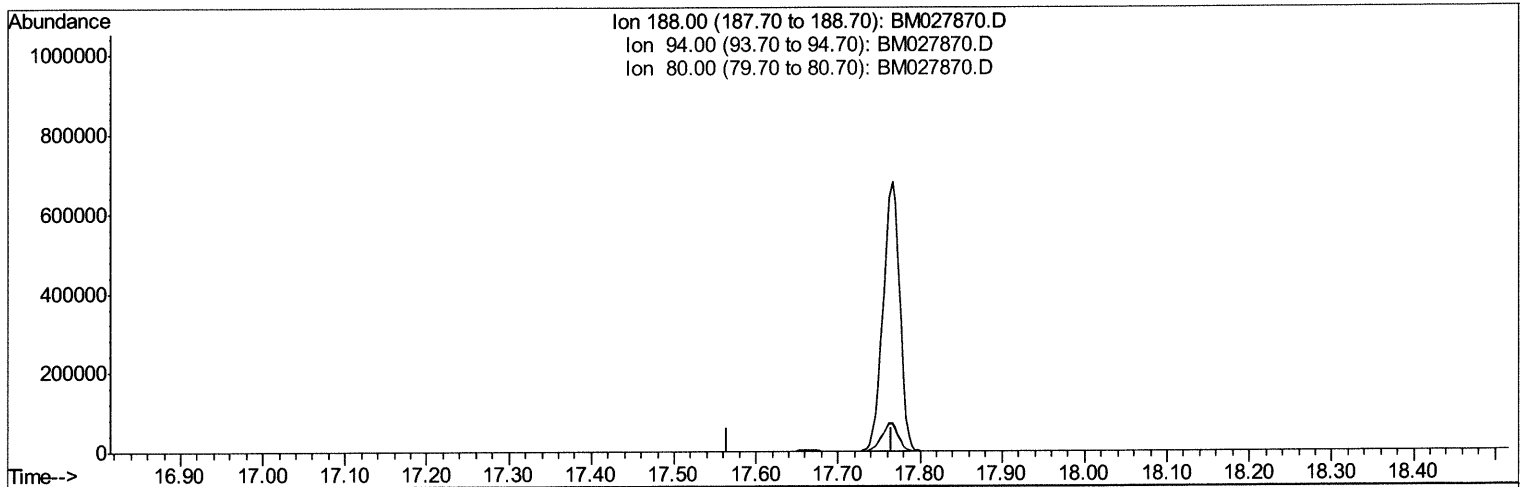

TIC: BM027870.D

(10) Phenanthrene-d10 (I)
 17.666min (-17.666) 0.00ng/ul
 response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	9.30	0.00#
80.00	10.20	0.00#
0.00	0.00	0.00


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM112020\
Data File : BM027870.D
Acq On : 21 Nov 2020 01:51
Operator : JU/CG
Sample : SP5357
Misc : SURROGATE SOLUTION
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SP5357

Manual Integrations
APPROVED

mohammad
11/24/2020 8:58:06 AM

Quant Time: Nov 21 03:23:52 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM112020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 21 02:40:49 2020
Response via : Initial Calibration

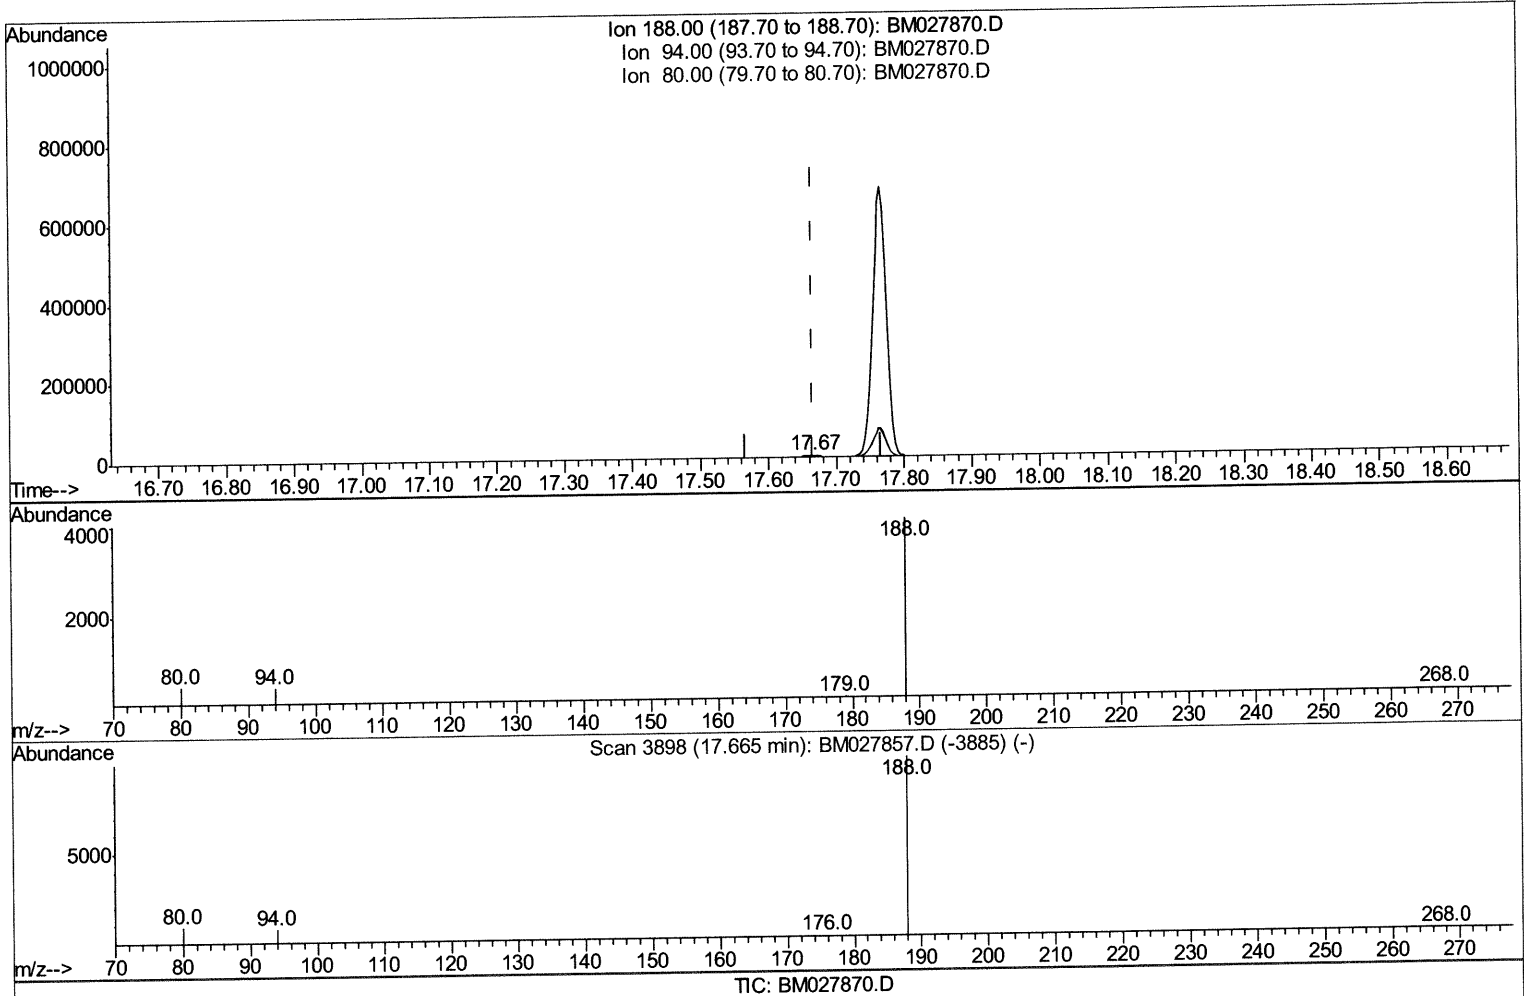

(10) Phenanthrene-d10 (I)

17.665min (-0.000) 0.40ng/ul m 11/27/20 50

response 5553

Ion	Exp%	Act%
188.00	100	100
94.00	9.30	9.74
80.00	10.20	10.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM112020\
 Data File : BM027870.D
 Acq On : 21 Nov 2020 01:51
 Operator : JU/CG
 Sample : SP5357
 Misc : SURROGATE SOLUTION
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SP5357

Manual Integrations
 APPROVED

mohammad
 11/24/2020 8:58:06 AM

Quant Time: Nov 21 03:26:25 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM112020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 21 02:40:49 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.33	152	989	0.40	ng/ul	0.00
2) Naphthalene-d8	11.17	136	4039	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.95	164	2898	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.67	188	5553m >	0.40	ng/ul >	0.00
16) Chrysene-d12	21.76	240	3934	0.40	ng/ul	0.00
20) Perylene-d12	24.18	264	2731	0.40	ng/ul	0.00

11/27/20 JU

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.73	152	4649	0.68	ng/ul	0.00
14) Fluoranthene-d10	19.65	212	9442	0.64	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed