


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM112020\
Data File : BM027876.D
Acq On : 21 Nov 2020 11:56
Operator : JU/CG
Sample : PB133084BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK84

Manual Integrations
APPROVED

mohammad
11/24/2020 8:58:31 AM

Quant Time: Nov 21 12:36:11 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM112020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 20 17:20:22 2020
Response via : Initial Calibration

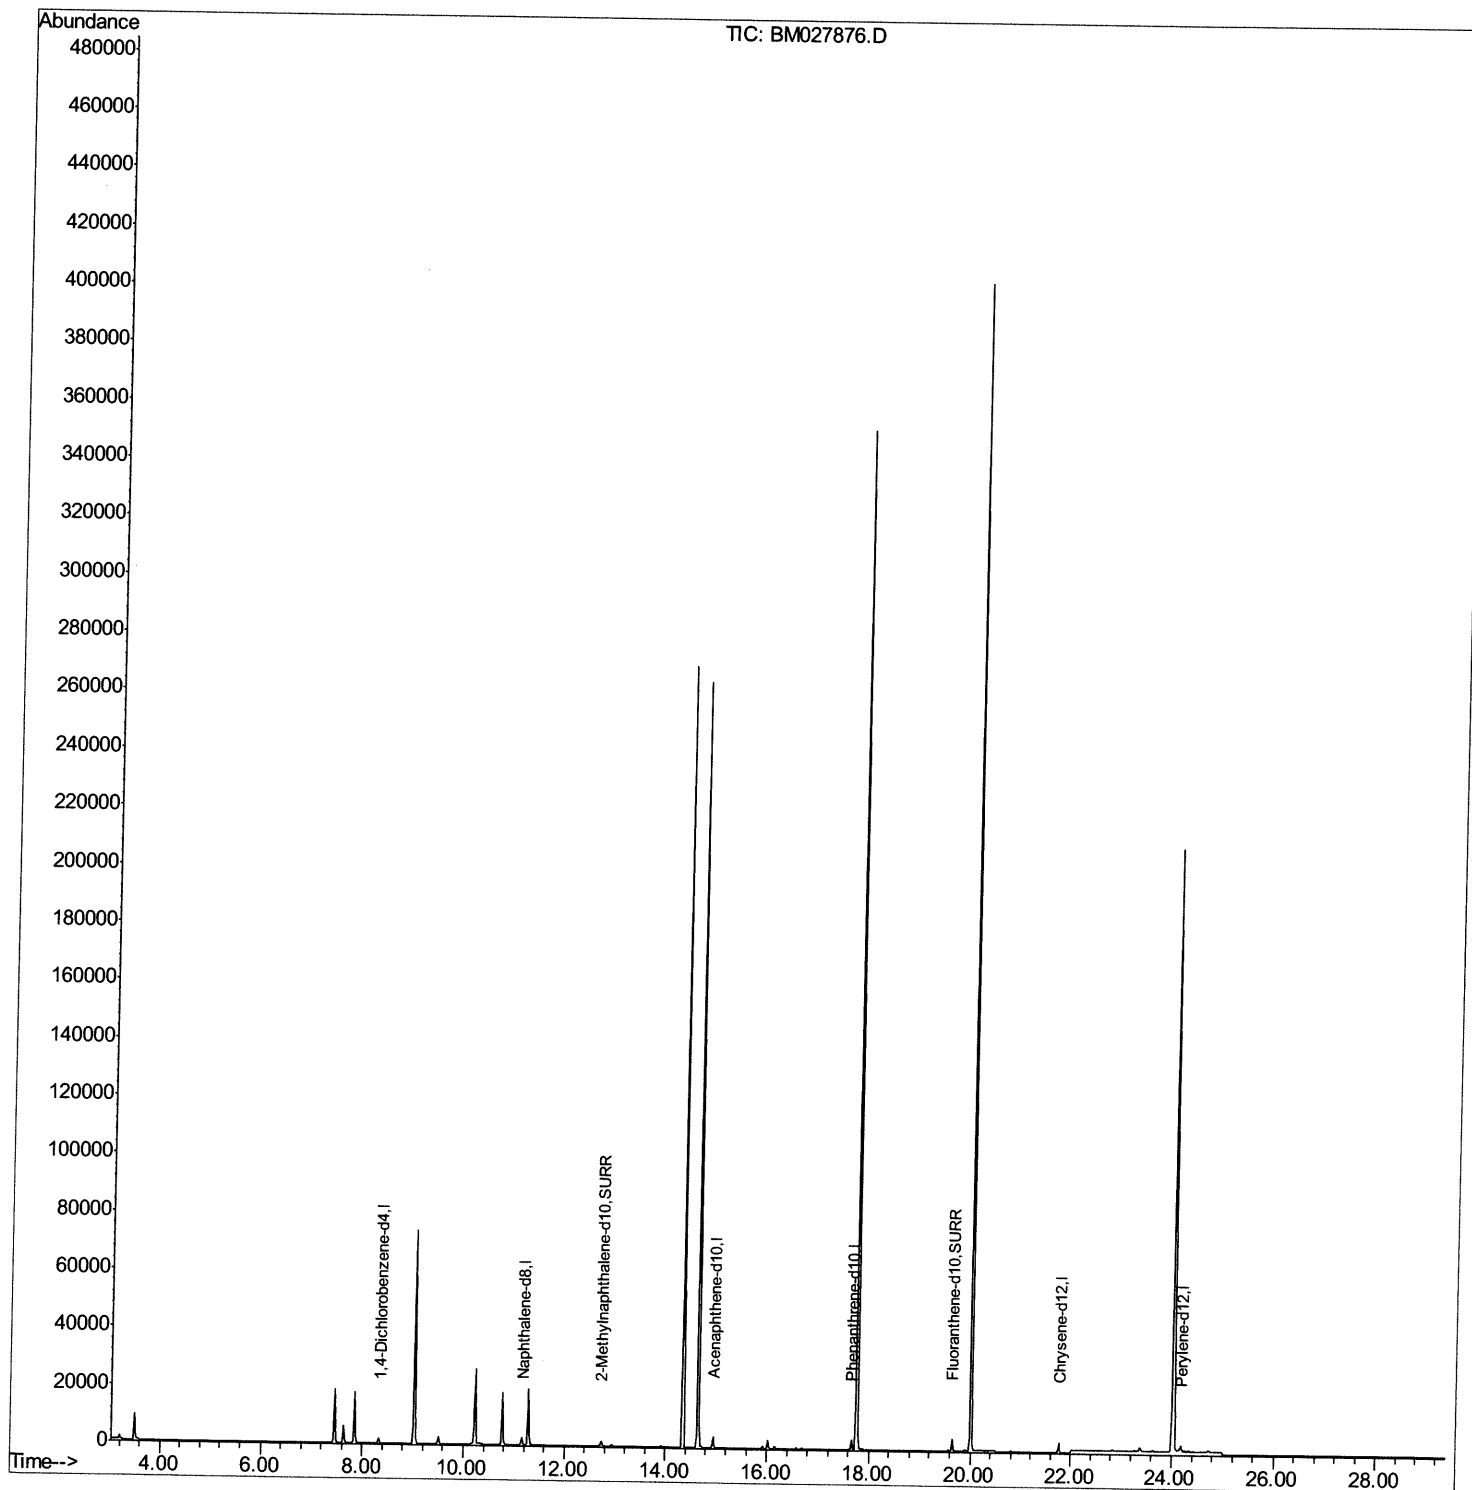

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM112020\
 Data File : BM027876.D
 Acq On : 21 Nov 2020 11:56
 Operator : JU/CG
 Sample : PB133084BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 SBLK84

Manual Integrations
APPROVED

mohammad
 11/24/2020 8:58:31 AM

Quant Time: Nov 21 12:34:33 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM112020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 20 17:20:22 2020
 Response via : Initial Calibration

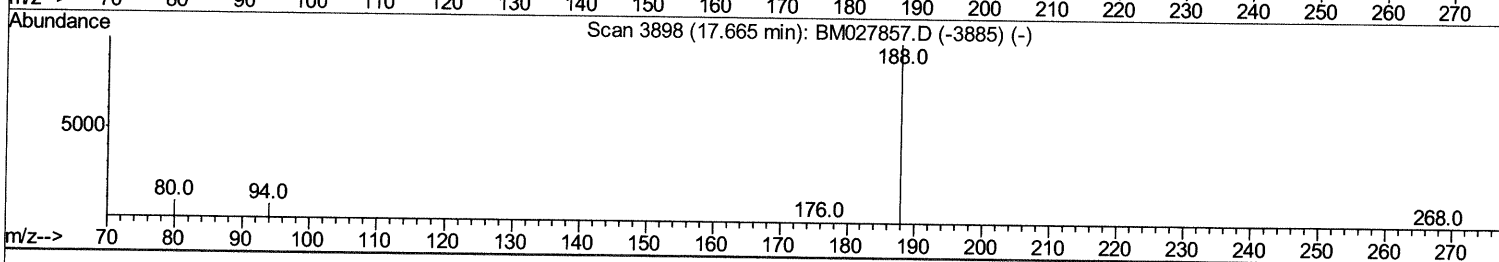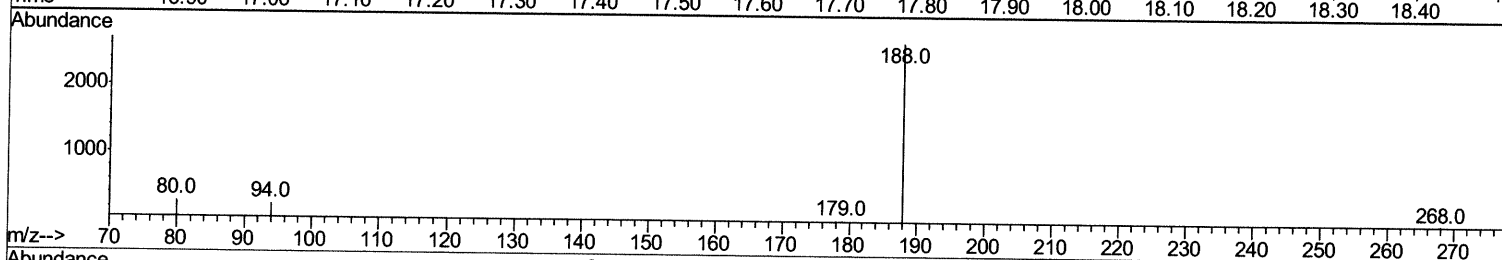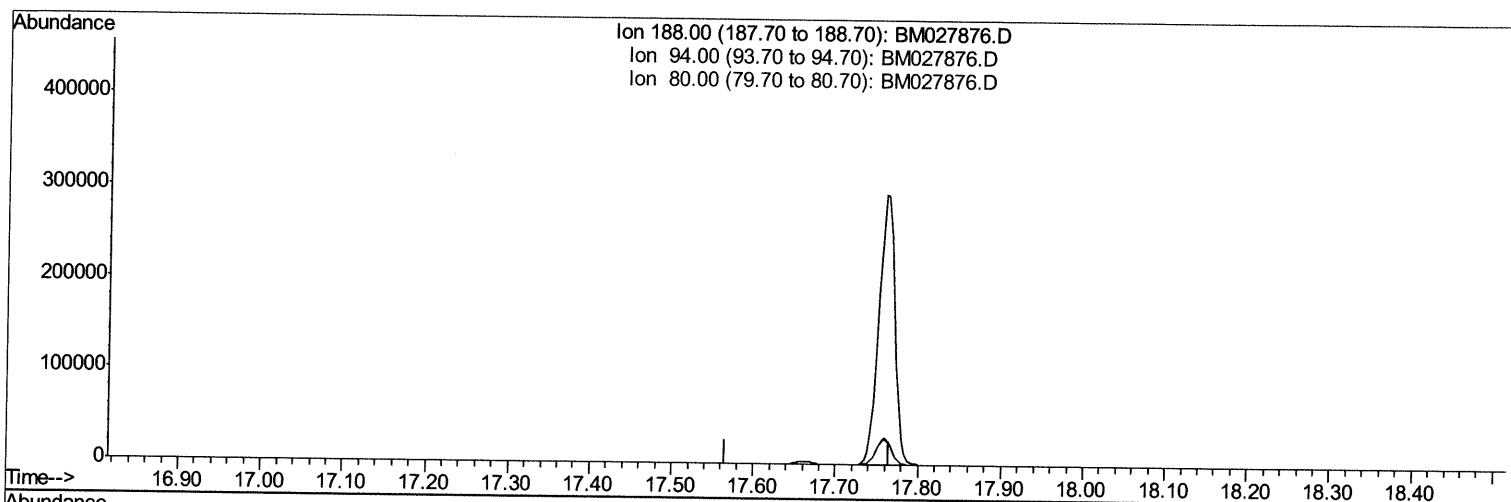

TIC: BM027876.D

(10) Phenanthrene-d10 (I)

17.666min (-17.666) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	9.30	0.00#
80.00	10.20	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM112020\
 Data File : BM027876.D
 Acq On : 21 Nov 2020 11:56
 Operator : JU/CG
 Sample : PB133084BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK84

Manual Integrations
 APPROVED

mohammad
 11/24/2020 8:58:31 AM

Ouant Time: Nov 21 12:34:33 2020
 Ouant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM112020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 20 17:20:22 2020
 Response via : Initial Calibration

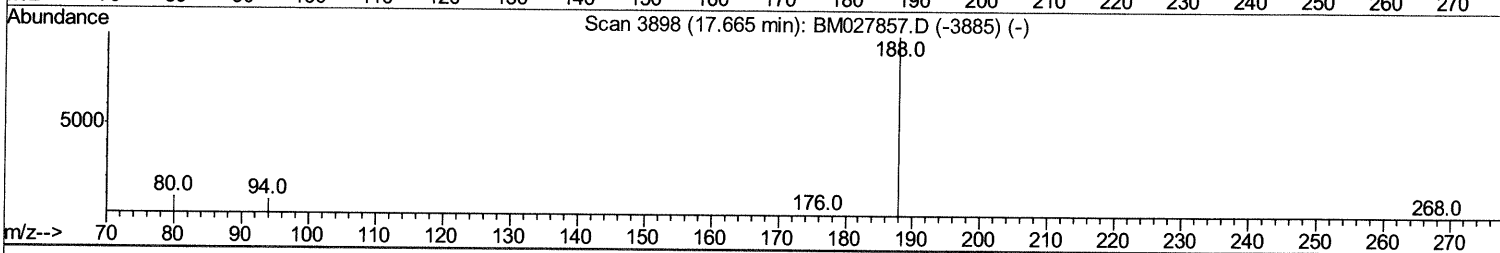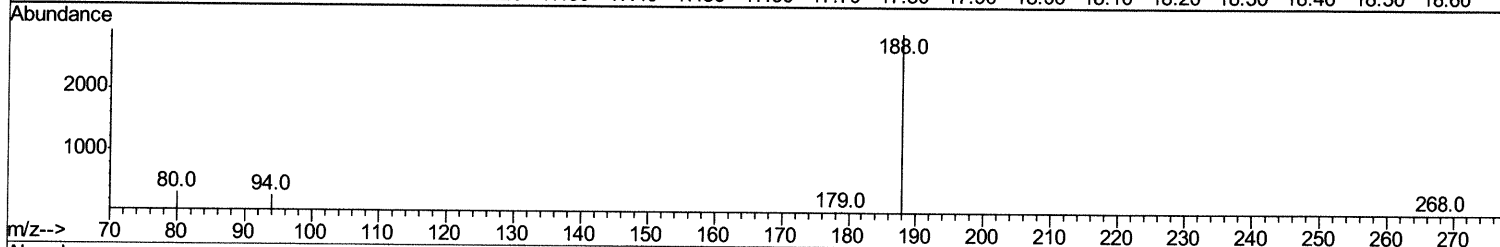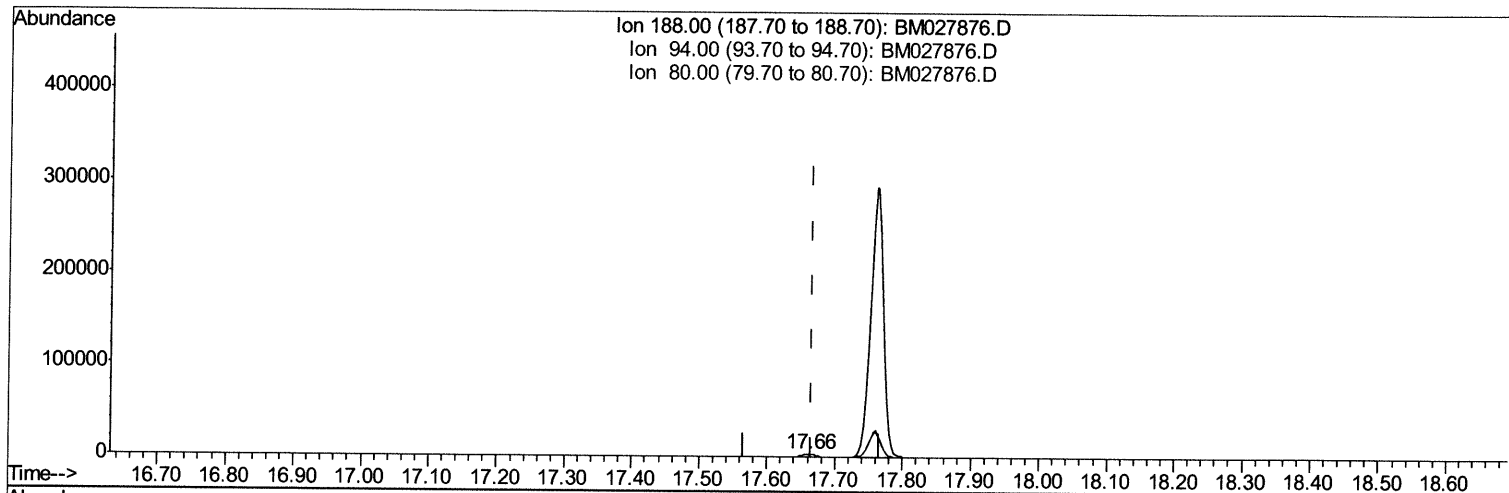

TIC: BM027876.D

(10) Phenanthrene-d10 (I)

17.662min (-0.004) 0.40ng/ul m 11/27/20 JU

response 4093

Ion	Exp%	Act%
188.00	100	100
94.00	9.30	9.68
80.00	10.20	10.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM112020\
 Data File : BM027876.D
 Acq On : 21 Nov 2020 11:56
 Operator : JU/CG
 Sample : PB133084BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK84

Manual Integrations
 APPROVED

mohammad
 11/24/2020 8:58:31 AM

Quant Time: Nov 21 12:36:11 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM112020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 20 17:20:22 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.33	152	691	0.40	ng/ul	0.00
2) Naphthalene-d8	11.17	136	2830	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.95	164	1945	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.66	188	4093m >	0.40	ng/ul >	0.00
16) Chrysene-d12	21.76	240	3212	0.40	ng/ul	0.00
20) Perylene-d12	24.18	264	2468	0.40	ng/ul	0.00

11/27/20 JU

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.73	152	1980	0.41	ng/ul	0.00
14) Fluoranthene-d10	19.65	212	4476	0.41	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed