


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112020\
Data File : BM027878.D
Acq On : 21 Nov 2020 13:09
Operator : JU/CG
Sample : PB133156BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK56

Manual Integrations
APPROVED

mohammad
11/24/2020 8:58:33 AM

Quant Time: Nov 23 03:19:22 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM112020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 20 17:20:22 2020
Response via : Initial Calibration

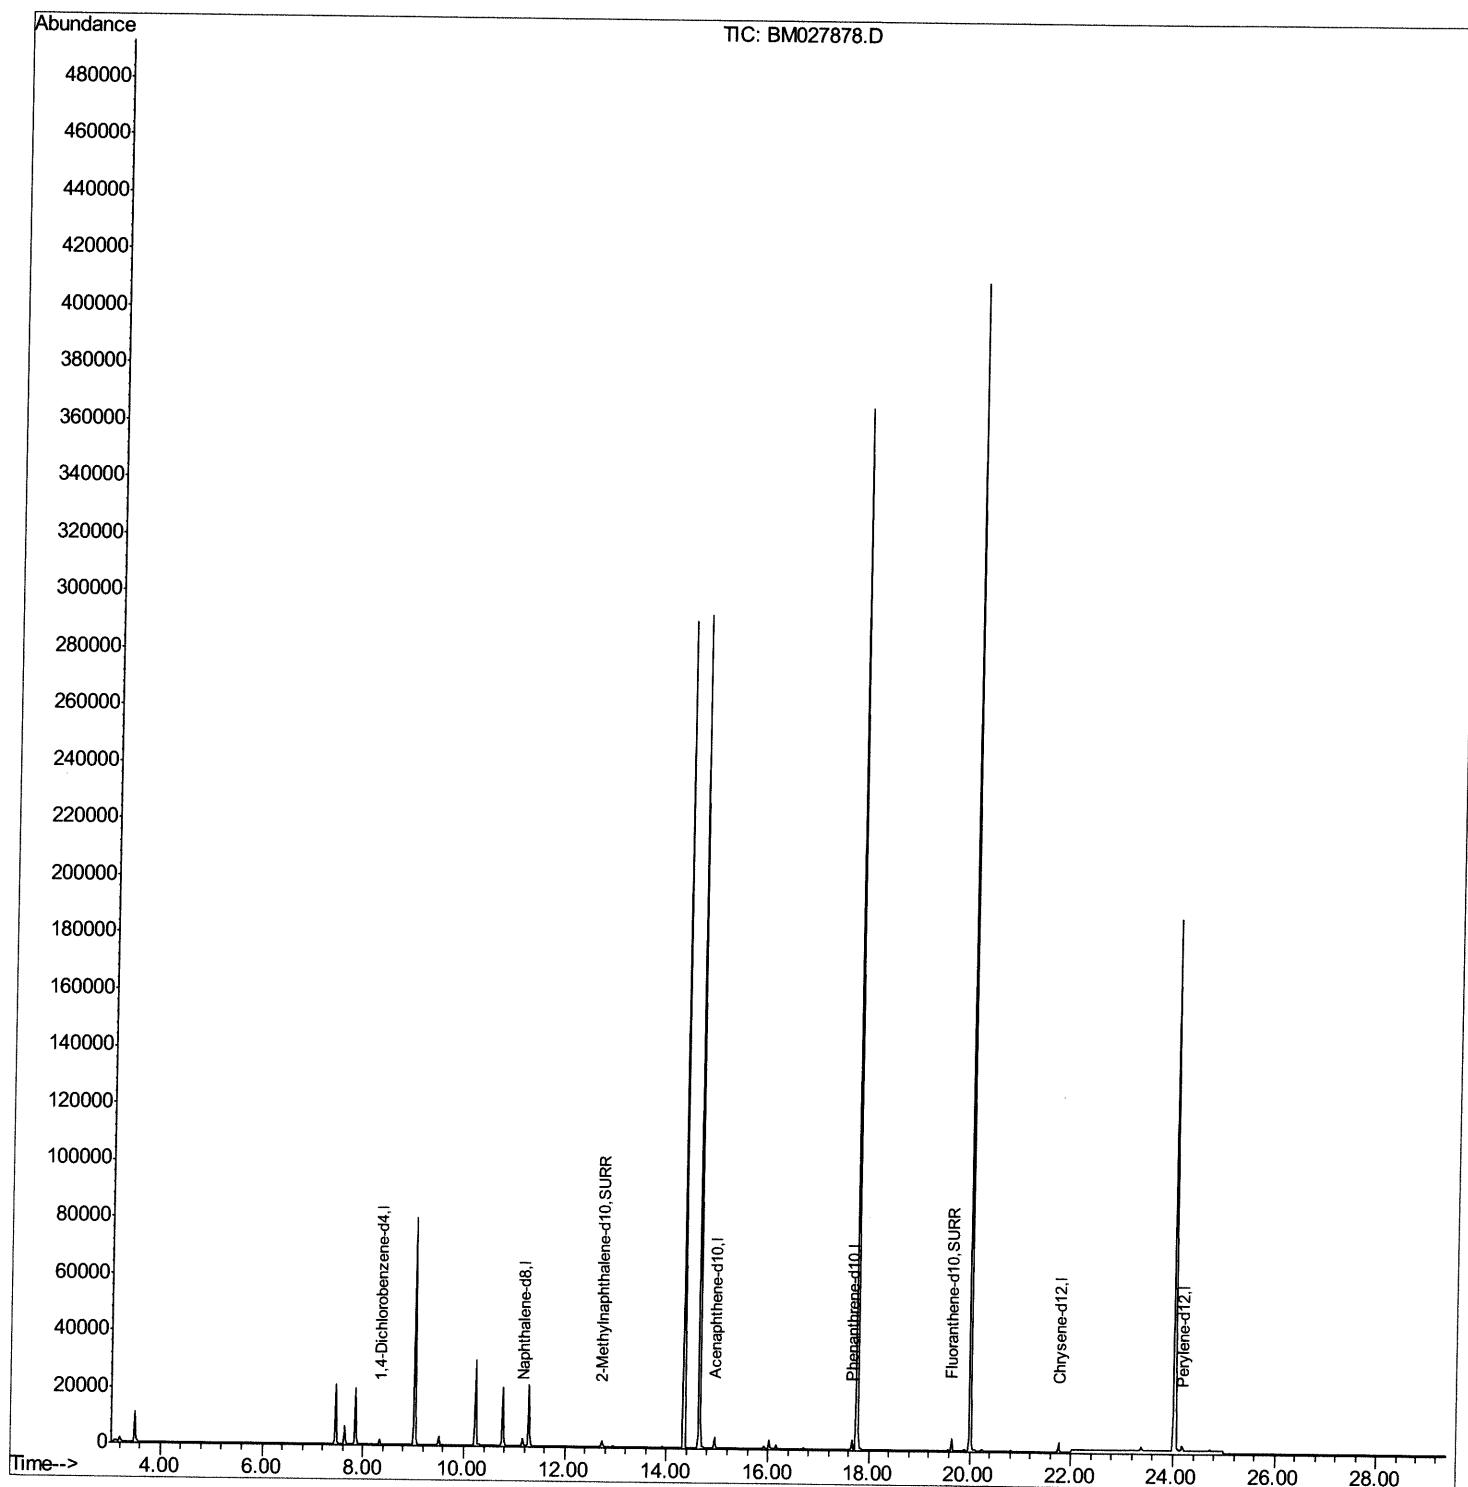

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112020\
 Data File : BM027878.D
 Acq On : 21 Nov 2020 13:09
 Operator : JU/CG
 Sample : PB133156BL
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK56

Manual Integrations
 APPROVED

mohammad
 11/24/2020 8:58:33 AM

Quant Time: Nov 23 02:59:57 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM112020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 20 17:20:22 2020
 Response via : Initial Calibration

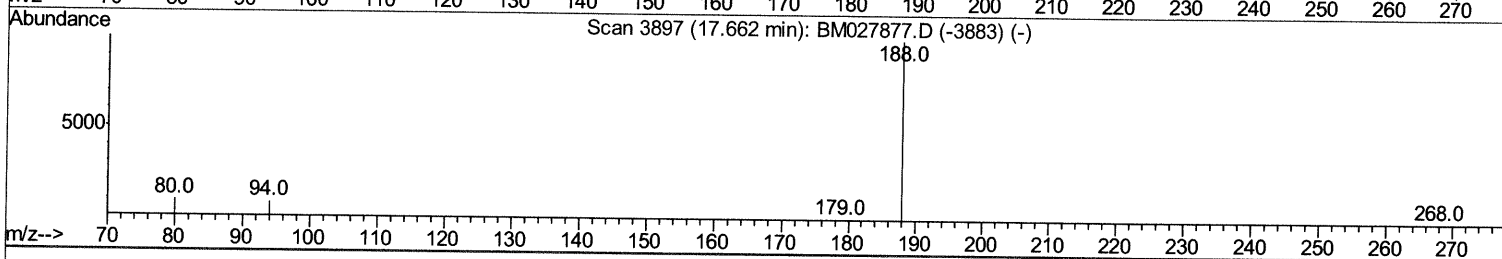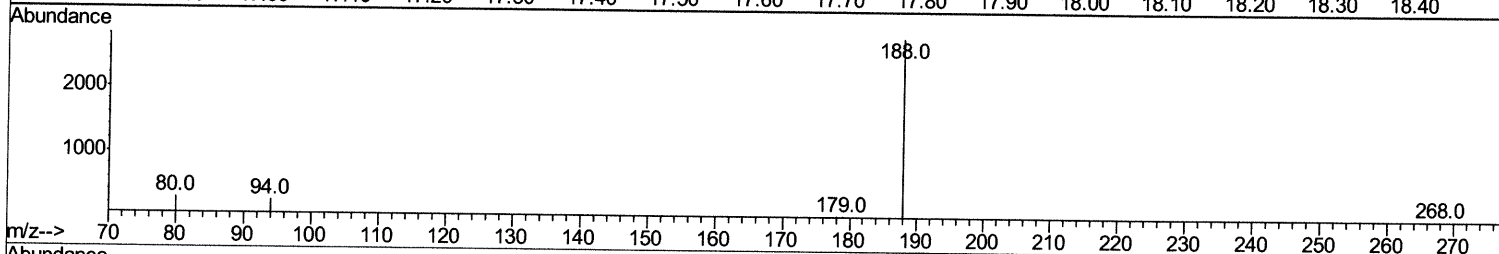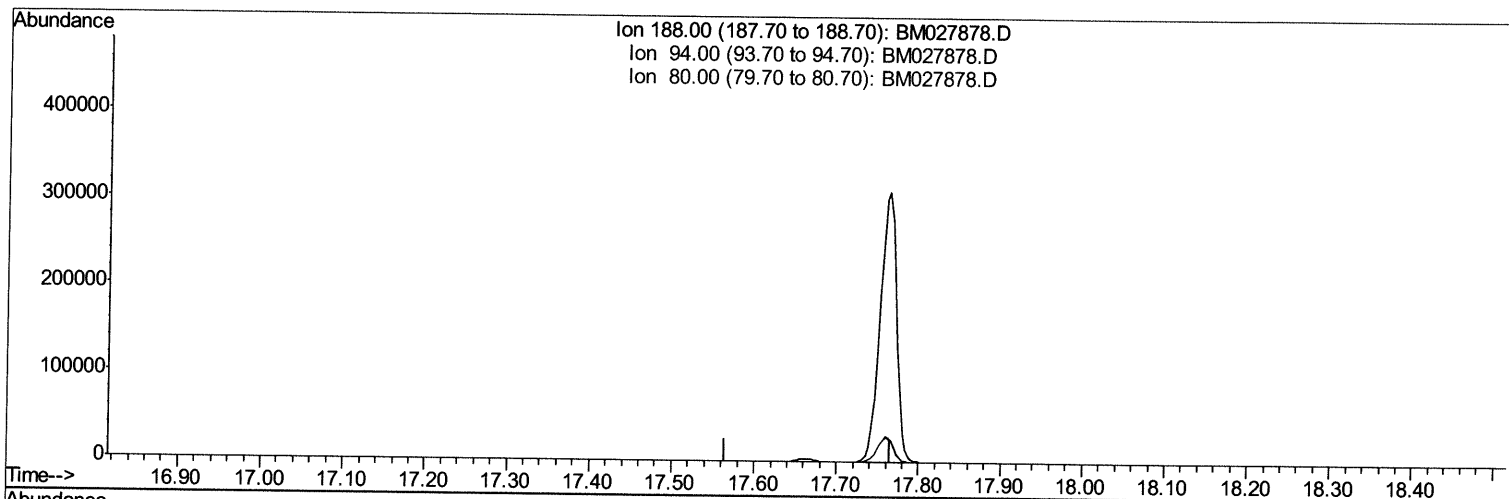

TIC: BM027878.D

(10) Phenanthrene-d10 (I)

17.666min (-17.666) 0.00ng/ui

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	9.30	0.00#
80.00	10.20	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112020\
Data File : BM027878.D
Acq On : 21 Nov 2020 13:09
Operator : JU/CG
Sample : PB133156BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK56

Manual Integrations
APPROVED

mohammad
11/24/2020 8:58:33 AM

Quant Time: Nov 23 03:07:30 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM112020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 20 17:20:22 2020
Response via : Initial Calibration

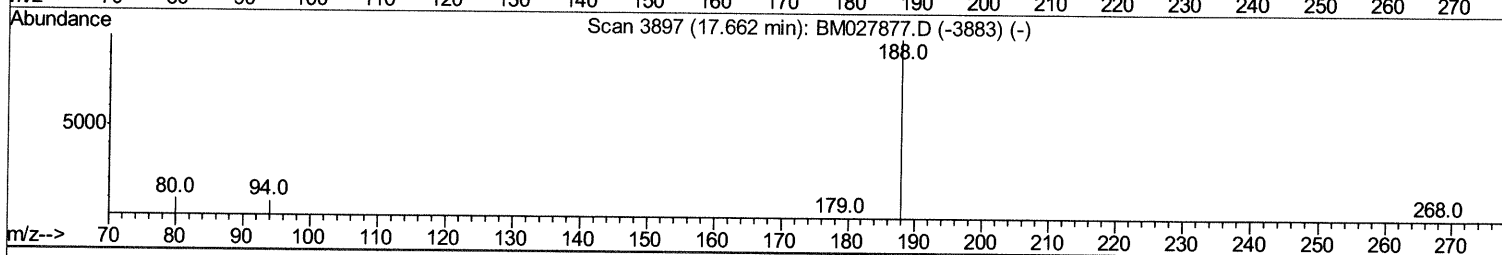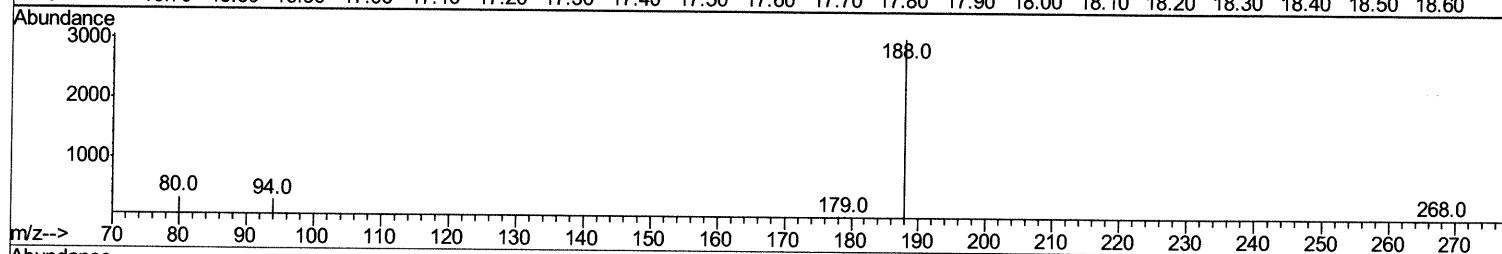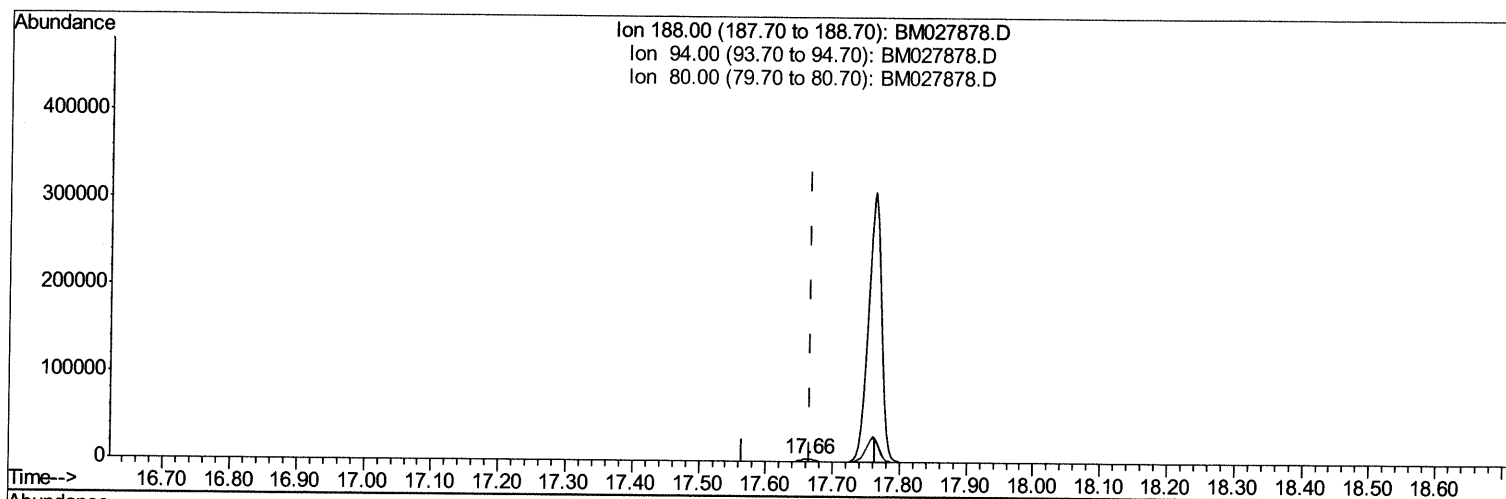

TIC: BM027878.D

(10) Phenanthrene-d10 (I)

17.662min (-0.003) 0.40ng/ul m 11/27/20 JU

response 4214

Ion	Exp%	Act%
188.00	100	100
94.00	9.30	9.41
80.00	10.20	10.47
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112020\
 Data File : BM027878.D
 Acq On : 21 Nov 2020 13:09
 Operator : JU/CG
 Sample : PB133156BL
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK56

Manual Integrations
 APPROVED

mohammad
 11/24/2020 8:58:33 AM

Quant Time: Nov 23 03:19:22 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM112020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 20 17:20:22 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.33	152	752	0.40	ng/ul	0.00
2) Naphthalene-d8	11.17	136	3075	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.95	164	2109	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.66	188	4214m>	0.40	ng/ul>	0.00
16) Chrysene-d12	21.76	240	3057	0.40	ng/ul	0.00
20) Perylene-d12	24.18	264	2279	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.73	152	2166	0.42	ng/ul	0.00
14) Fluoranthene-d10	19.65	212	4693	0.42	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed