


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112020\
Data File : BM027882.D
Acq On : 21 Nov 2020 15:34
Operator : JU/CG
Sample : L4854-06DL 5X
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD4DL

Manual Integrations
APPROVED

mohammad
11/24/2020 8:58:44 AM

Quant Time: Nov 23 04:01:46 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM112020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 23 02:58:43 2020
Response via : Initial Calibration

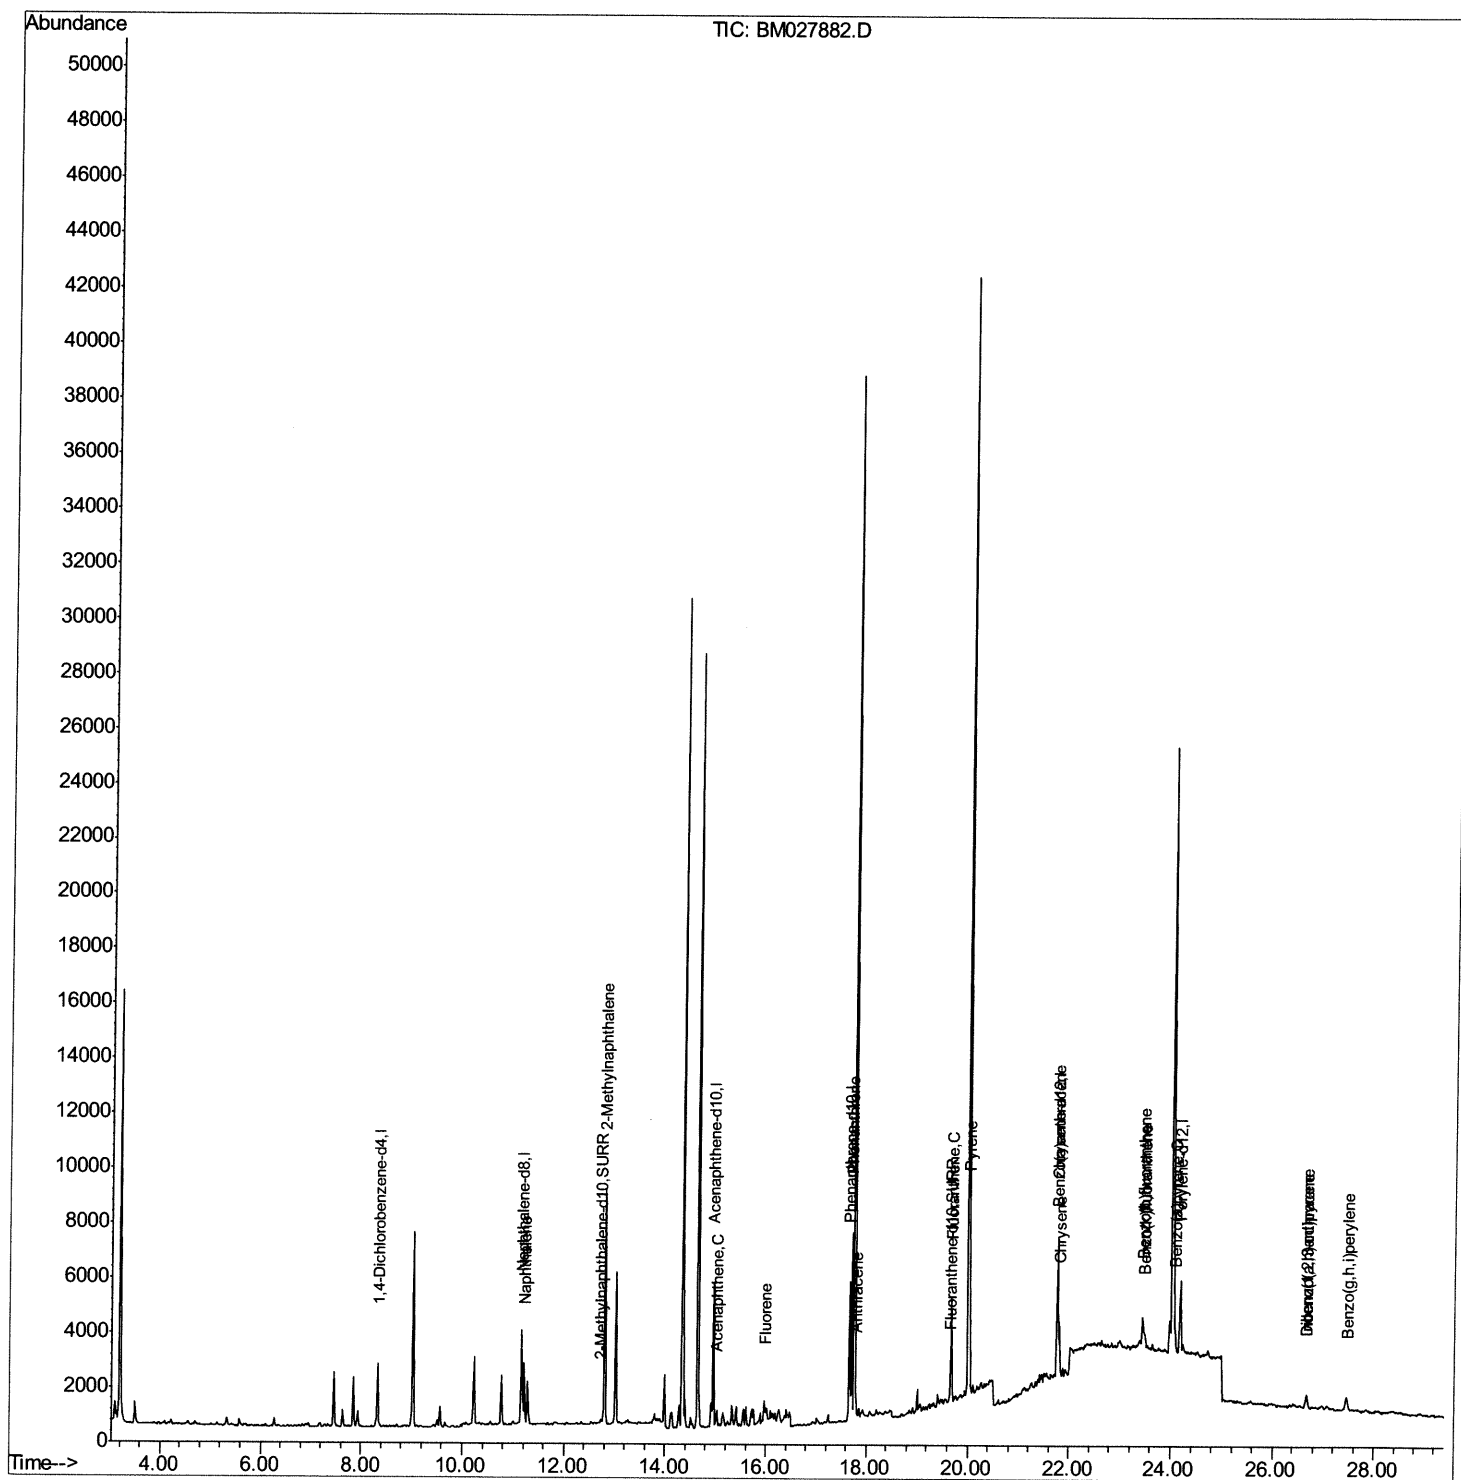

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112020\
 Data File : BM027882.D
 Acq On : 21 Nov 2020 15:34
 Operator : JU/CG
 Sample : L4854-06DL 5X
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AD4DL

Manual Integrations
 APPROVED

mohammad
 11/24/2020 8:58:44 AM

Quant Time: Nov 23 03:00:19 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM112020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 23 02:58:43 2020
 Response via : Initial Calibration

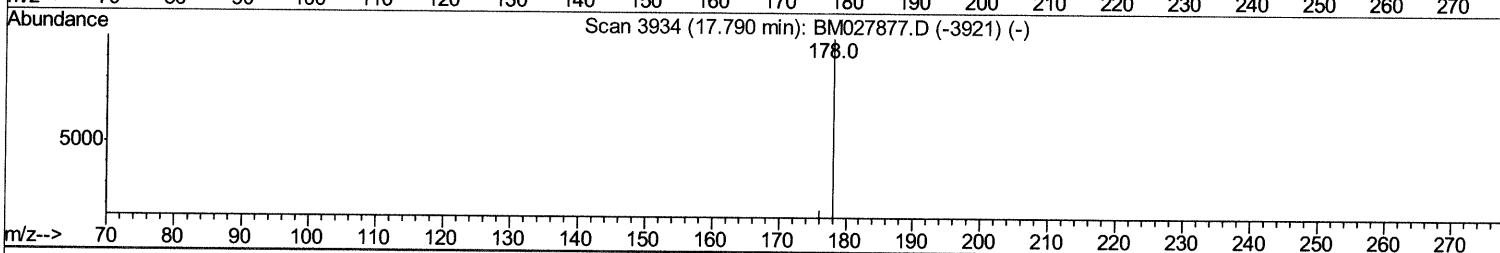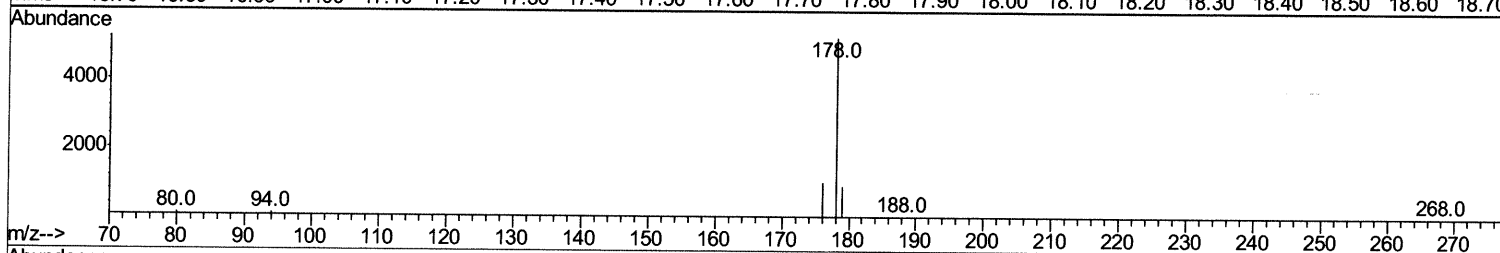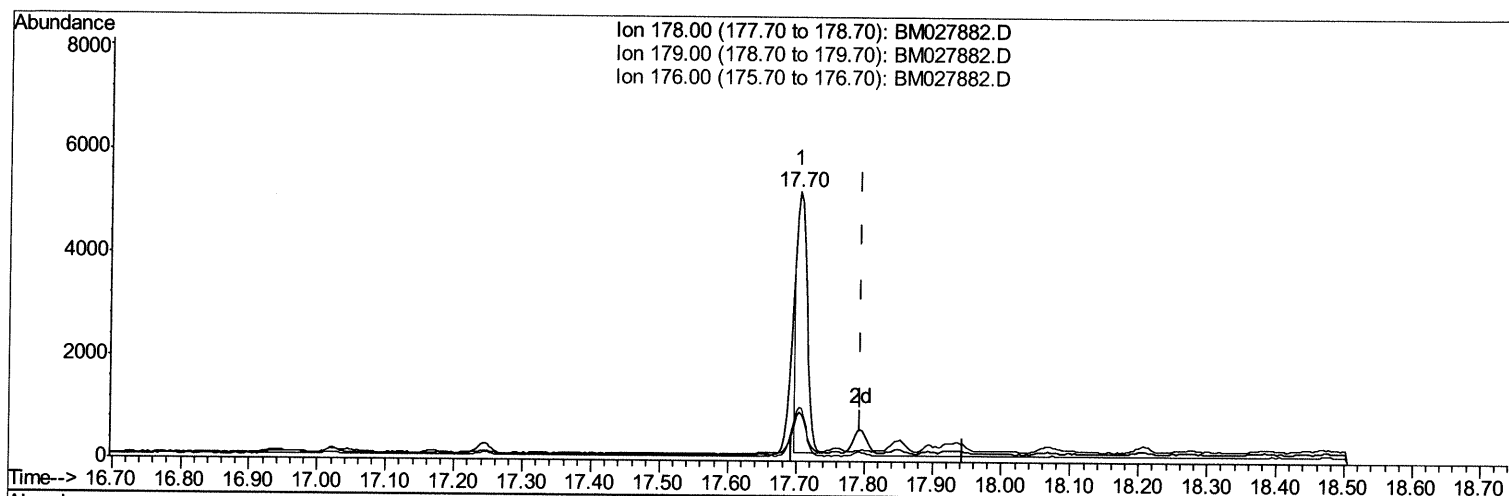

TIC: BM027882.D

(13) Anthracene

17.704min (-0.090) 0.29ng/ul

response 5213

Ion	Exp%	Act%
178.00	100	100
179.00	16.80	18.08
176.00	18.80	20.05
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112020\
 Data File : BM027882.D
 Acq On : 21 Nov 2020 15:34
 Operator : JU/CG
 Sample : L4854-06DL 5X
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 C0AD4DL

Manual Integrations
APPROVED

mohammad
 11/24/2020 8:58:44 AM

Quant Time: Nov 23 03:00:19 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM112020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 23 02:58:43 2020
 Response via : Initial Calibration

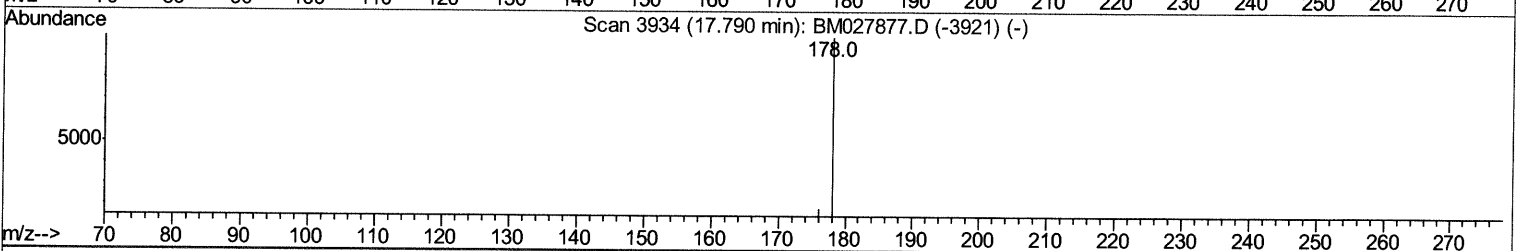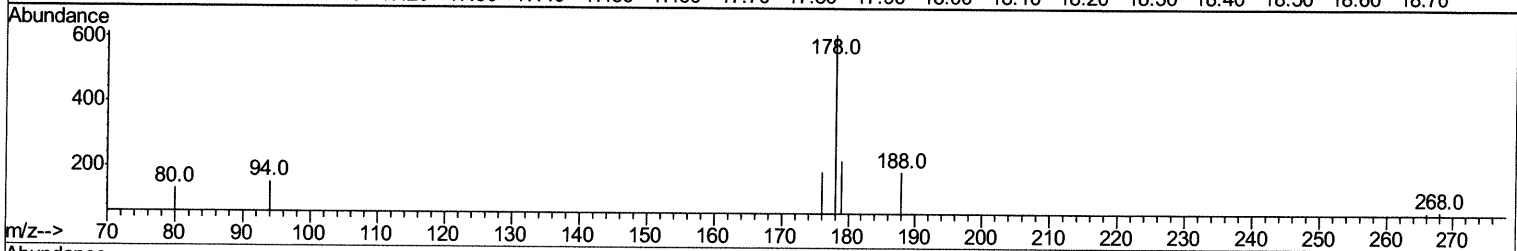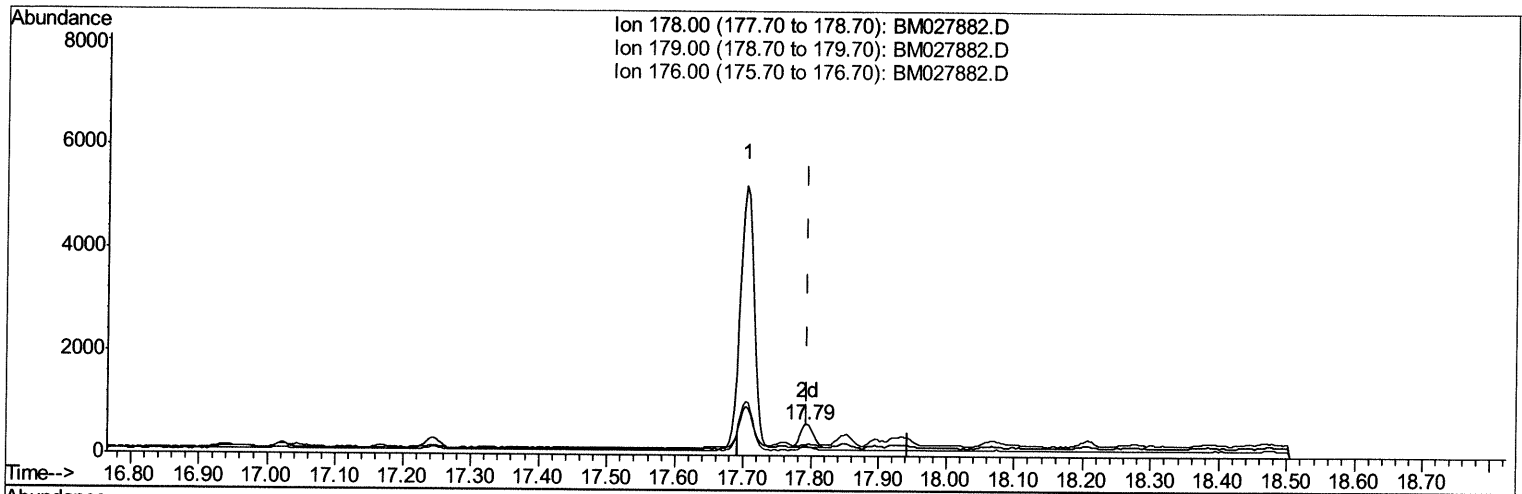

TIC: BM027882.D

(13) Anthracene

17.794min (-0.000) 0.03ng/ul m

11/27/2020

response 611

Ion	Exp%	Act%
178.00	100	100
179.00	16.80	36.50#
176.00	18.80	30.77#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112020\
Data File : BM027882.D
Acq On : 21 Nov 2020 15:34
Operator : JU/CG
Sample : L4854-06DL 5X
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD4DL

Manual Integrations
APPROVED

mohammad
11/24/2020 8:58:44 AM

Quant Time: Nov 23 03:00:19 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM112020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 23 02:58:43 2020
Response via : Initial Calibration

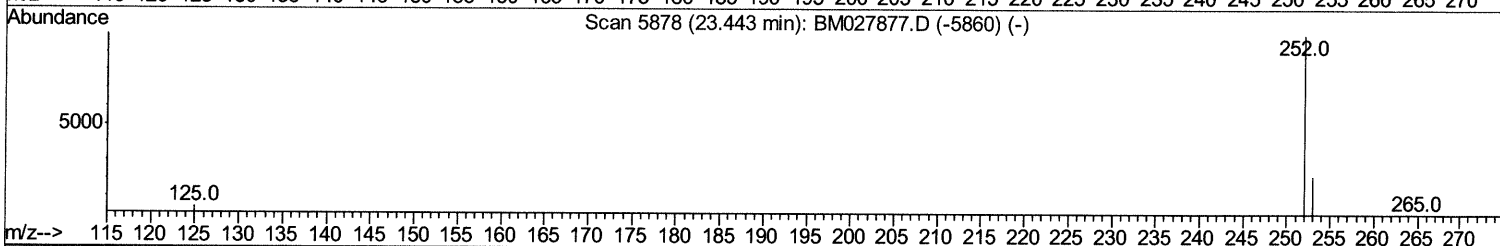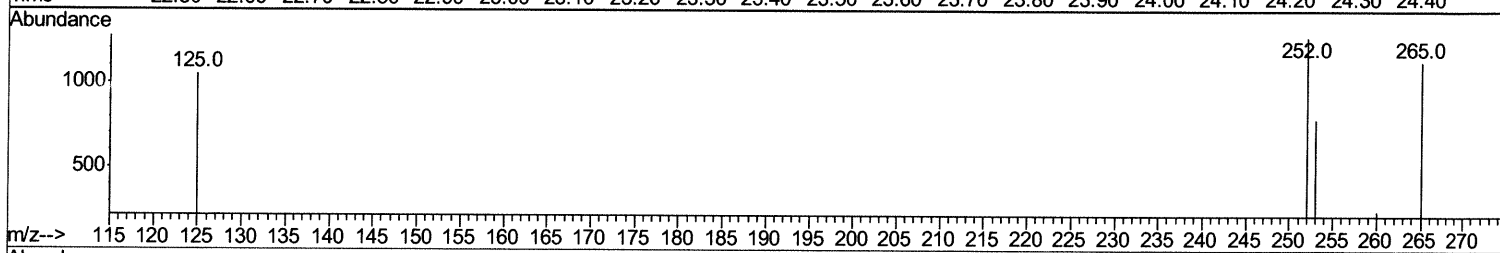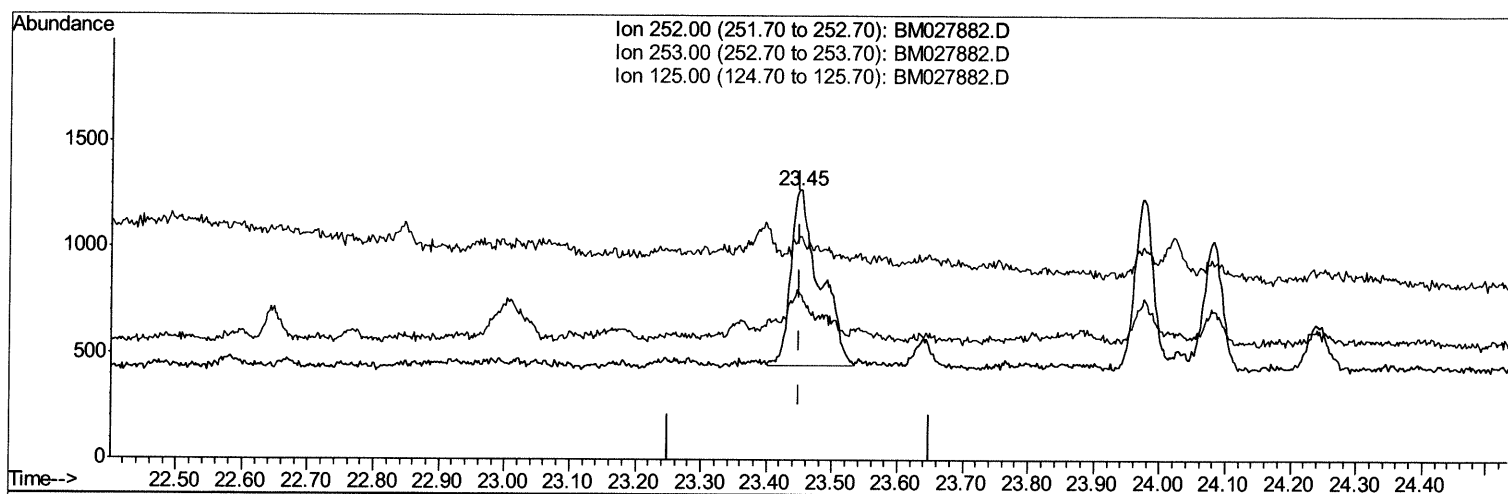

TIC: BM027882.D

(21) Benzo(b)fluoranthene
23.450min (-0.000) 0.17ng/ul
response 2563

Ion	Exp%	Act%
252.00	100	100
253.00	29.80	61.77#
125.00	14.20	82.65#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112020\
Data File : BM027882.D
Acq On : 21 Nov 2020 15:34
Operator : JU/CG
Sample : L4854-06DL 5X
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleID :
C0AD4DL

Manual Integrations
APPROVED

mohammad
11/24/2020 8:58:44 AM

Quant Time: Nov 23 03:00:19 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM112020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 23 02:58:43 2020
Response via : Initial Calibration

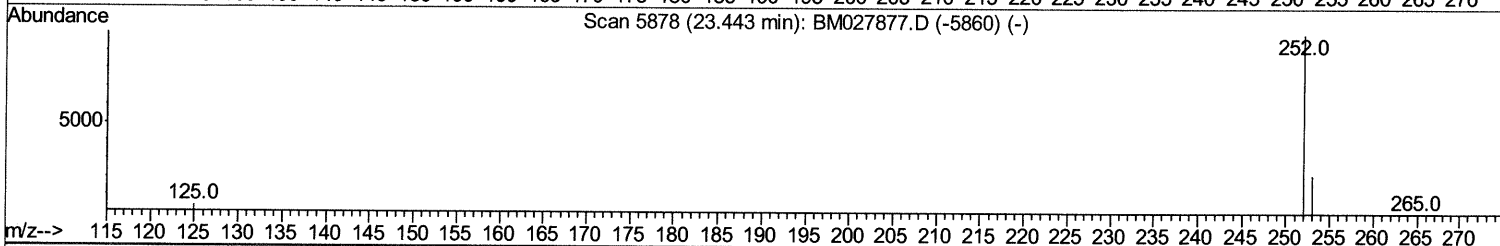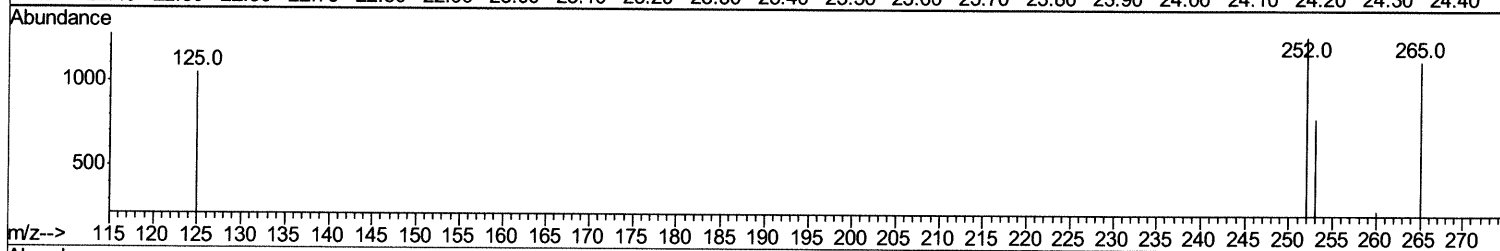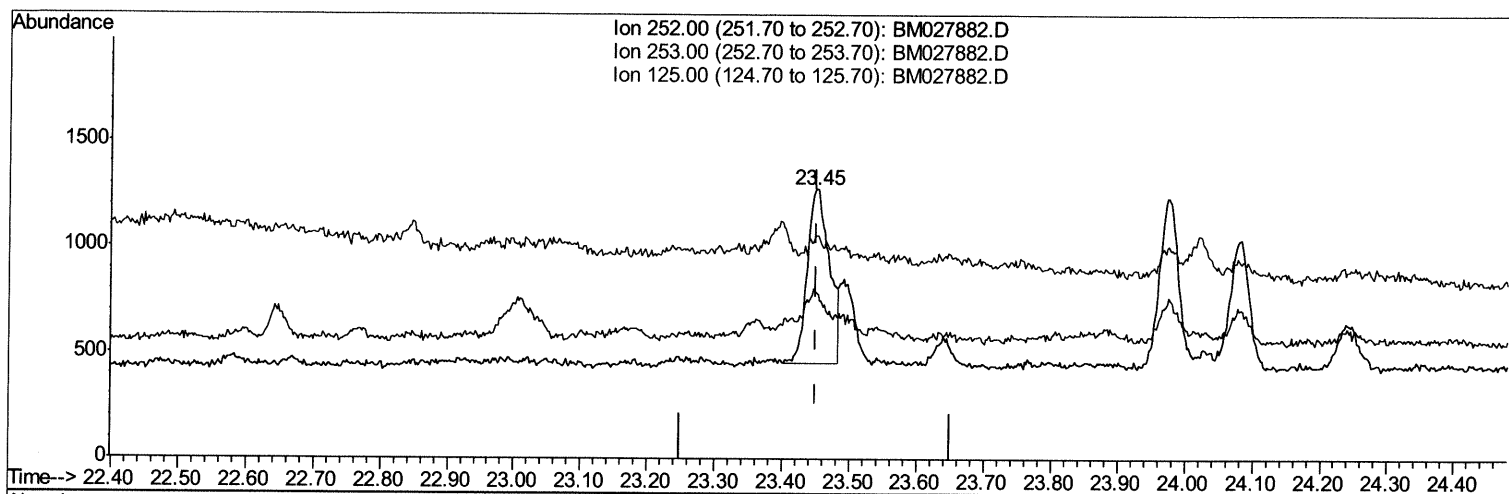

TIC: BM027882.D

(21) Benzo(b)fluoranthene

23.450min (-0.000) 0.12ng/ul m

11/21/20 JU

response 1896

Ion	Exp%	Act%
252.00	100	100
253.00	29.80	61.77#
125.00	14.20	82.65#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112020\
Data File : BM027882.D
Acq On : 21 Nov 2020 15:34
Operator : JU/CG
Sample : L4854-06DL 5X
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD4DL

Manual Integrations
APPROVED

mohammad
11/24/2020 8:58:44 AM

Quant Time: Nov 23 04:00:30 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM112020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 23 02:58:43 2020
Response via : Initial Calibration

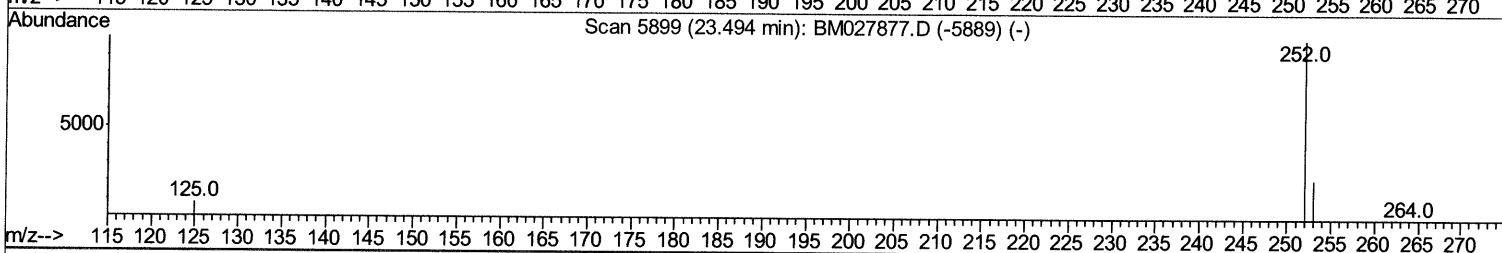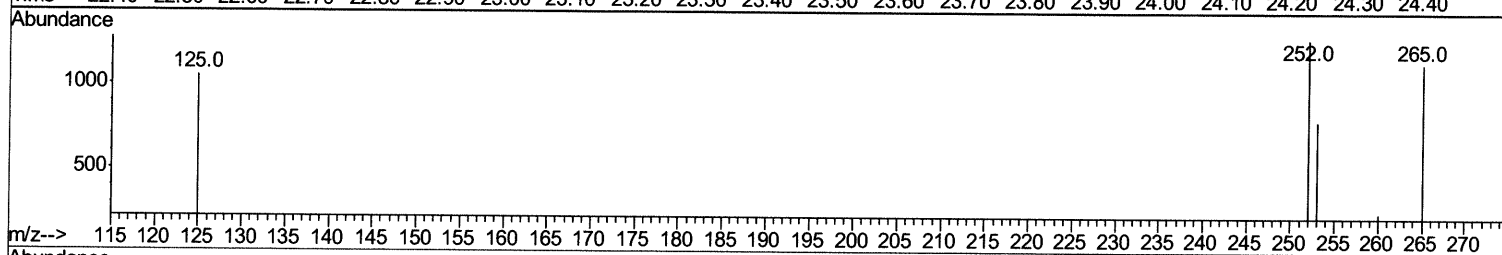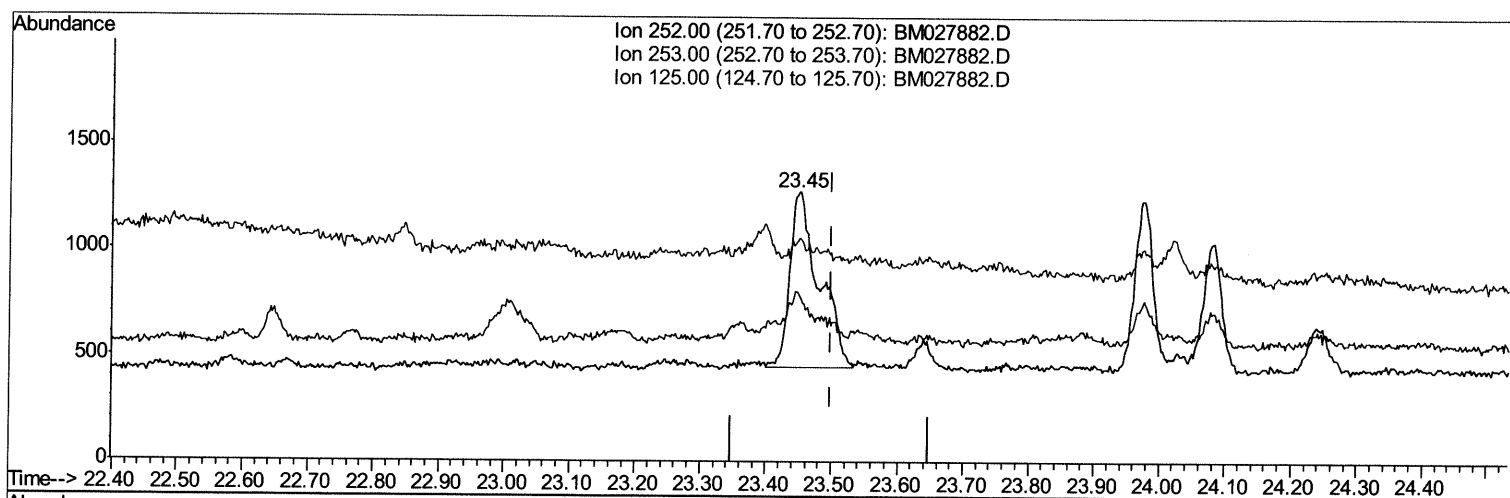

TIC: BM027882.D

(22) Benzo(k)fluoranthene

23.450min (-0.049) 0.17ng/ul

response 2565

Ion	Exp%	Act%
252.00	100	100
253.00	29.00	61.77#
125.00	14.70	82.65#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112020\
 Data File : BM027882.D
 Acq On : 21 Nov 2020 15:34
 Operator : JU/CG
 Sample : L4854-06DL 5X
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AD4DL

Manual Integrations
 APPROVED

mohammad
 11/24/2020 8:58:44 AM

Quant Time: Nov 23 04:00:30 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM112020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 23 02:58:43 2020
 Response via : Initial Calibration

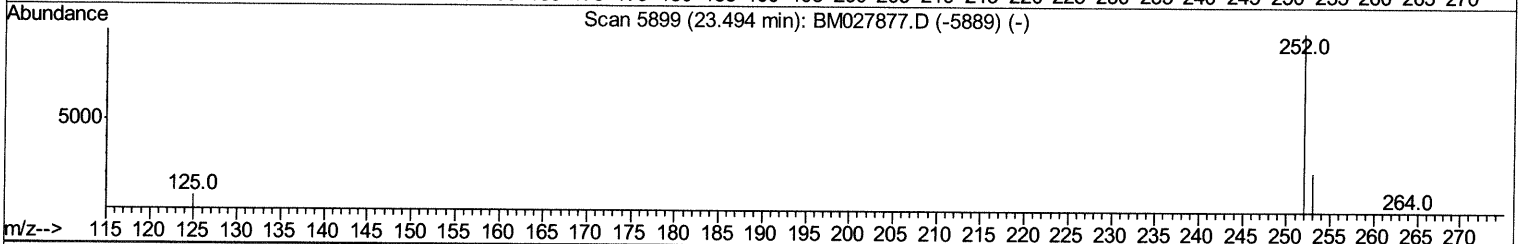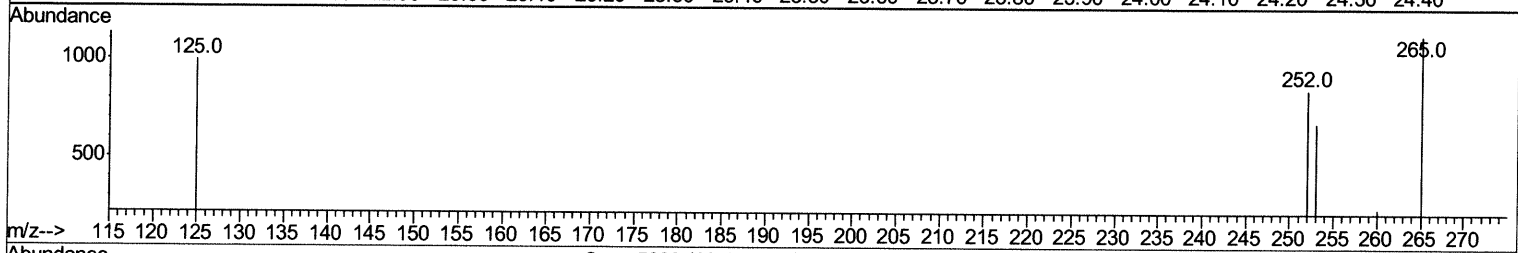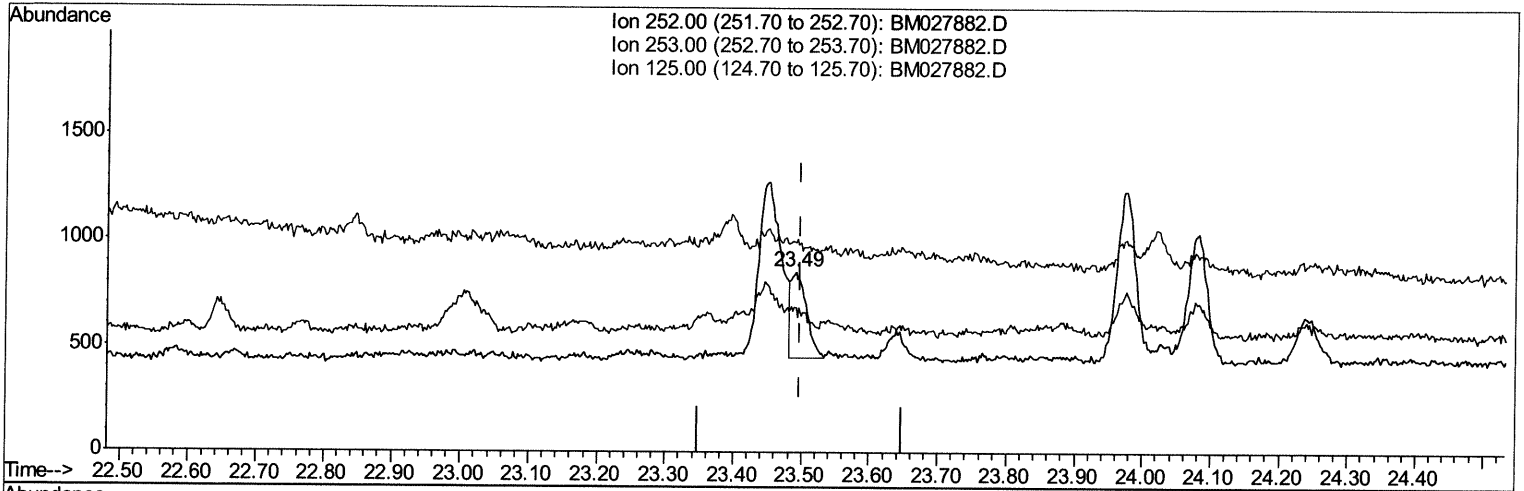

TIC: BM027882.D

(22) Benzo(k)fluoranthene

23.491min (-0.007) 0.04ng/ul m 11/27/20 JV

response 637

Ion	Exp%	Act%
252.00	100	100
253.00	29.00	79.93#
125.00	14.70	116.55#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM112020\
 Data File : BM027882.D
 Acq On : 21 Nov 2020 15:34
 Operator : JU/CG
 Sample : L4854-06DL 5X
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AD4DL

Manual Integrations
 APPROVED

mohammad
 11/24/2020 8:58:44 AM

Quant Time: Nov 23 04:01:46 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM112020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 23 02:58:43 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.33	152	1114	0.40	ng/ul	0.00
2) Naphthalene-d8	11.17	136	4520	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.95	164	2859	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.66	188	5876	0.40	ng/ul	0.00
16) Chrysene-d12	21.77	240	4062	0.40	ng/ul	0.00
20) Perylene-d12	24.19	264	3617	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.73	152	206	0.03	ng/ul	0.00
14) Fluoranthene-d10	19.65	212	434	0.03	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
3) Naphthalene	11.22	128	2984	0.220	ng/ul	98
5) 2-Methylnaphthalene	12.80	142	5618	0.610	ng/ul	99
8) Acenaphthene	15.02	153	255	0.024	ng/ul#	66
9) Fluorene	15.98	166	352	0.029	ng/ul#	80
12) Phenanthrene	17.70	178	7133	0.384	ng/ul	99
13) Anthracene	17.79	178	611m >	0.034	ng/ul >	11/27/2024
15) Fluoranthene	19.68	202	3224	0.157	ng/ul	93
17) Pyrene	20.04	202	3983	0.193	ng/ul#	92
18) Benzo(a)anthracene	21.75	228	1521	0.093	ng/ul#	41
19) Chrysene	21.80	228	2389	0.150	ng/ul#	55
21) Benzo(b)fluoranthene	23.45	252	1896m 3	0.125	ng/ul 3	11/27/2024
22) Benzo(k)fluoranthene	23.49	252	637m 3	0.043	ng/ul 3	
23) Benzo(a)pyrene	24.08	252	1228	0.092	ng/ul#	1
24) Indeno(1,2,3-cd)pyrene	26.68	276	798	0.055	ng/ul#	66
25) Dibenzo(a,h)anthracene	26.69	278	265	0.022	ng/ul#	1
26) Benzo(a,h,i)perylene	27.45	276	1190	0.099	ng/ul#	50

(#) = qualifier out of range (m) = manual integration (+) = signals summed